
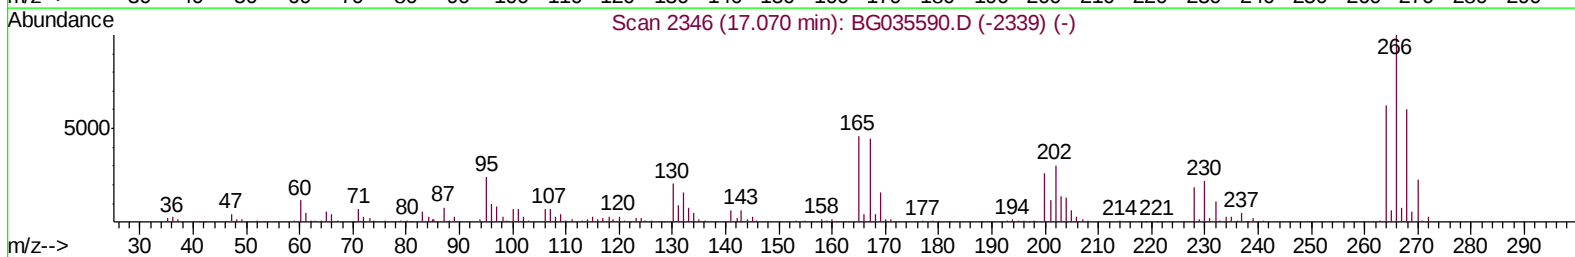
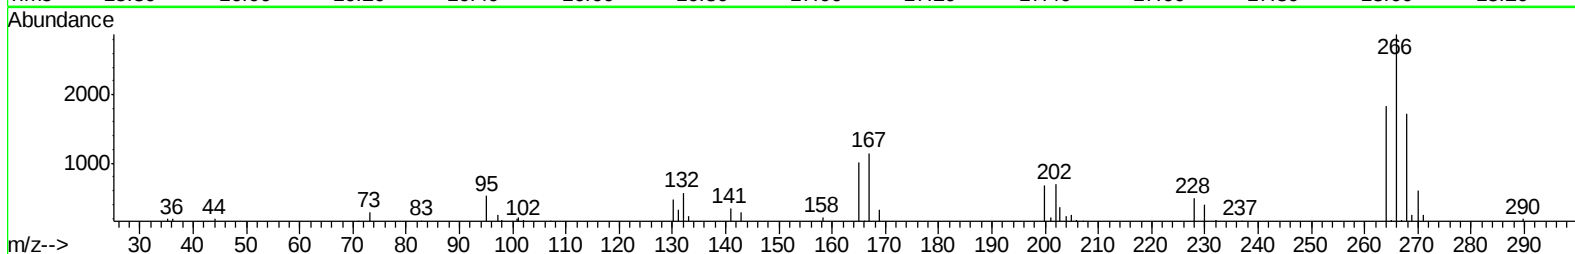


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073018\
Data File : BG035986.D
Acq On : 30 Jul 2018 22:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 01:56:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

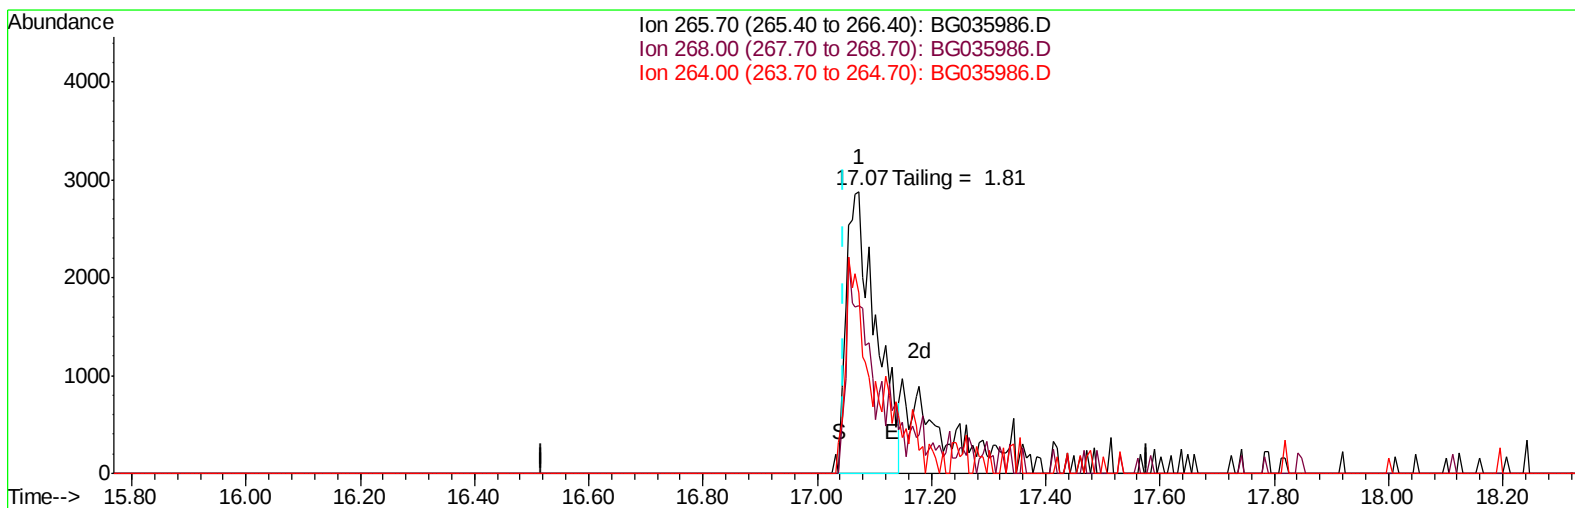

TIC: BG035986.D

(69) Pentachlorophenol (C)




17.073min (+0.025) 5996.16ng

response 10167

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.51
264.00	62.00	63.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073018\
 Data File : BG035986.D
 Acq On : 30 Jul 2018 22:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 01:56:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 31 12:30:06 2018
 Response via : Initial Calibration

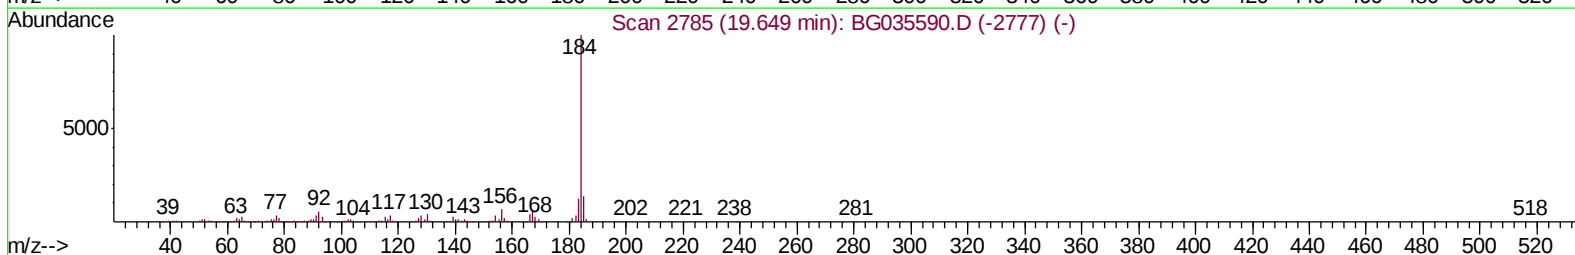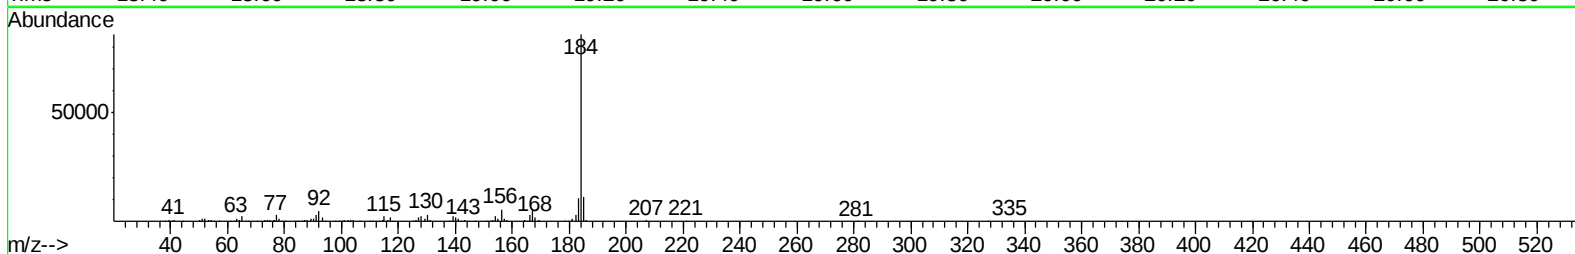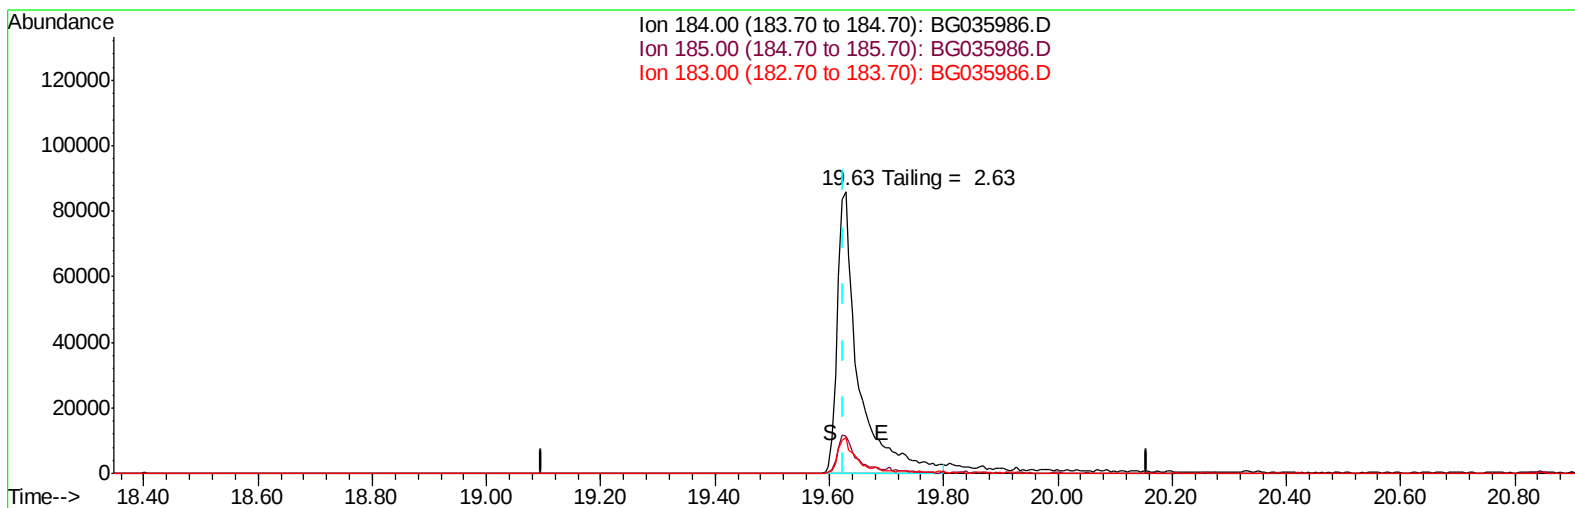

TIC: BG035986.D

(76) Benzidine

19.628min (+0.002) 155365.27ng

response 220568

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.41
183.00	13.30	12.83
0.00	0.00	0.00