

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073018\
 Data File : BG035989.D
 Acq On : 31 Jul 2018 00:45
 Operator : JU/SJ
 Sample : J4187-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DSN-001A-072618

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.132	308	314	323	rBV	30787	54223	1.52%	0.341%
2	5.537	377	383	389	rBV	82519	133083	3.72%	0.836%
3	5.602	389	394	400	rVV	280100	468124	13.08%	2.942%
4	5.666	400	405	417	rVB	253116	548333	15.32%	3.447%
5	6.036	461	468	472	rBV	134332	228259	6.38%	1.435%
6	7.188	657	664	679	rBV	188346	379610	10.61%	2.386%
7	7.558	717	727	739	rBV	534964	962773	26.91%	6.051%
8	8.022	800	806	813	rBV2	106981	183962	5.14%	1.156%
9	8.345	852	861	870	rBV	497796	862777	24.11%	5.423%
10	9.185	996	1004	1017	rBV	408814	757838	21.18%	4.763%
11	10.824	1272	1283	1289	rBV	142151	273697	7.65%	1.720%
12	10.877	1289	1292	1299	rVB	27928	46214	1.29%	0.290%
13	11.482	1387	1395	1405	rBV3	22715	52580	1.47%	0.330%
14	11.664	1419	1426	1433	rBV2	25732	64159	1.79%	0.403%
15	13.268	1691	1699	1709	rBV	1304260	2006012	56.06%	12.609%
16	14.096	1832	1840	1847	rBV	37275	73645	2.06%	0.463%
17	14.642	1927	1933	1941	rBV2	263271	440715	12.32%	2.770%
18	16.134	2175	2187	2201	rBV	1152177	1889569	52.81%	11.877%
19	17.392	2395	2401	2405	rBV	402601	612949	17.13%	3.853%
20	17.433	2405	2408	2416	rVB	55631	81094	2.27%	0.510%
21	18.273	2547	2551	2555	rBV3	28010	42722	1.19%	0.269%
22	20.000	2838	2845	2854	rBV	2596752	3578110	100.00%	22.490%
23	21.651	3120	3126	3133	rBV2	406669	685188	19.15%	4.307%
24	23.119	3369	3376	3383	rBV10	16989	42716	1.19%	0.268%
25	23.307	3401	3408	3416	rVB	343565	644835	18.02%	4.053%
26	23.912	3505	3511	3517	rBV10	21951	48080	1.34%	0.302%
27	24.846	3660	3670	3686	rVB2	242921	699886	19.56%	4.399%
28	25.951	3852	3858	3868	rVB9	15050	48607	1.36%	0.306%


Sum of corrected areas: 15909760

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073018\
Data File : BG035989.D
Acq On : 31 Jul 2018 00:45
Operator : JU/SJ
Sample : J4187-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DSN-001A-072618

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

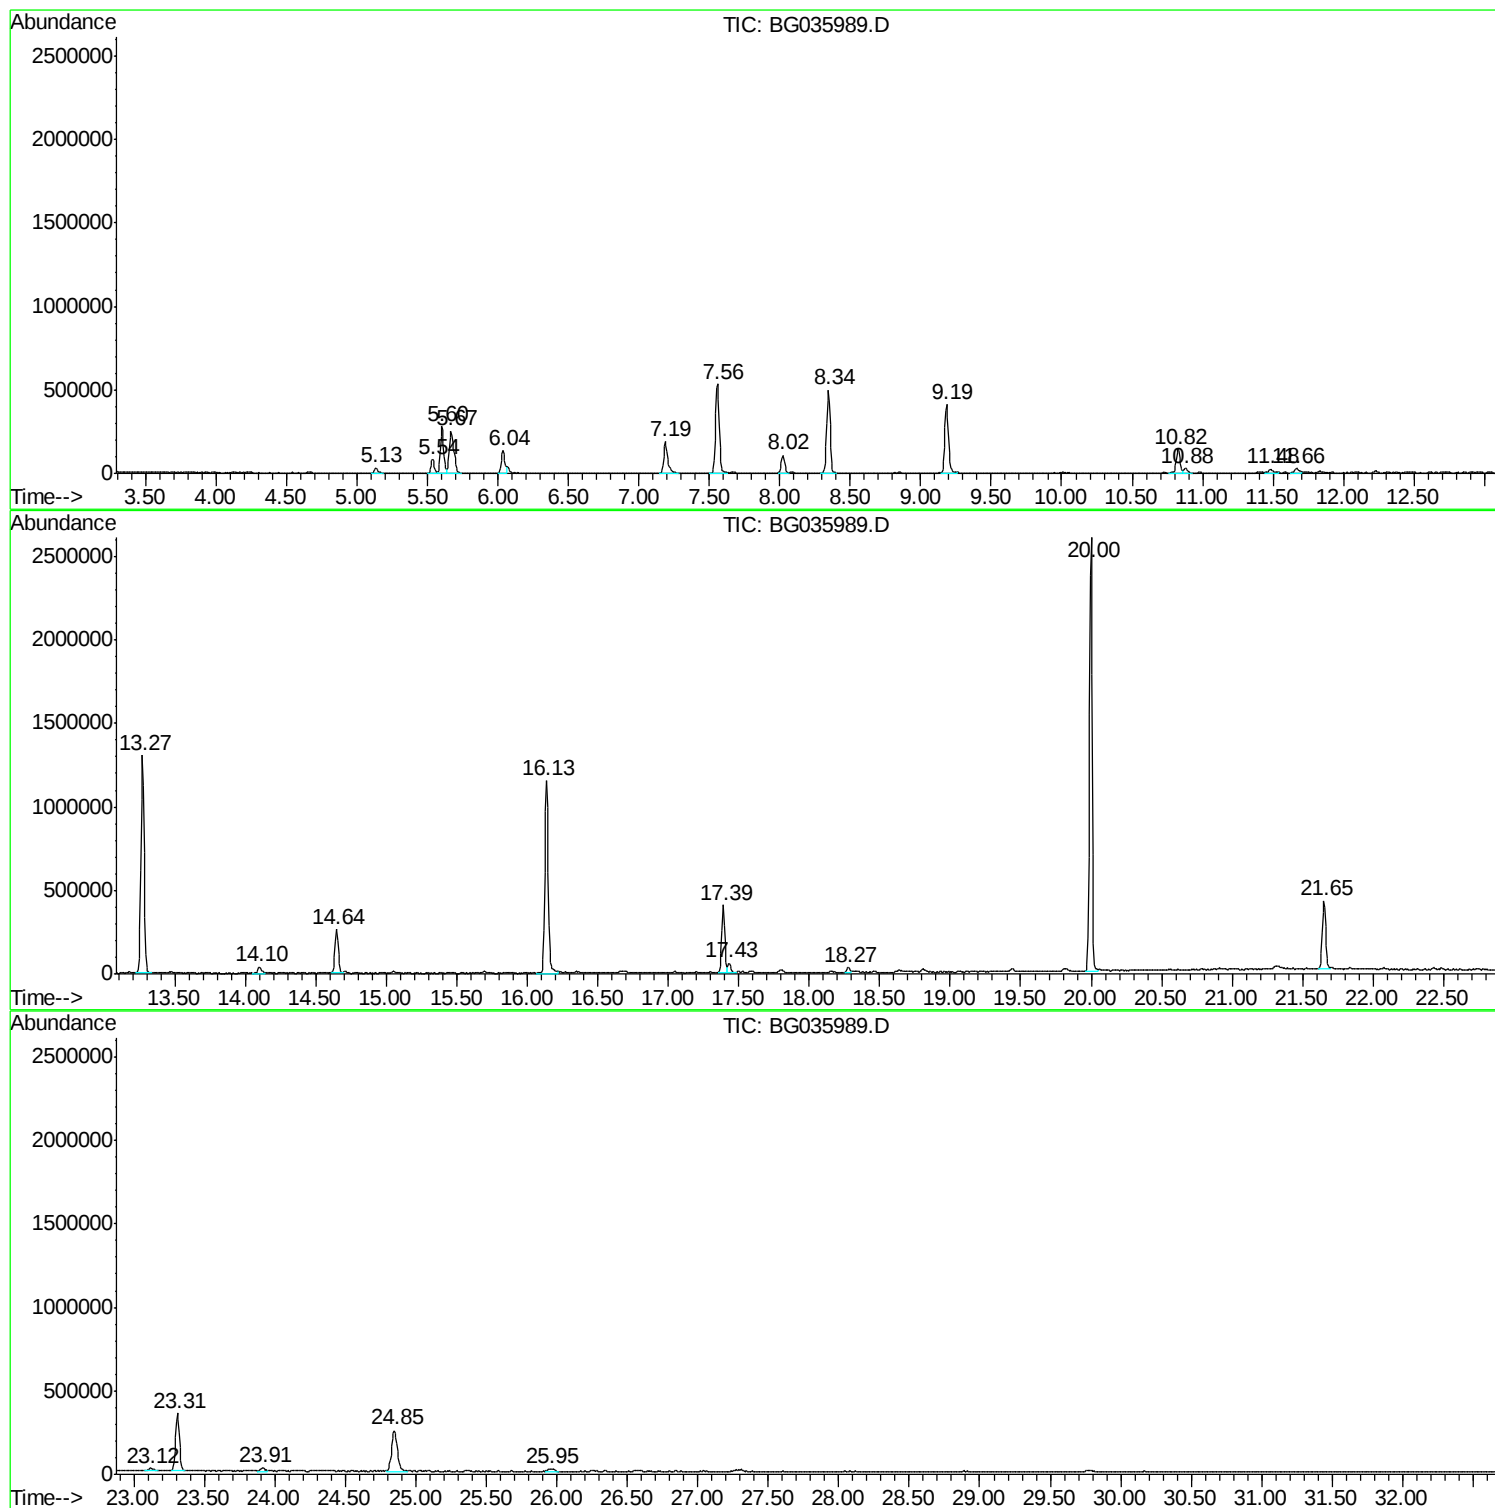

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073018\
Data File : BG035989.D
Acq On : 31 Jul 2018 00:45
Operator : JU/SJ
Sample : J4187-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DSN-001A-072618

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073018\
Data File : BG035989.D
Acq On : 31 Jul 2018 00:45
Operator : JU/SJ
Sample : J4187-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DSN-001A-072618

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc