
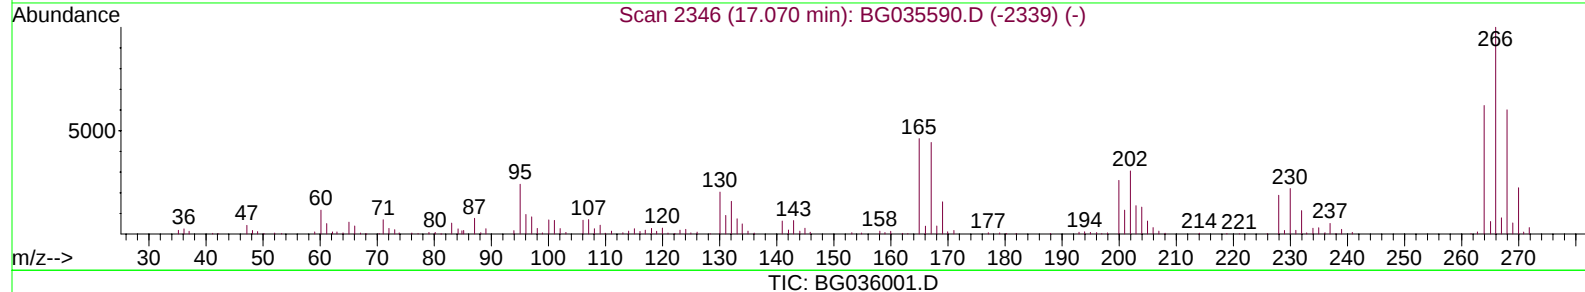
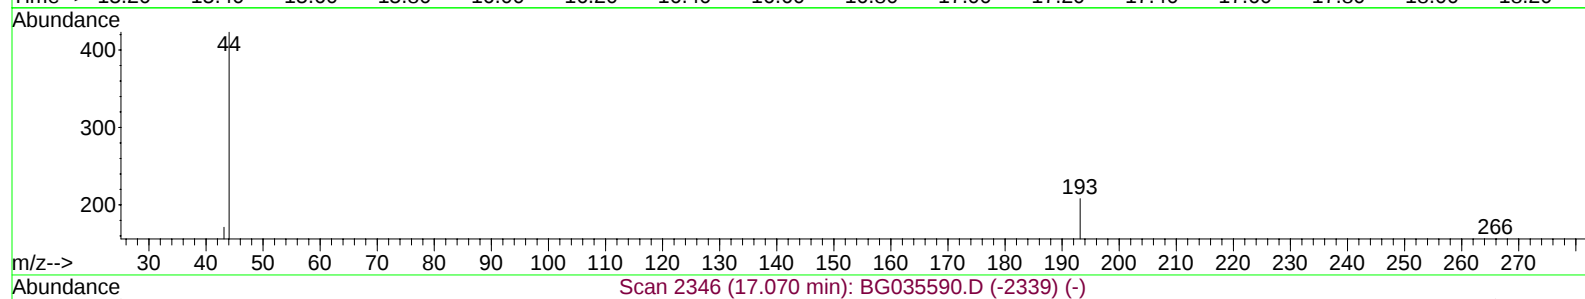


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073118\
Data File : BG036001.D
Acq On : 31 Jul 2018 14:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 18:34:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

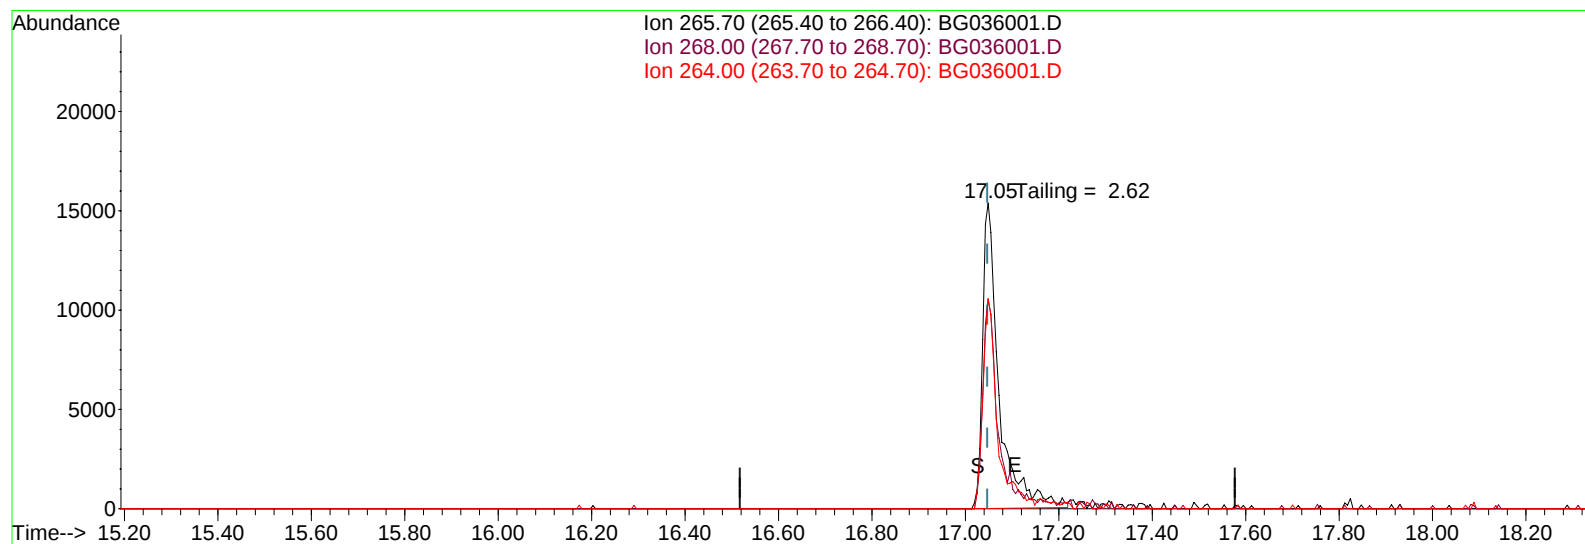

(69) Pentachlorophenol (C)




16.203min (-0.845) 132.59ng

response 55

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	0.00#
264.00	62.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073118\
Data File : BG036001.D
Acq On : 31 Jul 2018 14:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 18:34:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

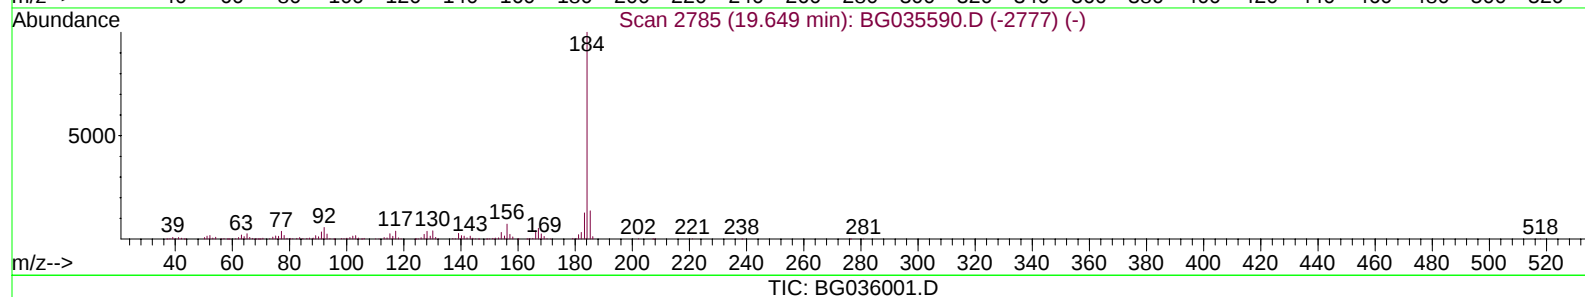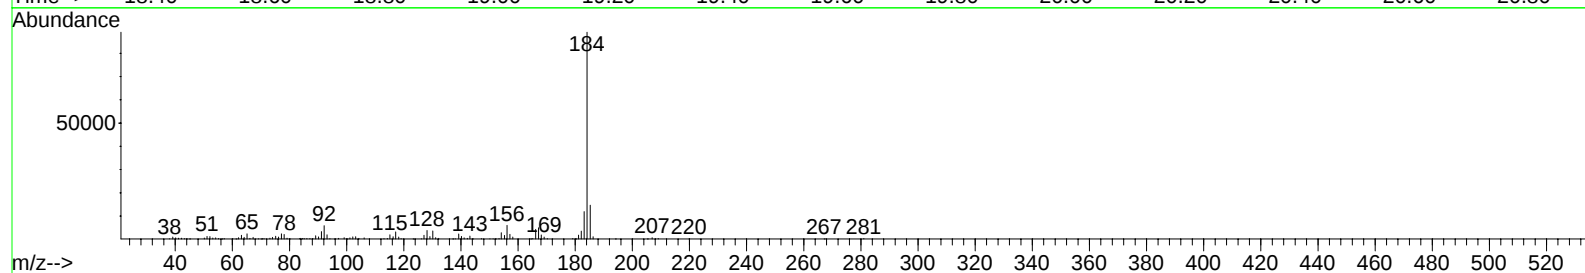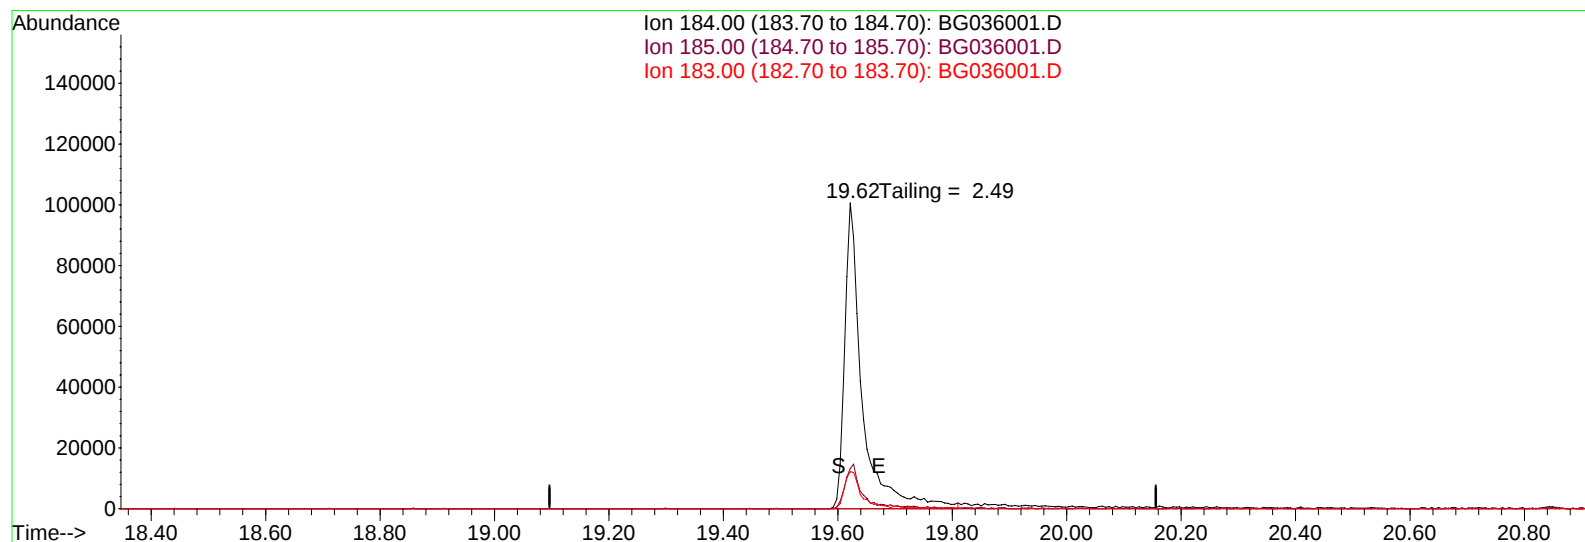

(76) Benzidine

19.626min (-19.626) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00