
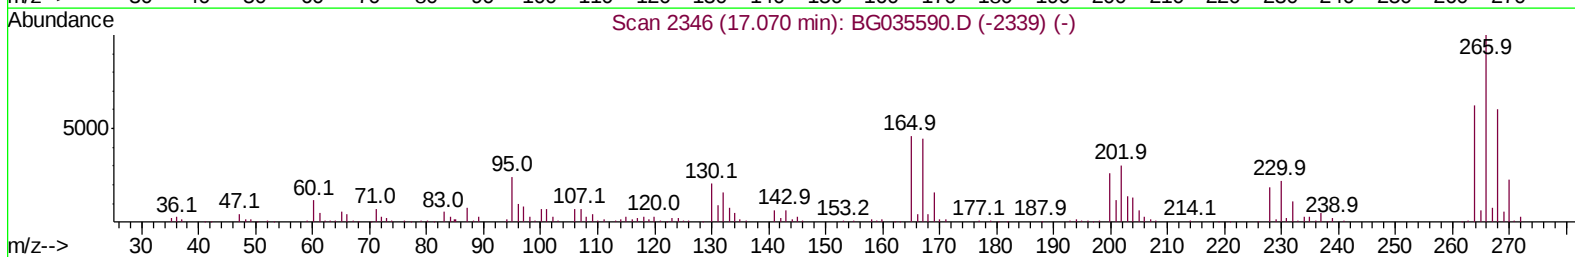
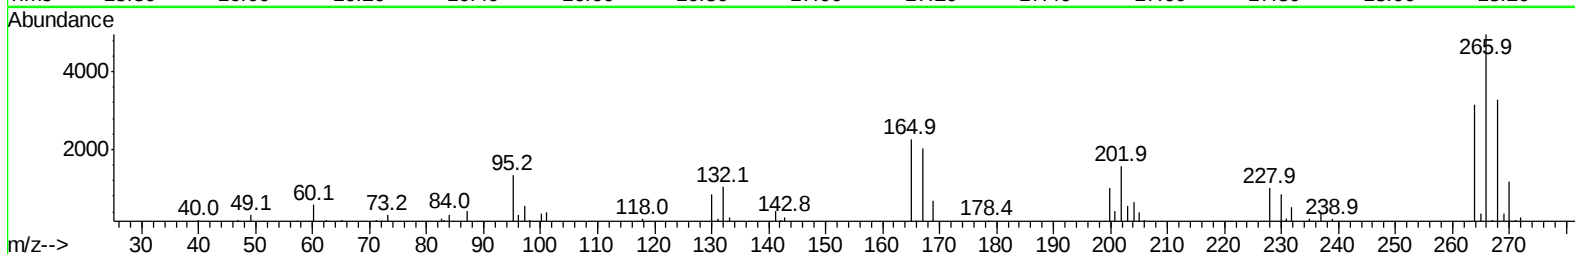


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073118\
Data File : BG036020.D
Acq On : 1 Aug 2018 3:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 07:56:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

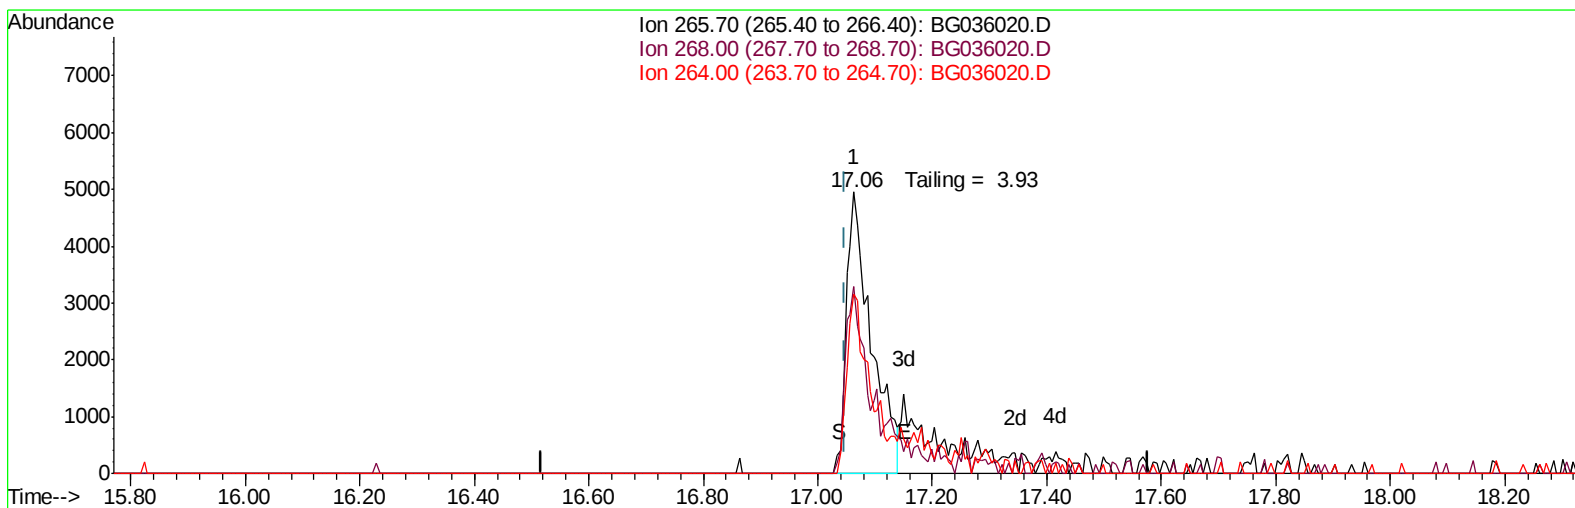

TIC: BG036020.D

(69) Pentachlorophenol (C)




17.063min (+0.015) 30031.41ng

response 14861

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.20
264.00	62.00	63.45
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG073118\
Data File : BG036020.D
Acq On : 1 Aug 2018 3:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 07:56:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

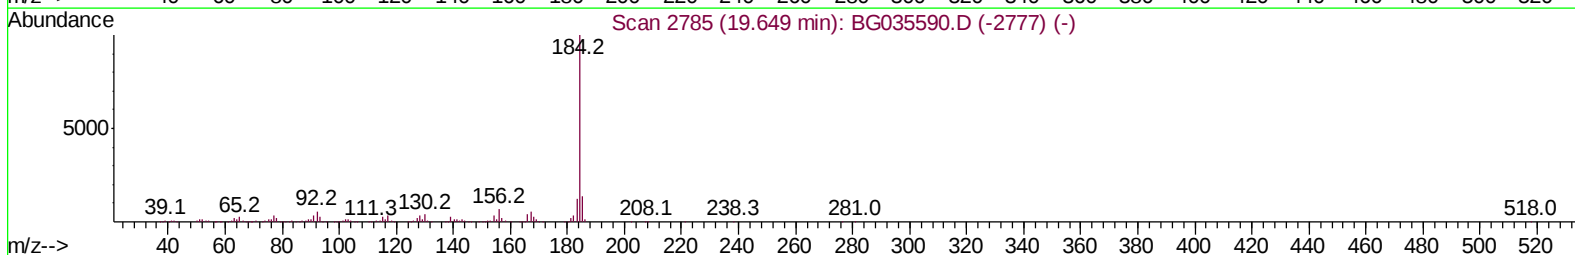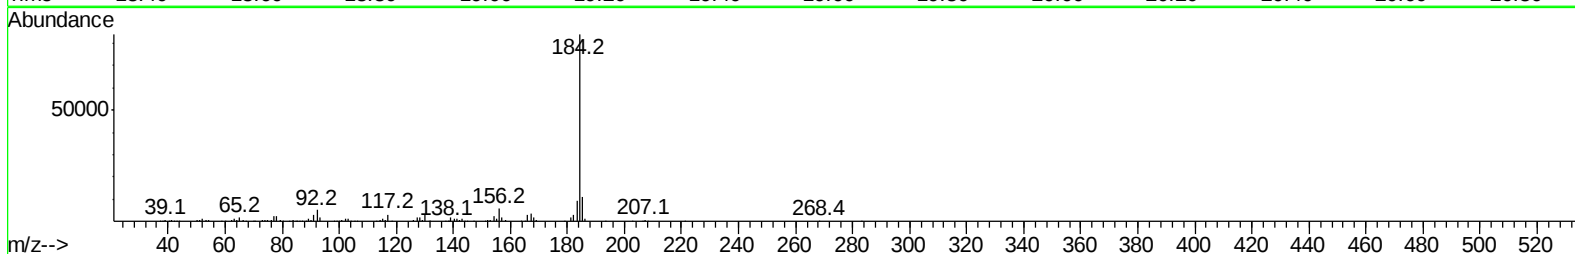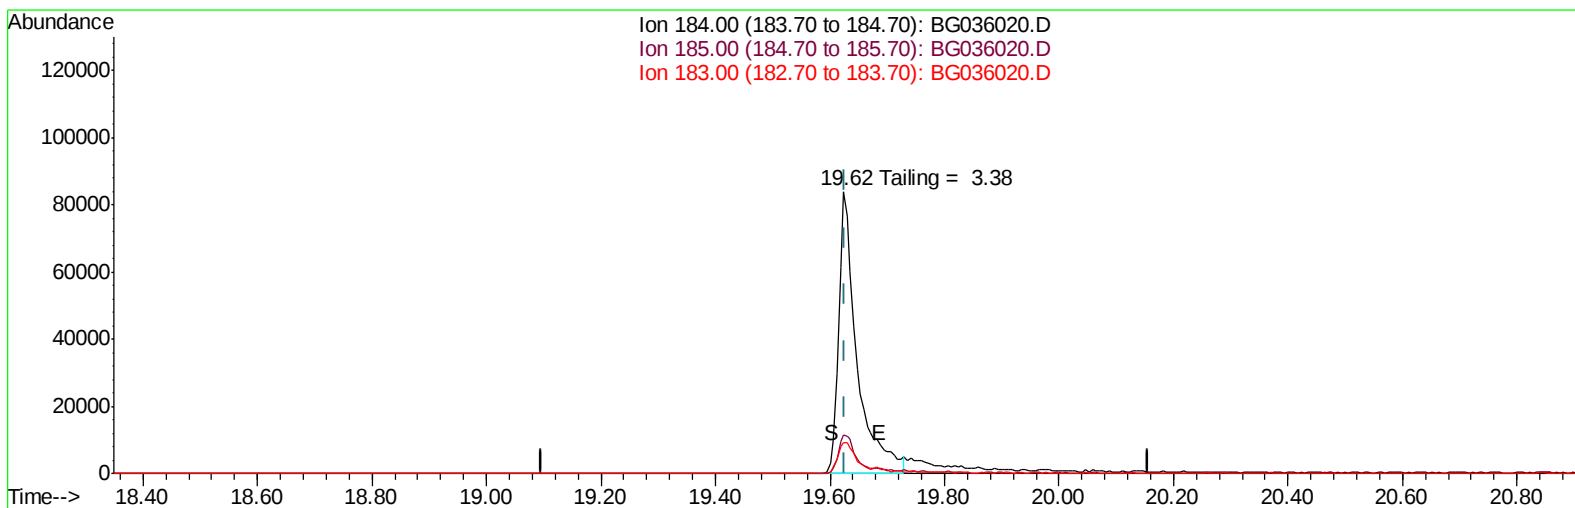

TIC: BG036020.D

(76) Benzidine

19.624min (-0.002) 60842.79ng

response 187150

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.45
183.00	13.30	11.00
0.00	0.00	0.00