


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073118\
 Data File : BG036020.D
 Acq On : 1 Aug 2018 3:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

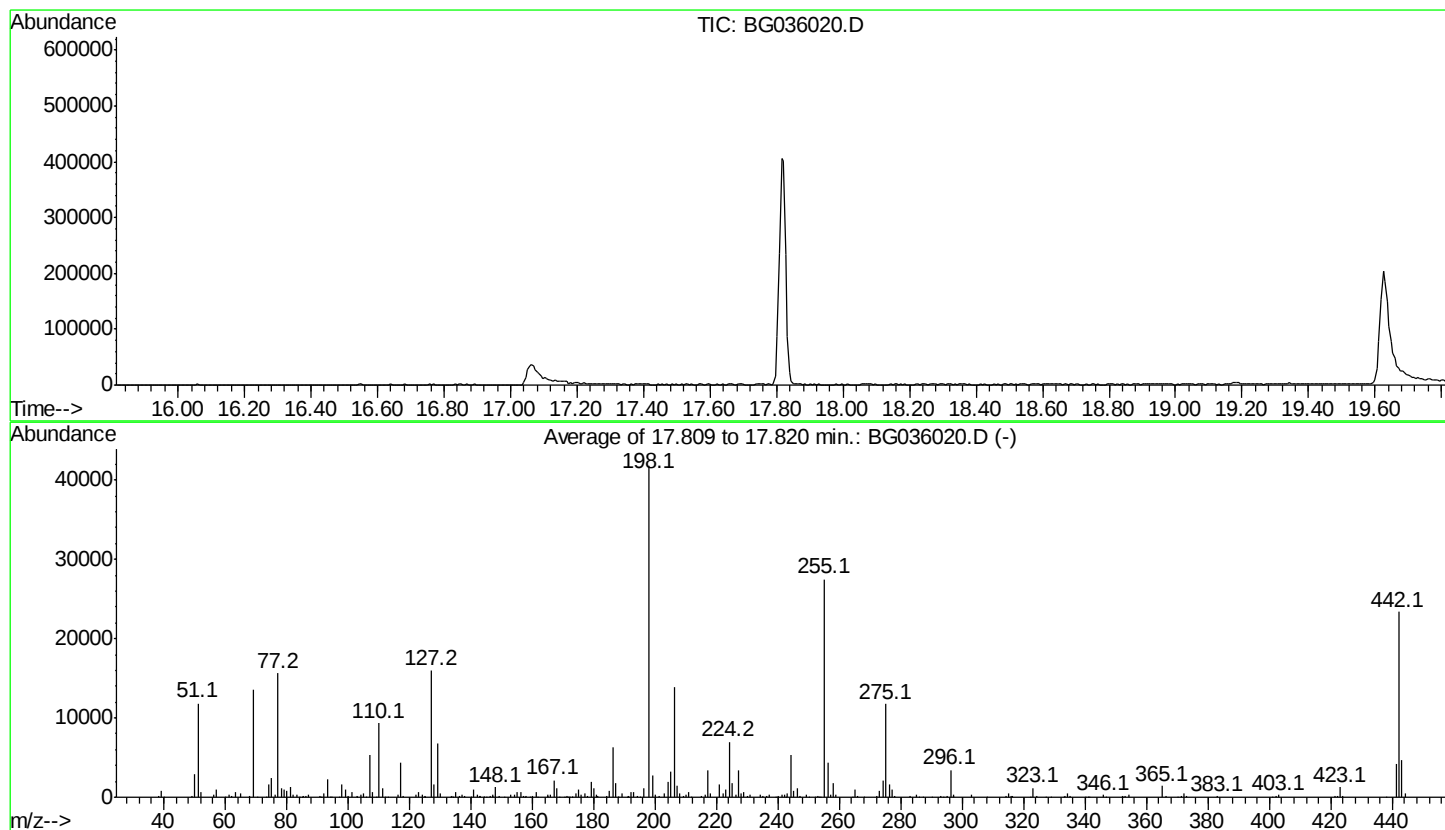

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	11814	PASS
68	69	0.00	2	0.7	91	PASS
69	198	0.00	100	32.6	13645	PASS
70	69	0.00	2	0.5	69	PASS
127	198	10	80	38.1	15941	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41821	PASS
199	198	5	9	6.6	2759	PASS
275	198	10	60	28.0	11716	PASS
365	198	1	100	3.5	1444	PASS
441	198	0.01	100	9.9	4157	PASS
442	198	50	100	55.9	23371	PASS
443	442	15	24	20.0	4682	PASS