


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073118\  
 Data File : BG036020.D  
 Acq On : 1 Aug 2018 3:14  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG071218.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jul 31 12:30:06 2018

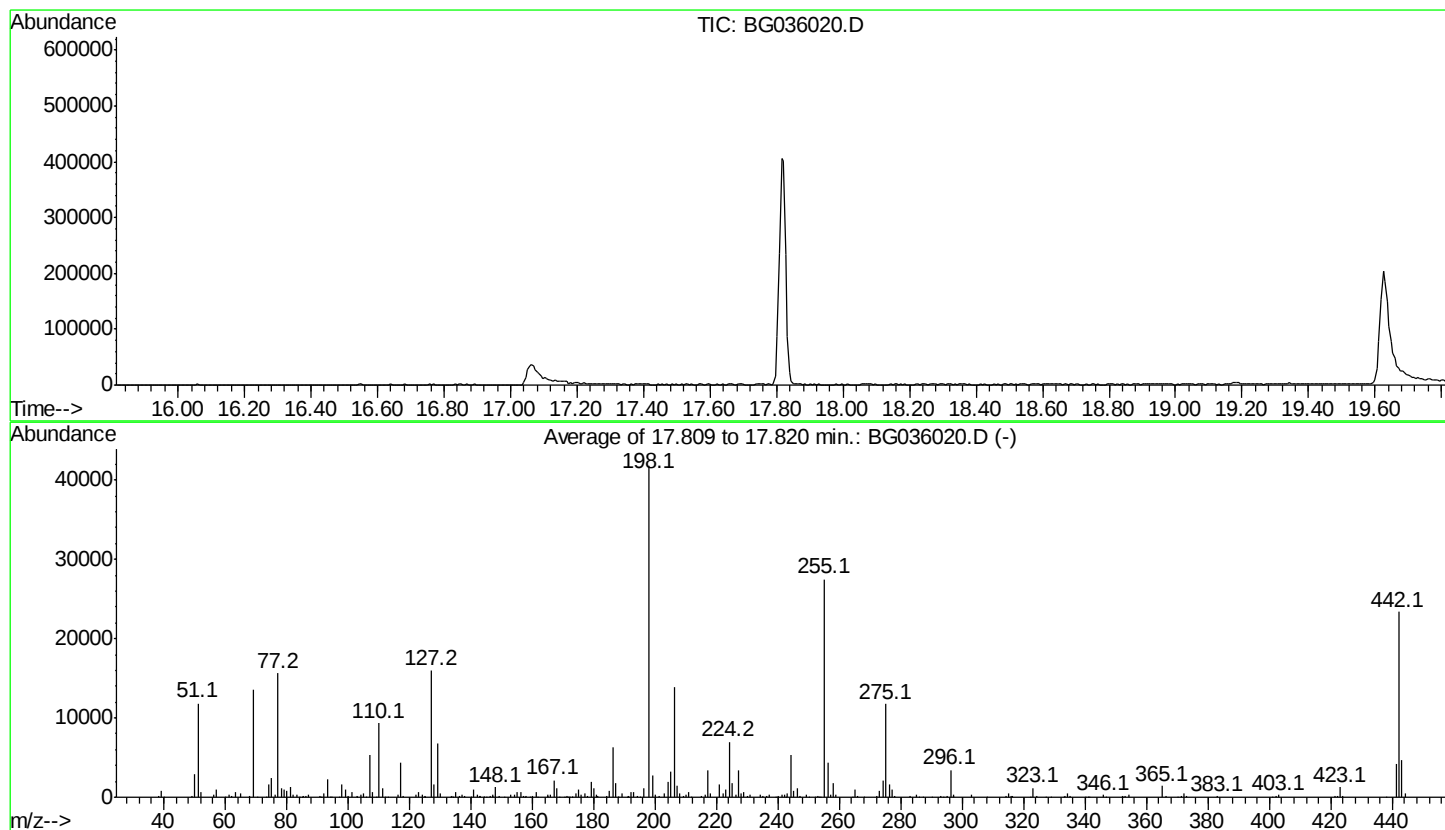

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 28.2      | 11814   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.7       | 91      | PASS             |
| 69          | 198          | 0.00         | 100          | 32.6      | 13645   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 69      | PASS             |
| 127         | 198          | 10           | 80           | 38.1      | 15941   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 41821   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 2759    | PASS             |
| 275         | 198          | 10           | 60           | 28.0      | 11716   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 1444    | PASS             |
| 441         | 443          | 0.01         | 100          | 88.8      | 4157    | PASS             |
| 442         | 198          | 50           | 100          | 55.9      | 23371   | PASS             |
| 443         | 442          | 15           | 24           | 20.0      | 4682    | PASS             |