
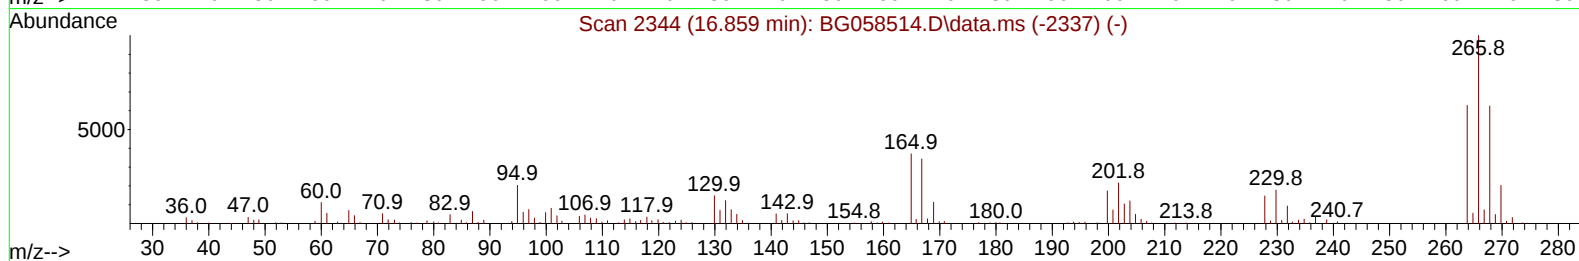
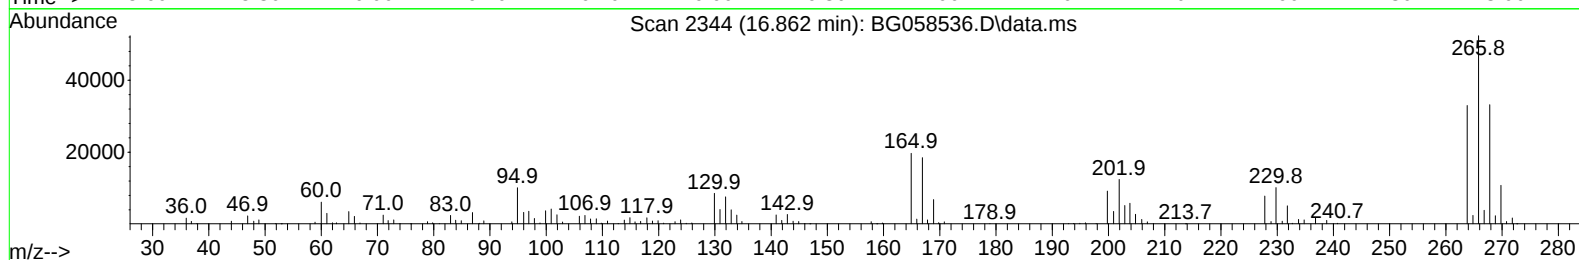


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073123\
Data File : BG058536.D
Acq On : 31 Jul 2023 9:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 12:17:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

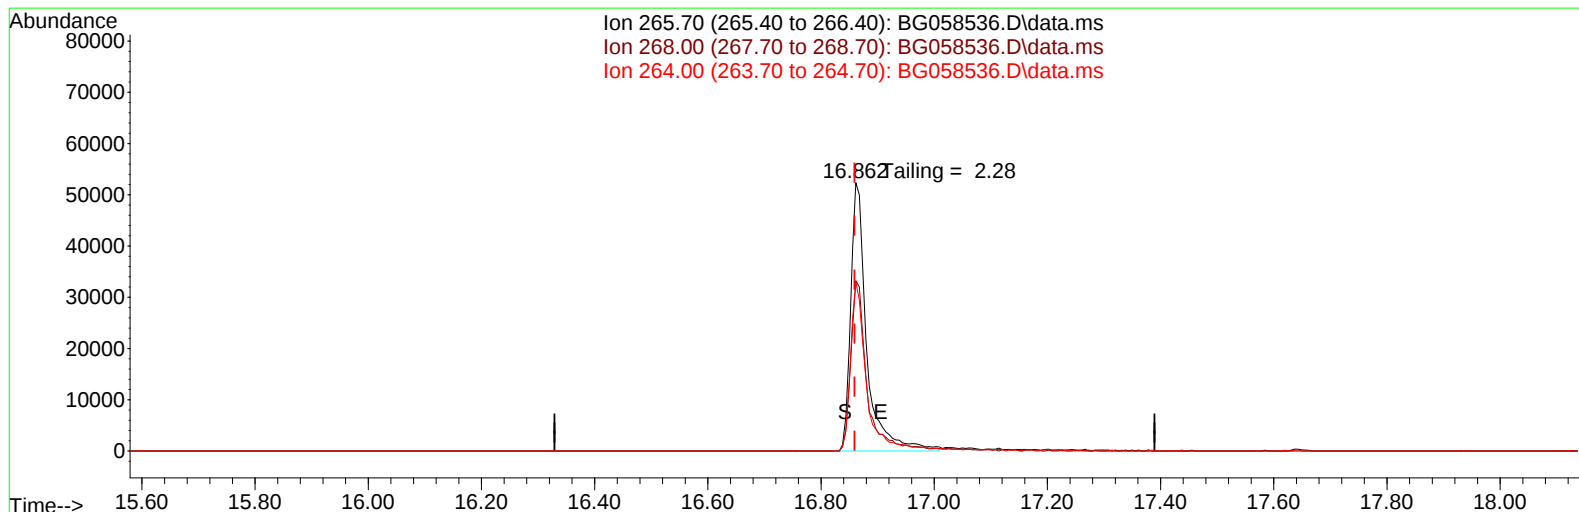

TIC: BG058536.D\data.ms

(70) Pentachlorophenol (C)




16.862min (+ 0.003) 31611.60 ng

response 103944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.46
264.00	62.80	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073123\
Data File : BG058536.D
Acq On : 31 Jul 2023 9:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 12:17:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

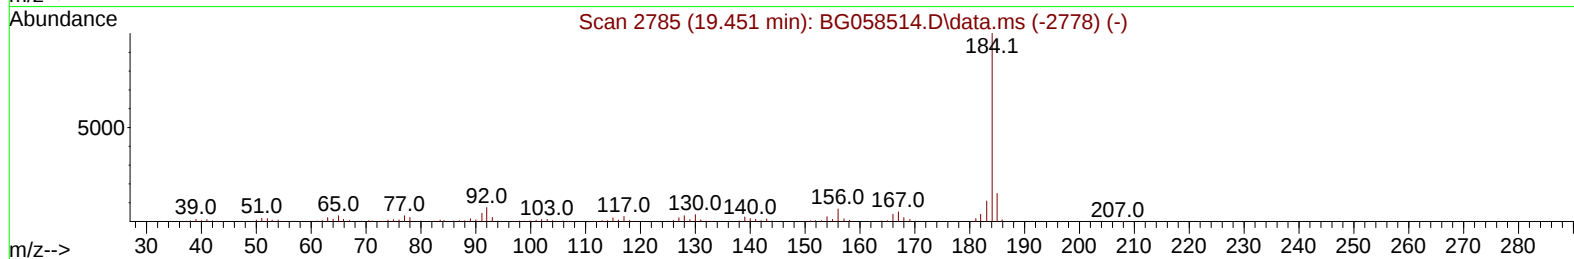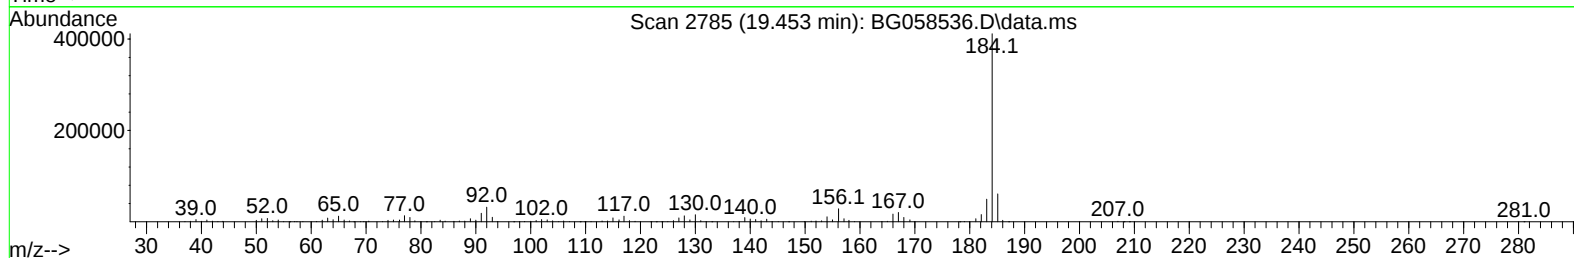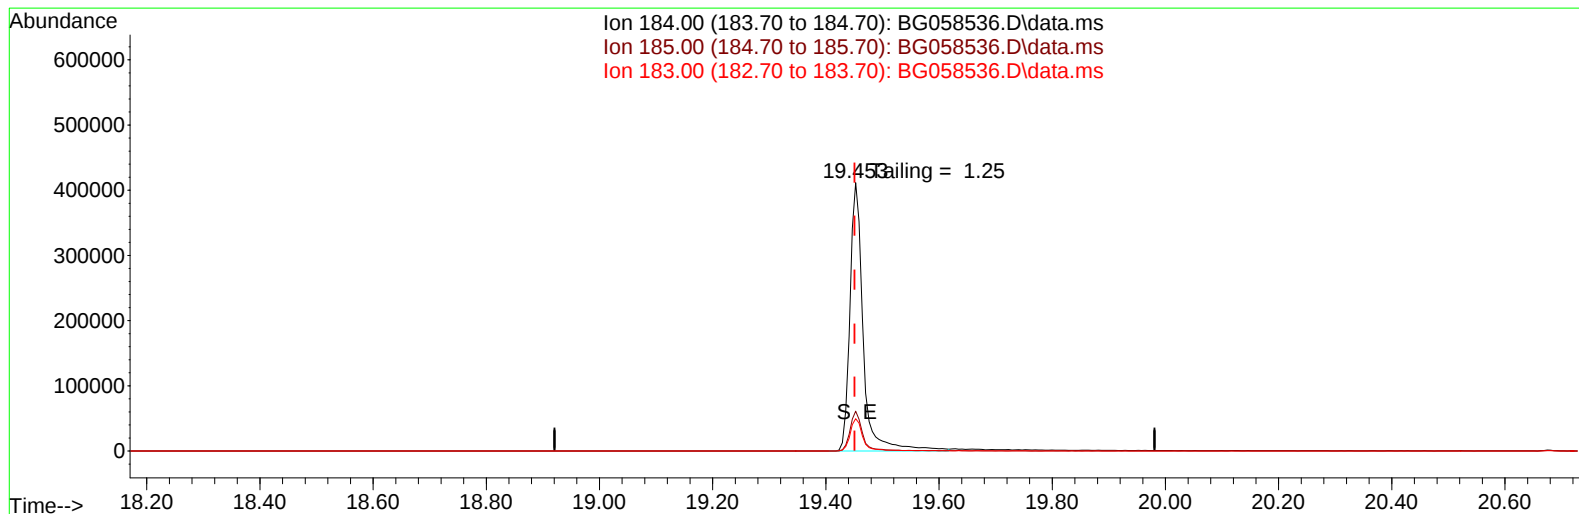

TIC: BG058536.D\data.ms

(77) Benzidine

19.453min (+ 0.002) 0.00 ng

response 673077

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.85
183.00	10.90	12.07
0.00	0.00	0.00