

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG073123\  
Data File : BG058538.D  
Acq On : 31 Jul 2023 11:09  
Operator : MA/JU  
Sample : PB154403BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB154403BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG058538.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 384           | 391         | 406          | rBV      | 950115         | 1513606       | 40.89%          | 10.299%       |
| 2         | 6.989       | 656           | 664         | 679          | rBV      | 857668         | 1491809       | 40.30%          | 10.151%       |
| 3         | 7.811       | 798           | 804         | 814          | rBV      | 145966         | 246770        | 6.67%           | 1.679%        |
| 4         | 8.981       | 995           | 1003        | 1022         | rBV      | 481413         | 901715        | 24.36%          | 6.136%        |
| 5         | 10.614      | 1273          | 1281        | 1295         | rBV      | 175557         | 346662        | 9.37%           | 2.359%        |
| 6         | 13.082      | 1694          | 1701        | 1727         | rBV      | 1220365        | 2006272       | 54.20%          | 13.652%       |
| 7         | 14.462      | 1929          | 1936        | 1949         | rBV      | 299148         | 481580        | 13.01%          | 3.277%        |
| 8         | 15.955      | 2183          | 2190        | 2217         | rBV      | 1014955        | 1701876       | 45.98%          | 11.581%       |
| 9         | 17.206      | 2396          | 2403        | 2417         | rBV      | 404291         | 650430        | 17.57%          | 4.426%        |
| 10        | 19.827      | 2843          | 2849        | 2862         | rBV      | 2641564        | 3701629       | 100.00%         | 25.188%       |
| 11        | 21.448      | 3119          | 3125        | 3138         | rBV      | 444052         | 801675        | 21.66%          | 5.455%        |
| 12        | 24.521      | 3638          | 3648        | 3660         | rBV      | 302851         | 851957        | 23.02%          | 5.797%        |




Sum of corrected areas: 14695981

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG073123\  
Data File : BG058538.D  
Acq On : 31 Jul 2023 11:09  
Operator : MA/JU  
Sample : PB154403BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB154403BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

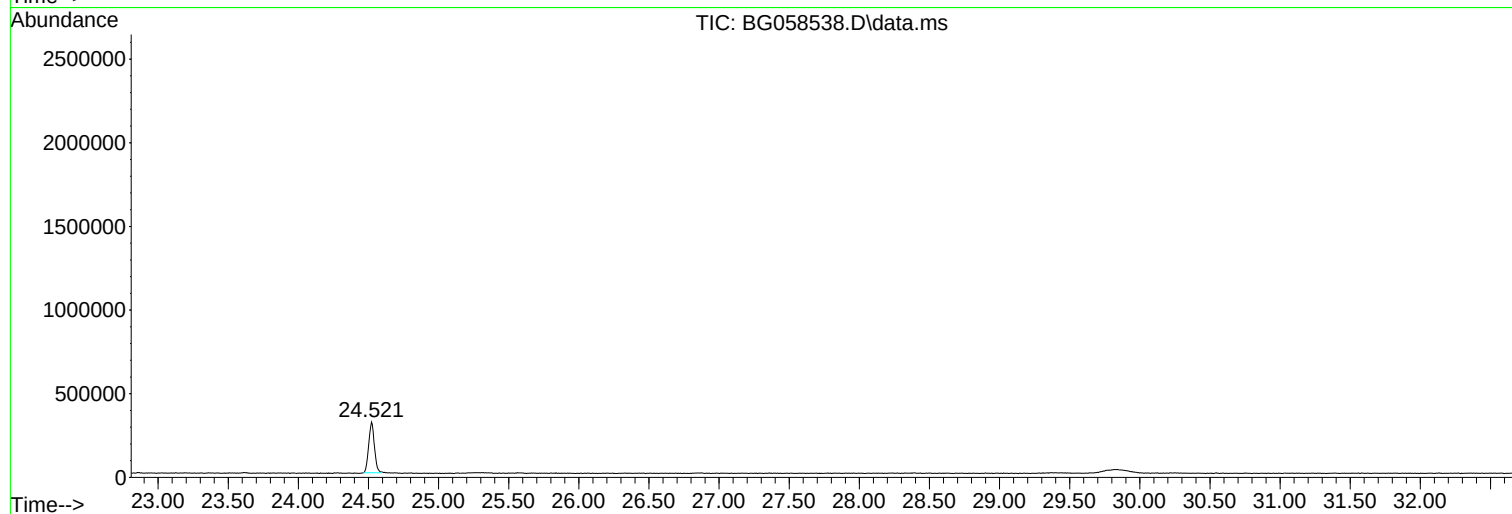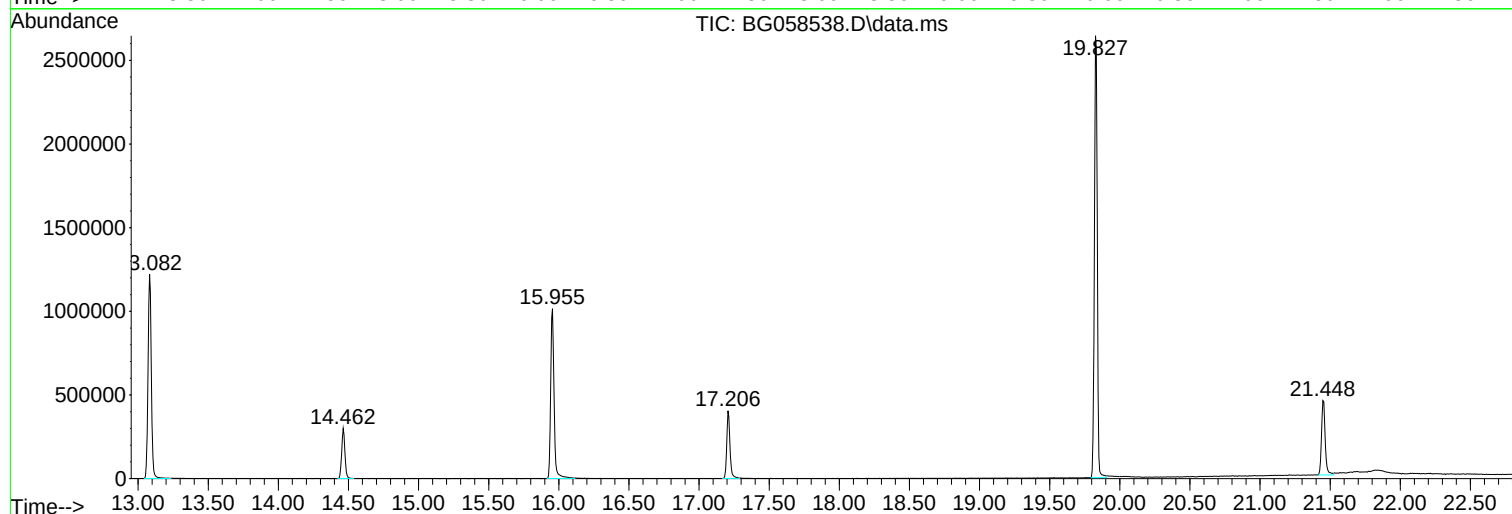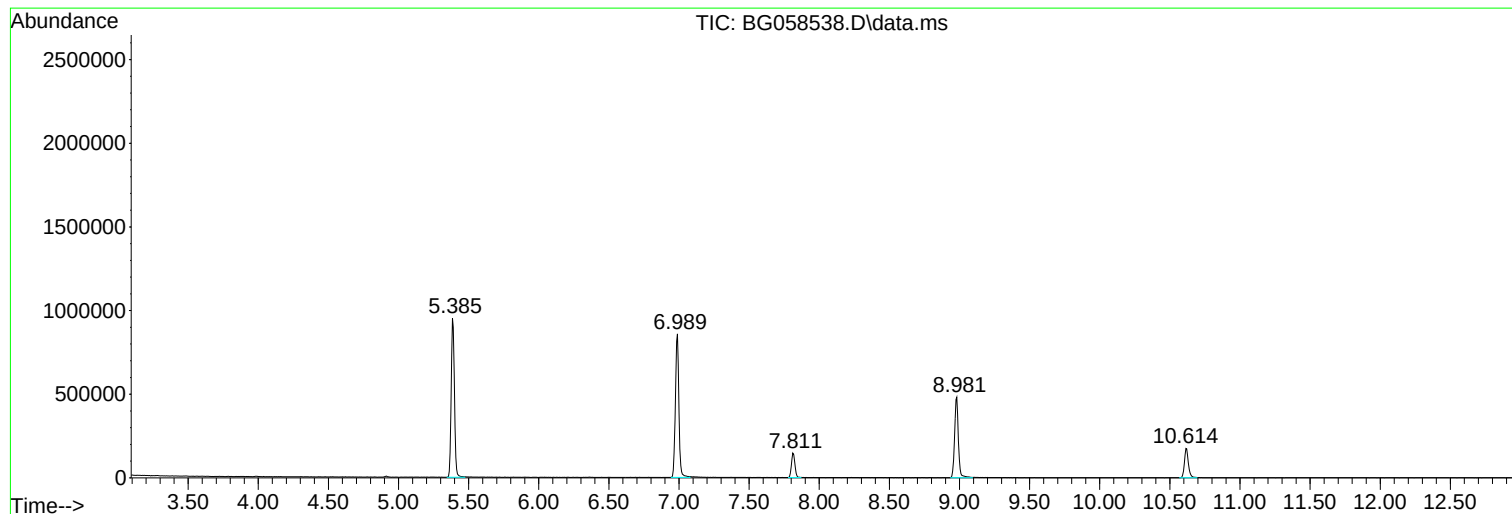

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG073123\  
Data File : BG058538.D  
Acq On : 31 Jul 2023 11:09  
Operator : MA/JU  
Sample : PB154403BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB154403BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG073123\  
Data File : BG058538.D  
Acq On : 31 Jul 2023 11:09  
Operator : MA/JU  
Sample : PB154403BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB154403BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|