
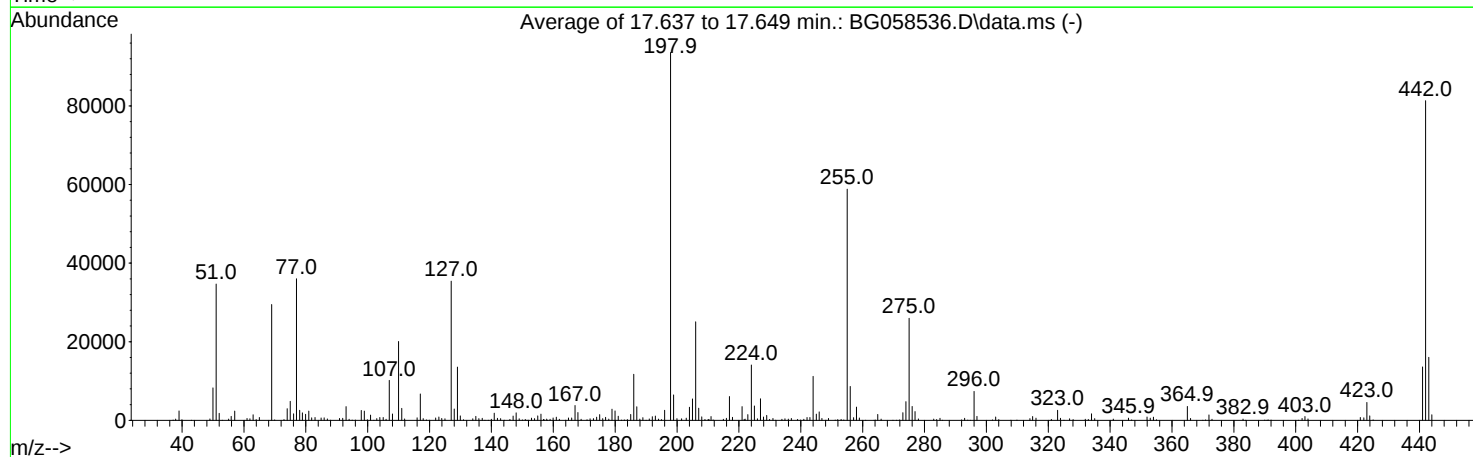


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073123\
Data File : BG058536.D
Acq On : 31 Jul 2023 9:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

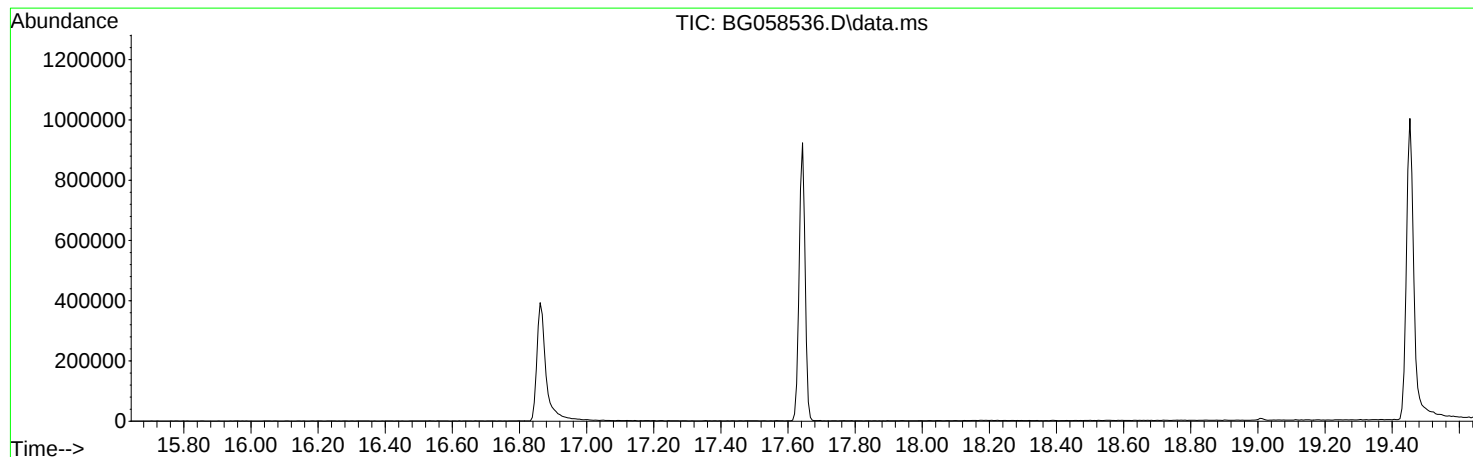

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	34699	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.5	29459	PASS
70	69	0.00	2	0.4	126	PASS
127	198	10	80	37.8	35413	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93584	PASS
199	198	5	9	6.9	6465	PASS
275	198	10	60	27.8	25981	PASS
365	198	1	100	3.8	3560	PASS
441	198	0.01	100	14.5	13604	PASS
442	442	50	100	100.0	81325	PASS
443	442	15	24	19.7	16057	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/31/2023	BNA_G	<u>BG058536.D</u>
Compound Name	Response	Retention Time
DDT	329179	20.675
DDD	5749	20.293
DDE	169	19.735
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5918	335097	1.77

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073123\
Data File : BG058536.D
Acq On : 31 Jul 2023 9:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 31 12:17:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

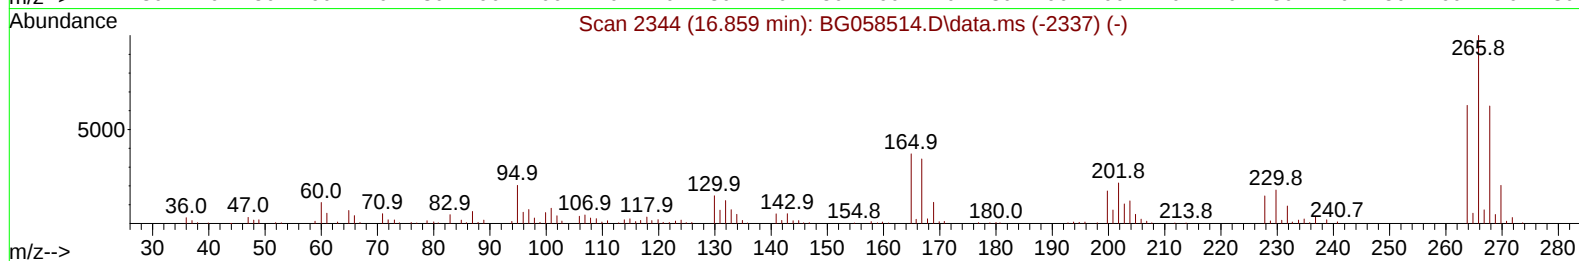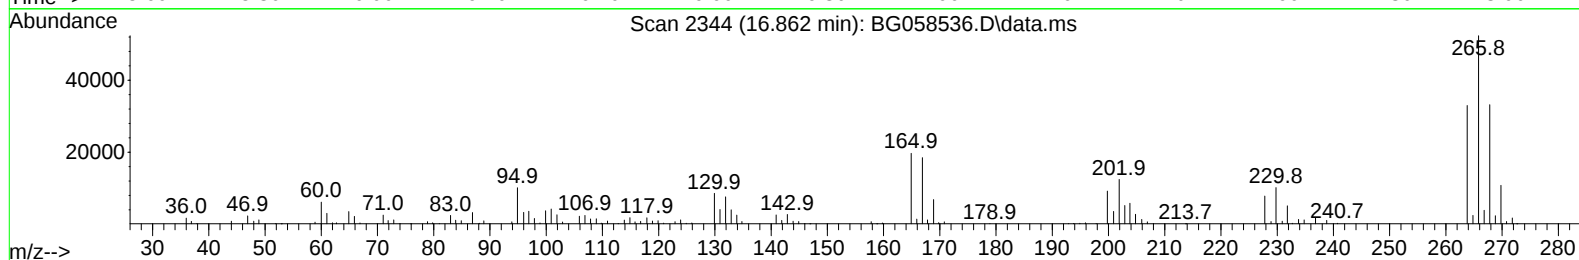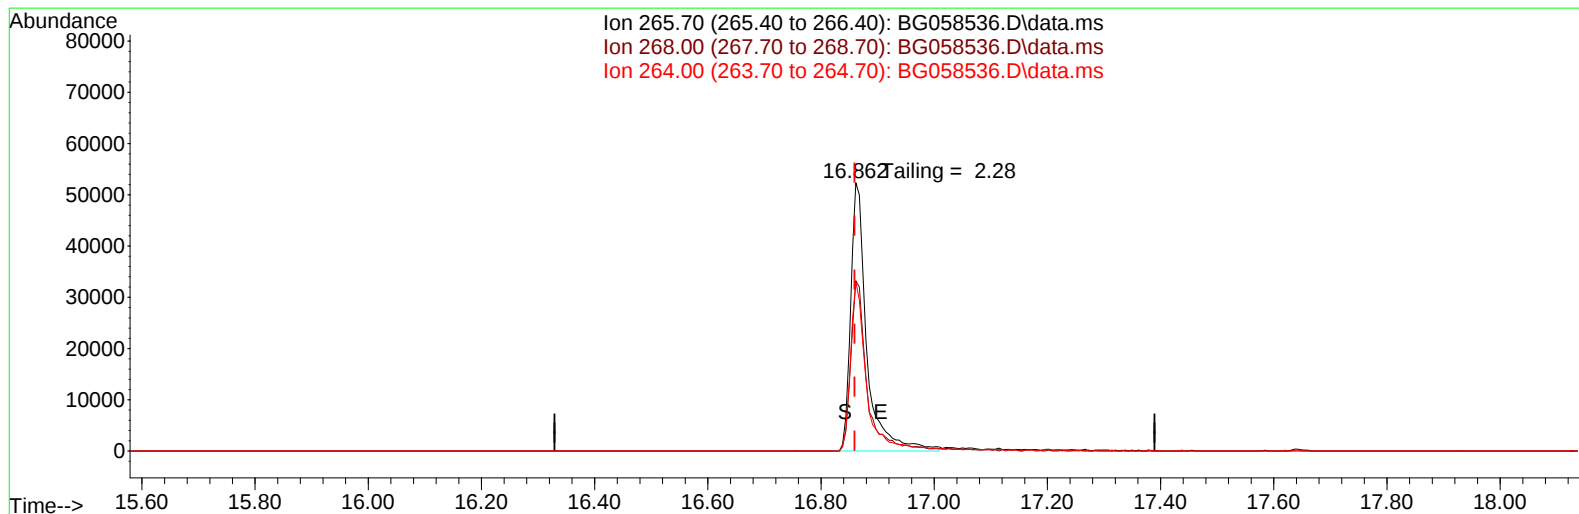

TIC: BG058536.D\data.ms

(70) Pentachlorophenol (C)

16.862min (+ 0.003) 31611.60 ng




response 103944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.46
264.00	62.80	63.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG073123\
Data File : BG058536.D
Acq On : 31 Jul 2023 9:48
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 31 12:17:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

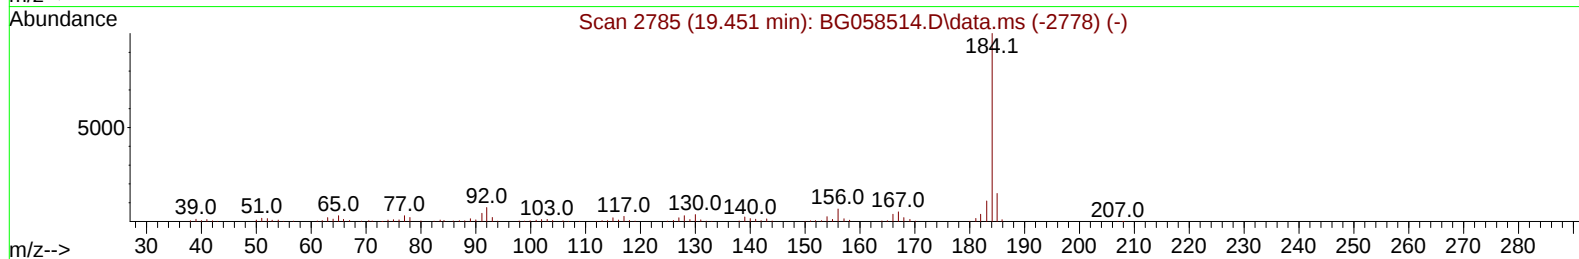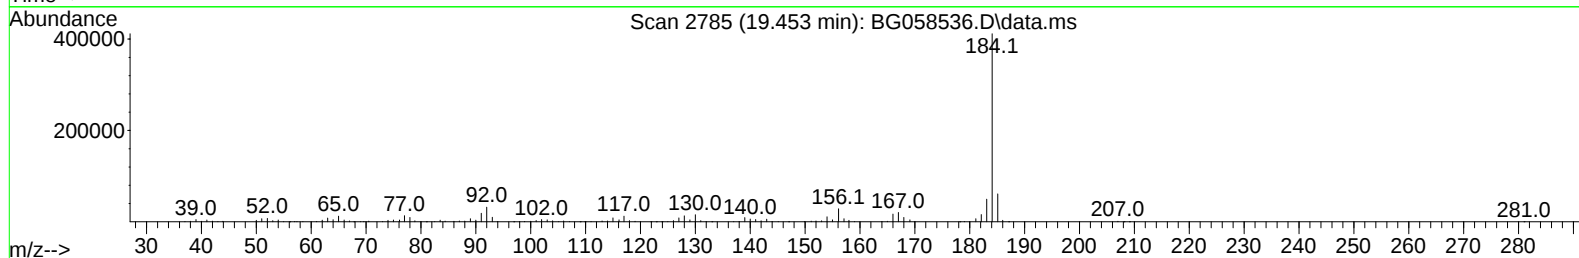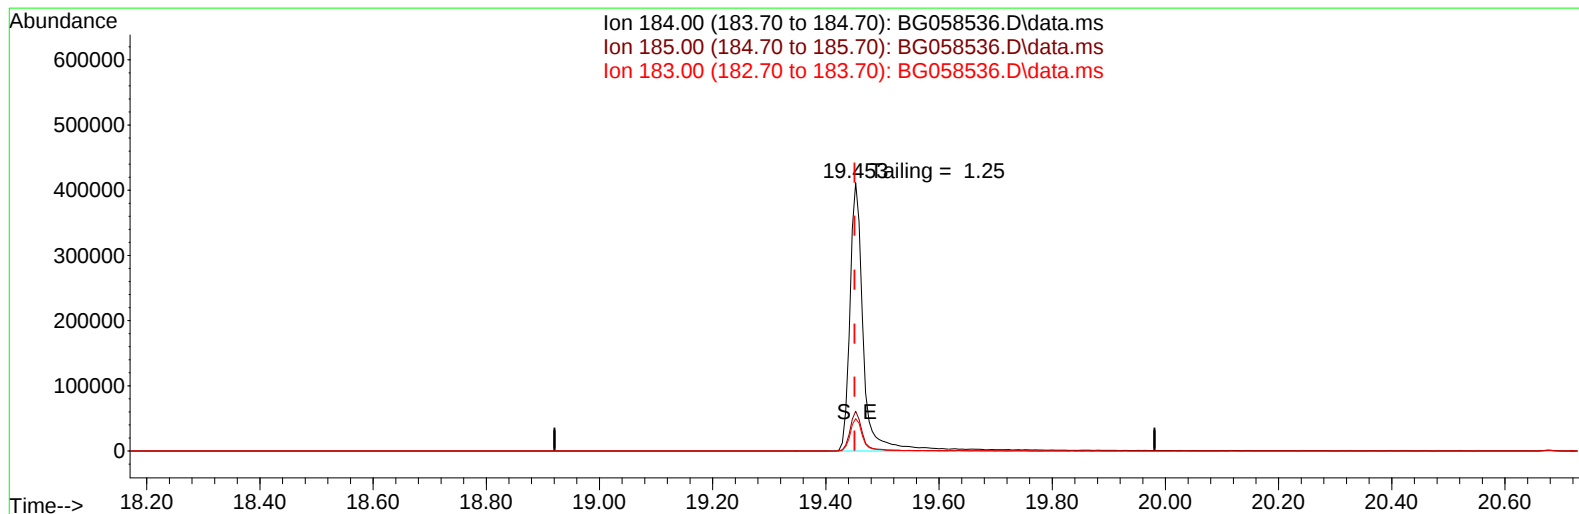

TIC: BG058536.D\data.ms

(77) Benzidine

19.453min (+ 0.002) 0.00 ng

response 673077

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.85
183.00	10.90	12.07
0.00	0.00	0.00