
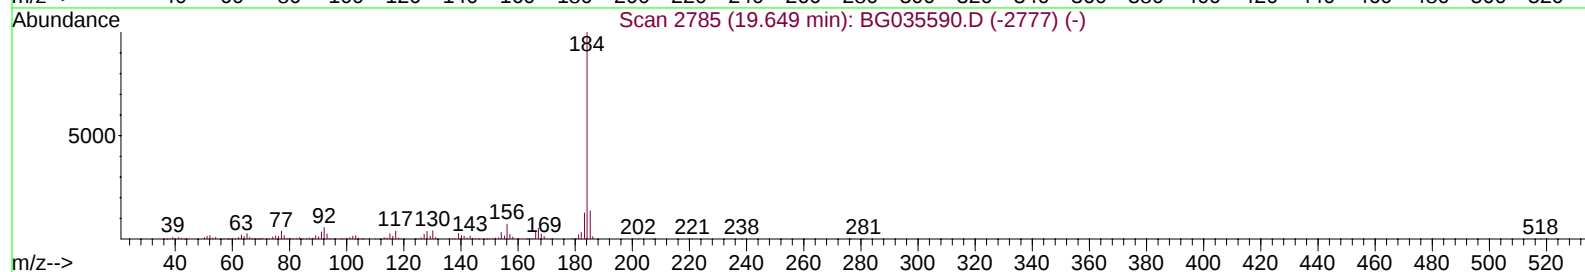
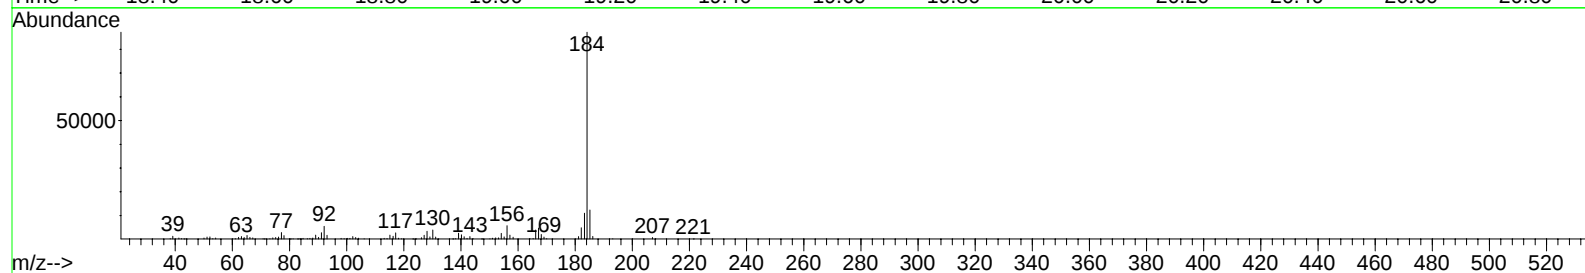


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080118\
Data File : BG036027.D
Acq On : 1 Aug 2018 10:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 13:06:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

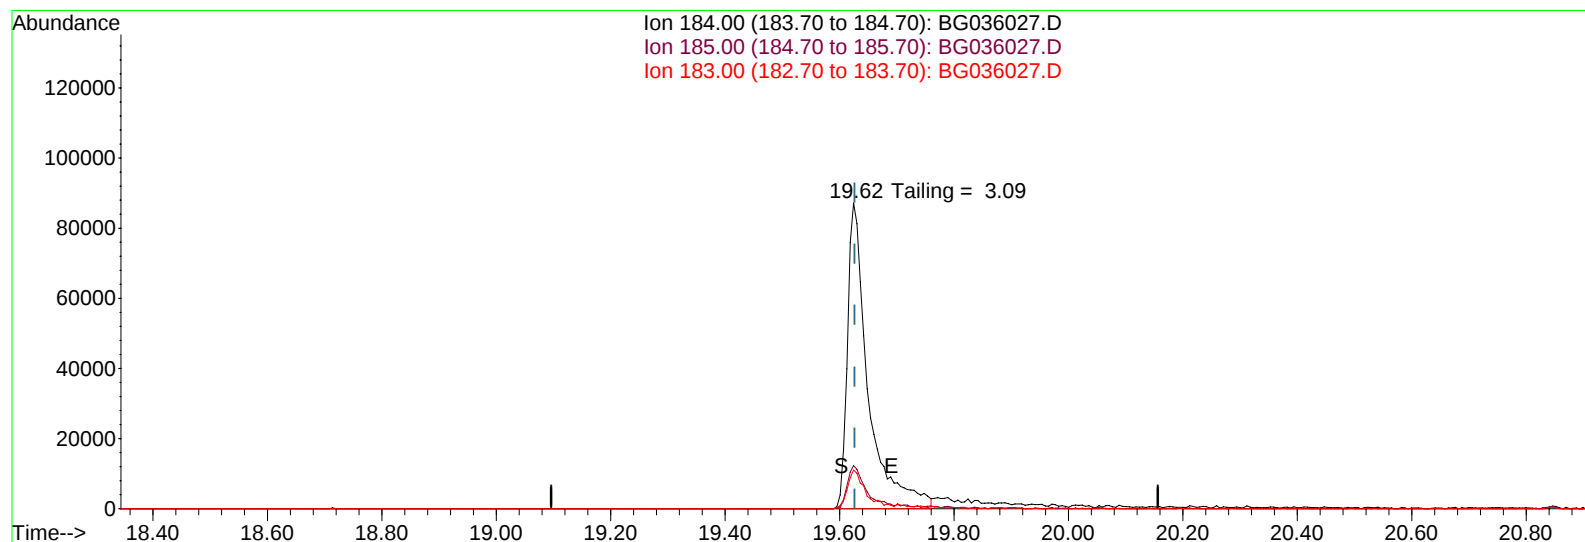

TIC: BG036027.D

(76) Benzidine




19.625min (-0.002) 0.00ng

response 220648

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.14
183.00	13.30	12.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080118\
Data File : BG036027.D
Acq On : 1 Aug 2018 10:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 13:06:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

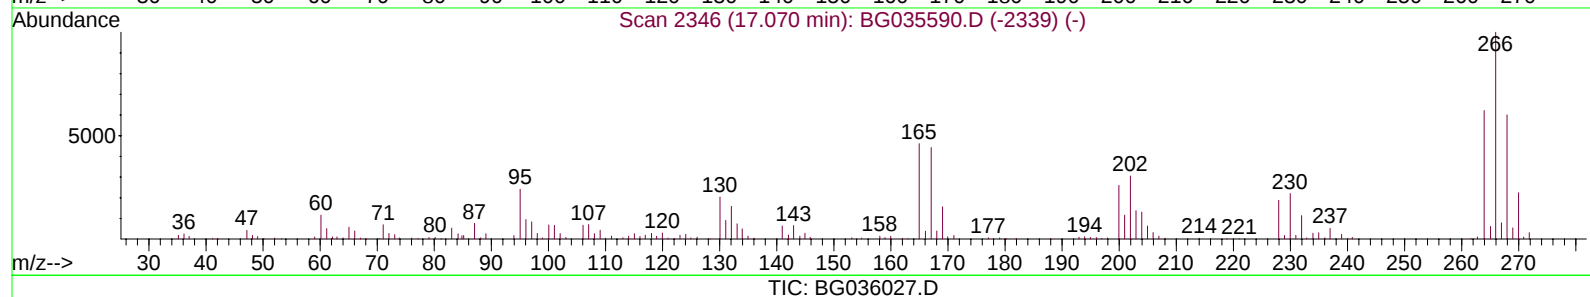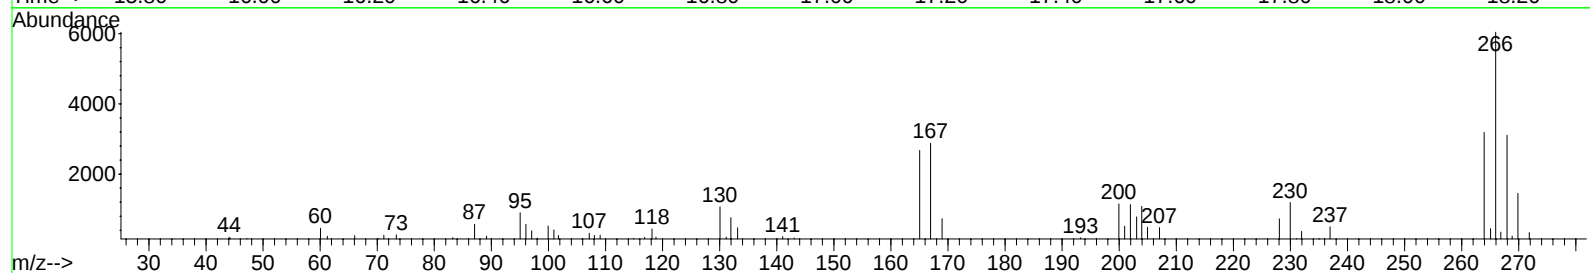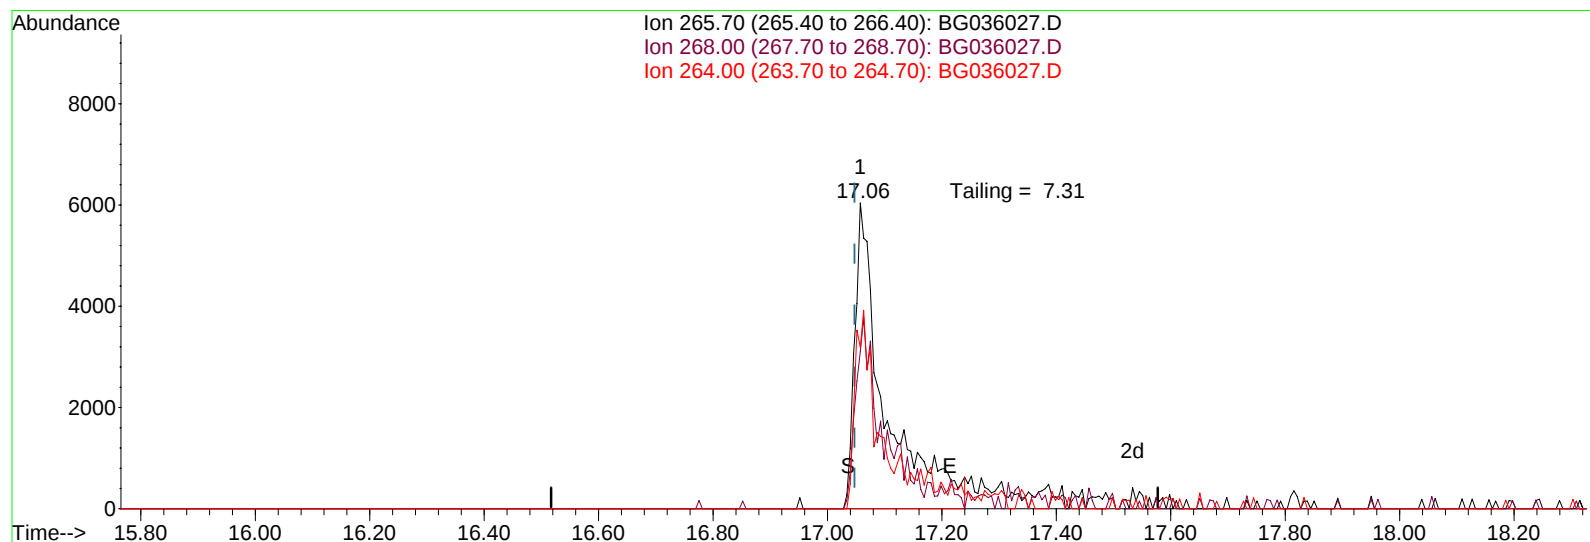

(69) Pentachlorophenol (C)

17.057min (+0.010) 11367.46ng

response 16131

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	51.39
264.00	62.00	52.81
0.00	0.00	0.00