
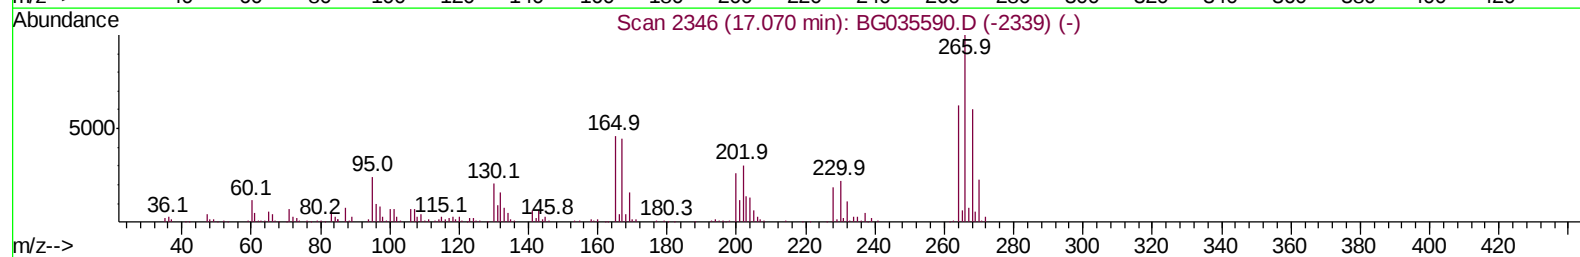
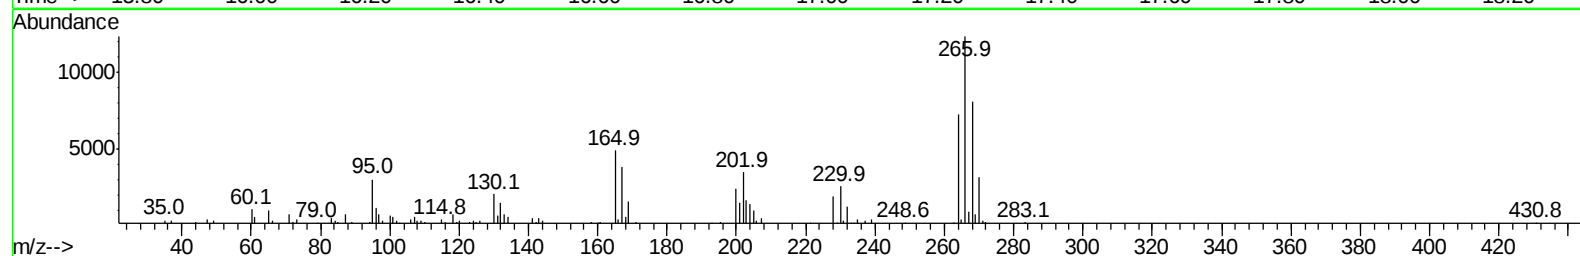


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080118\  
Data File : BG036045.D  
Acq On : 1 Aug 2018 23:07  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 10:01:39 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 31 12:30:06 2018  
Response via : Initial Calibration

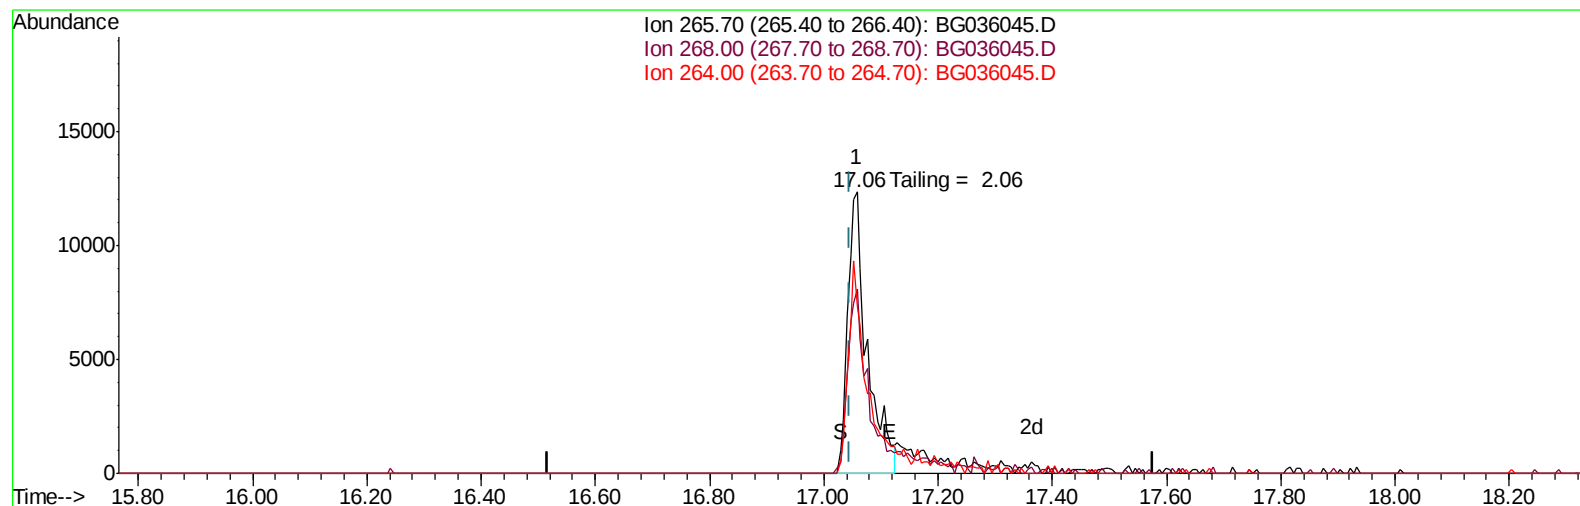

TIC: BG036045.D

(69) Pentachlorophenol (C)




17.058min (+0.011) 60914.13ng

response 26597

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 65.39 |
| 264.00 | 62.00 | 59.04 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080118\  
Data File : BG036045.D  
Acq On : 1 Aug 2018 23:07  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 10:01:39 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 31 12:30:06 2018  
Response via : Initial Calibration

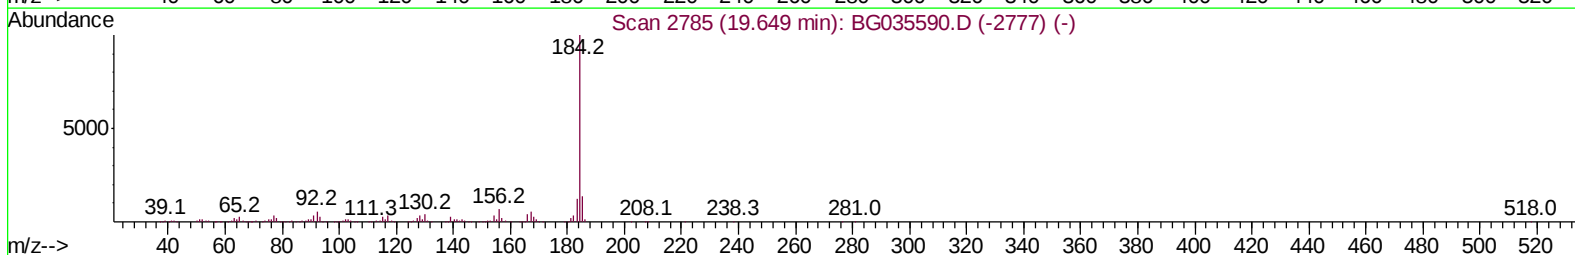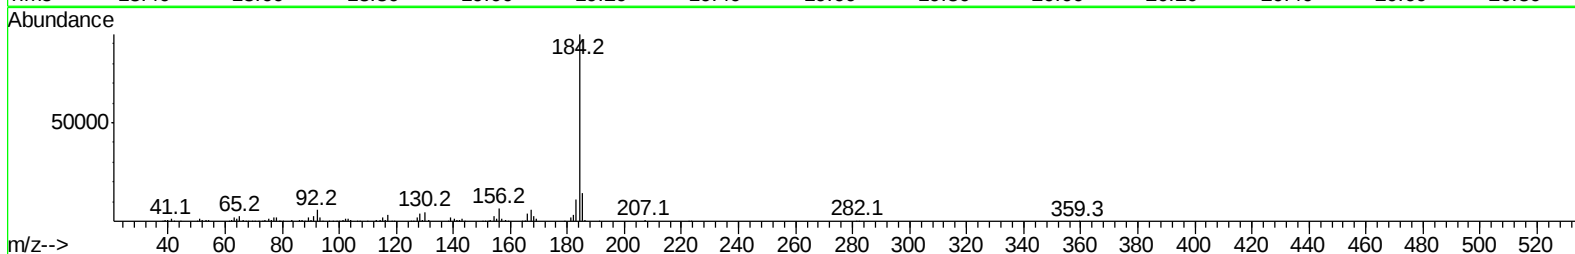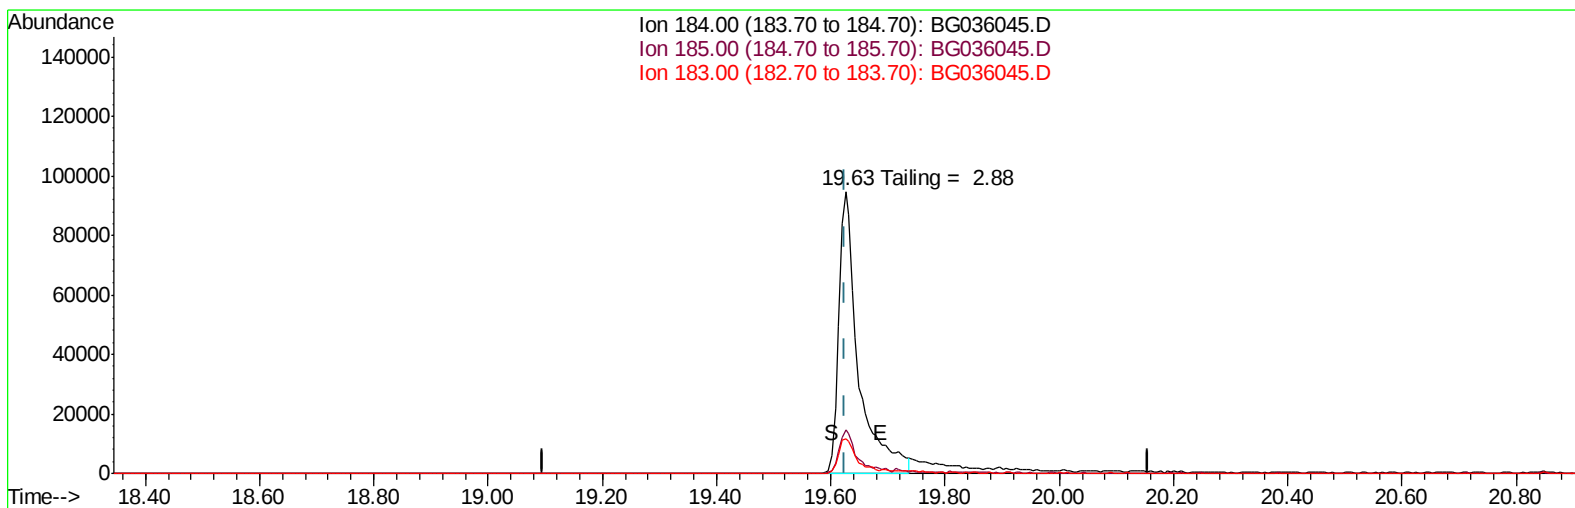

TIC: BG036045.D

(76) Benzidine

19.625min (-0.001) 171230.39ng

response 247593

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 15.39 |
| 183.00 | 13.30 | 12.08 |
| 0.00   | 0.00  | 0.00  |