


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080118\
 Data File : BG036027.D
 Acq On : 1 Aug 2018 10:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

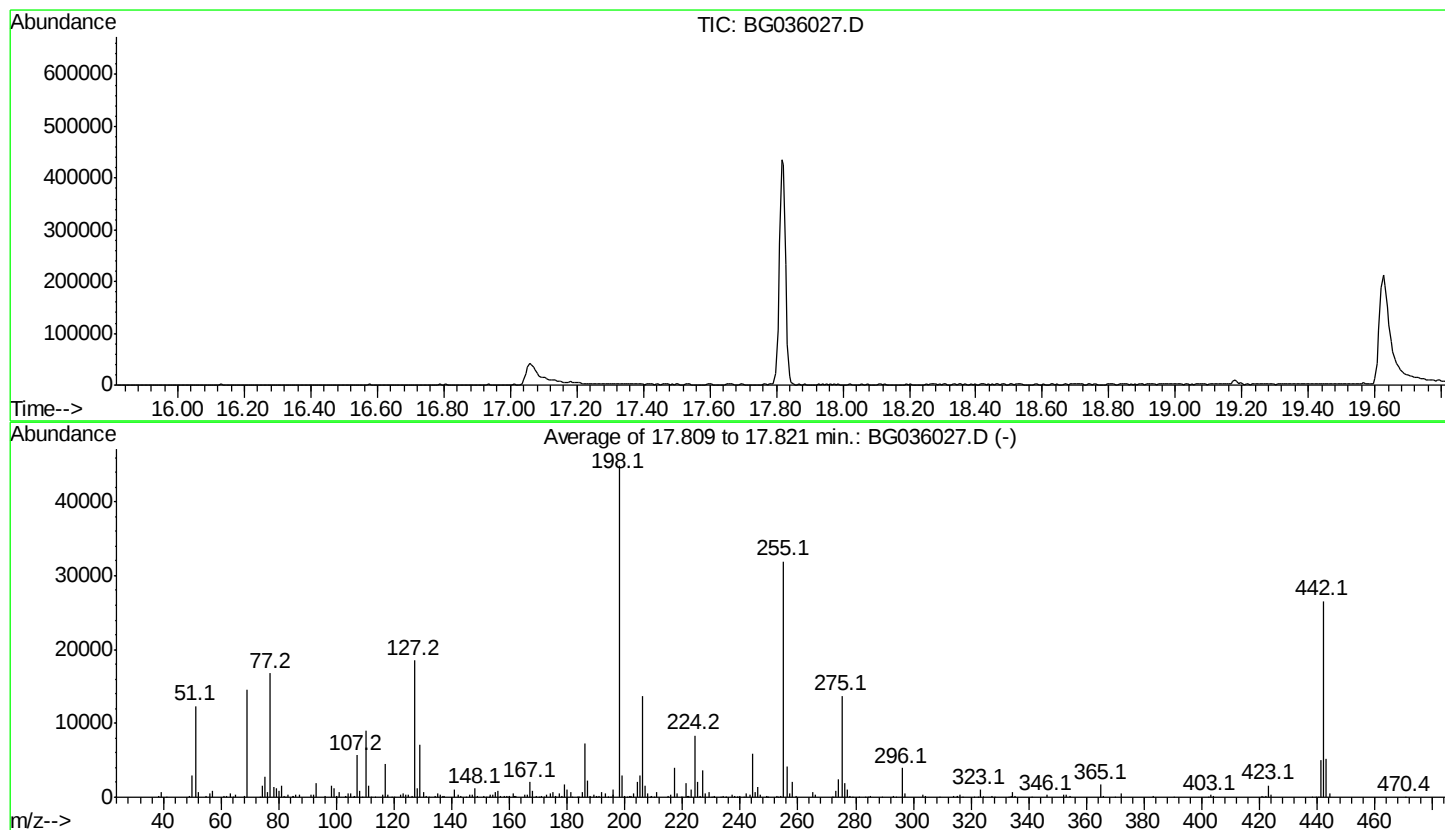

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	12390	PASS
68	69	0.00	2	1.2	175	PASS
69	198	0.00	100	32.6	14645	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.3	18525	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44896	PASS
199	198	5	9	6.5	2926	PASS
275	198	10	60	30.6	13753	PASS
365	198	1	100	3.9	1731	PASS
441	198	0.01	100	11.0	4951	PASS
442	198	50	100	59.2	26579	PASS
443	442	15	24	19.4	5165	PASS