
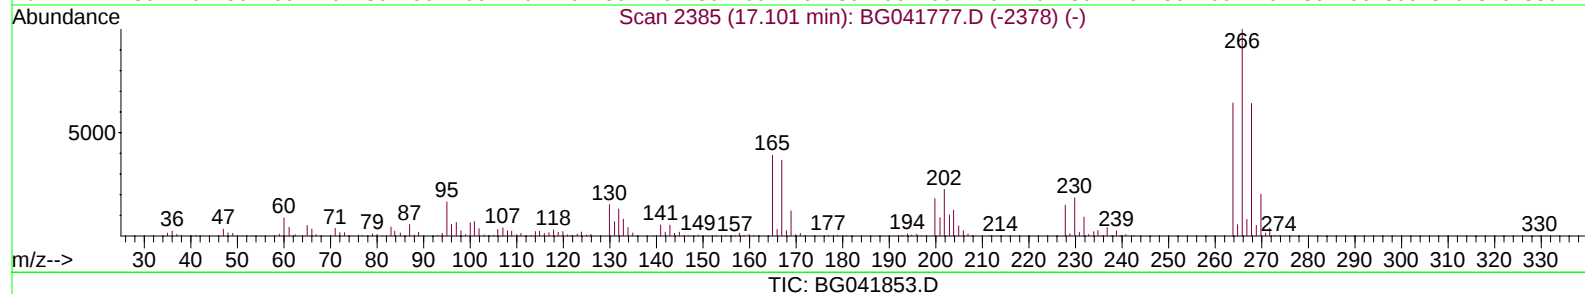
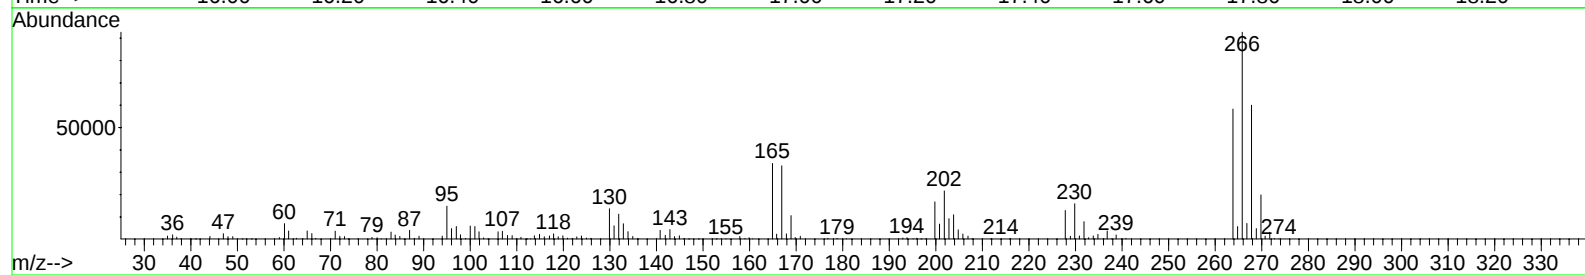


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080119\
Data File : BG041853.D
Acq On : 1 Aug 2019 8:29
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 18:47:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

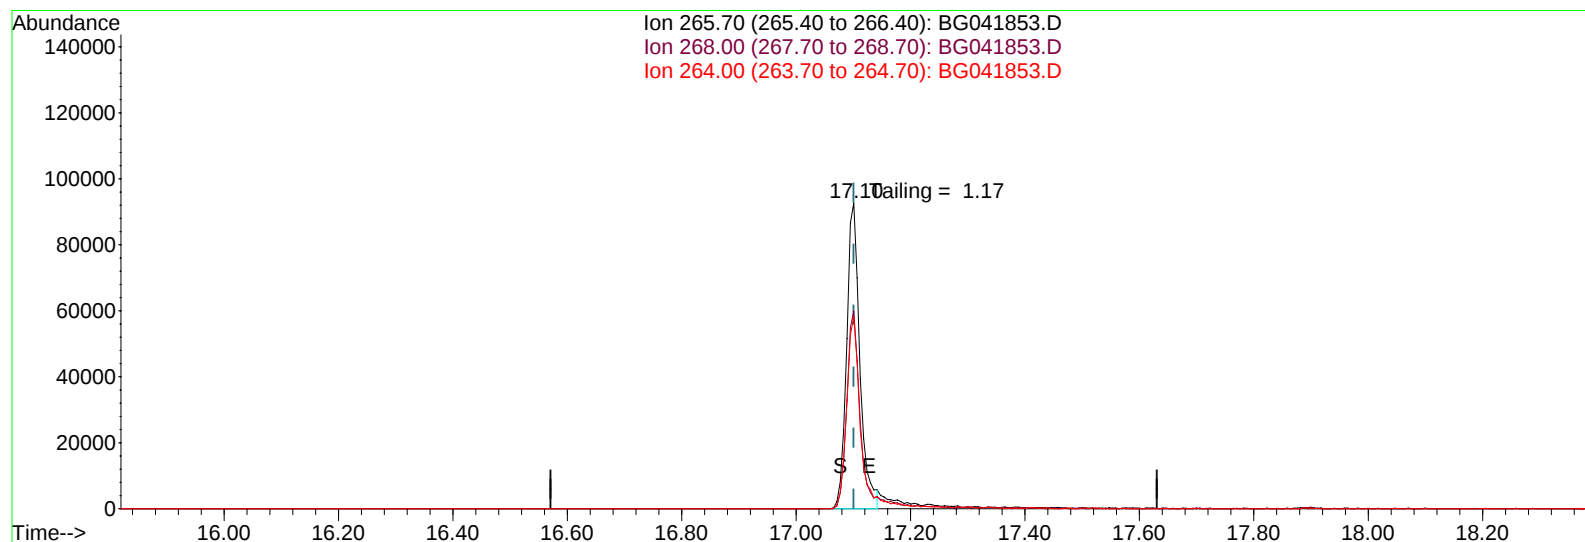

(70) Pentachlorophenol (C)




17.101min (-0.000) 28122.79ng

response 160793

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	64.74
264.00	64.30	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080119\
Data File : BG041853.D
Acq On : 1 Aug 2019 8:29
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 18:47:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

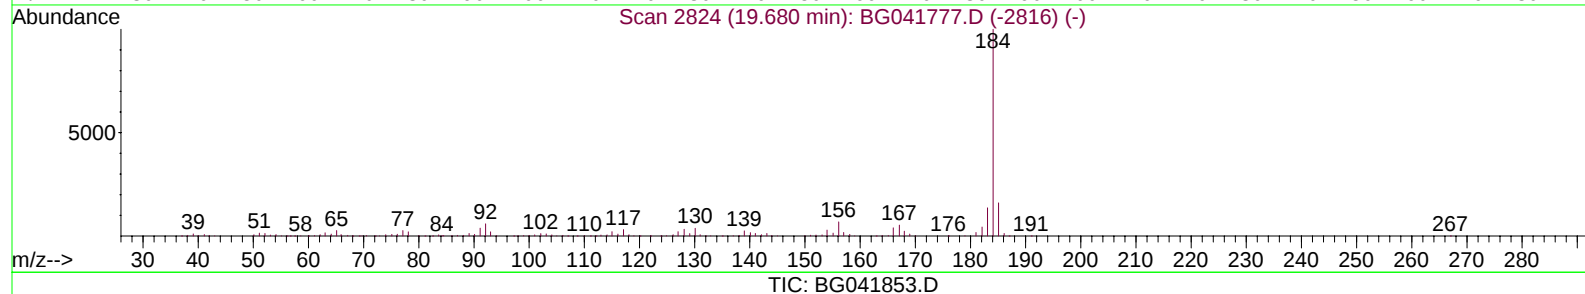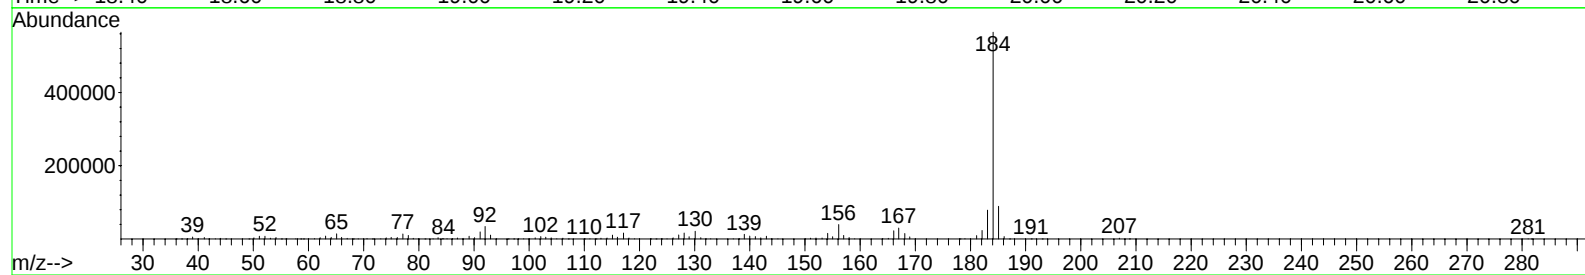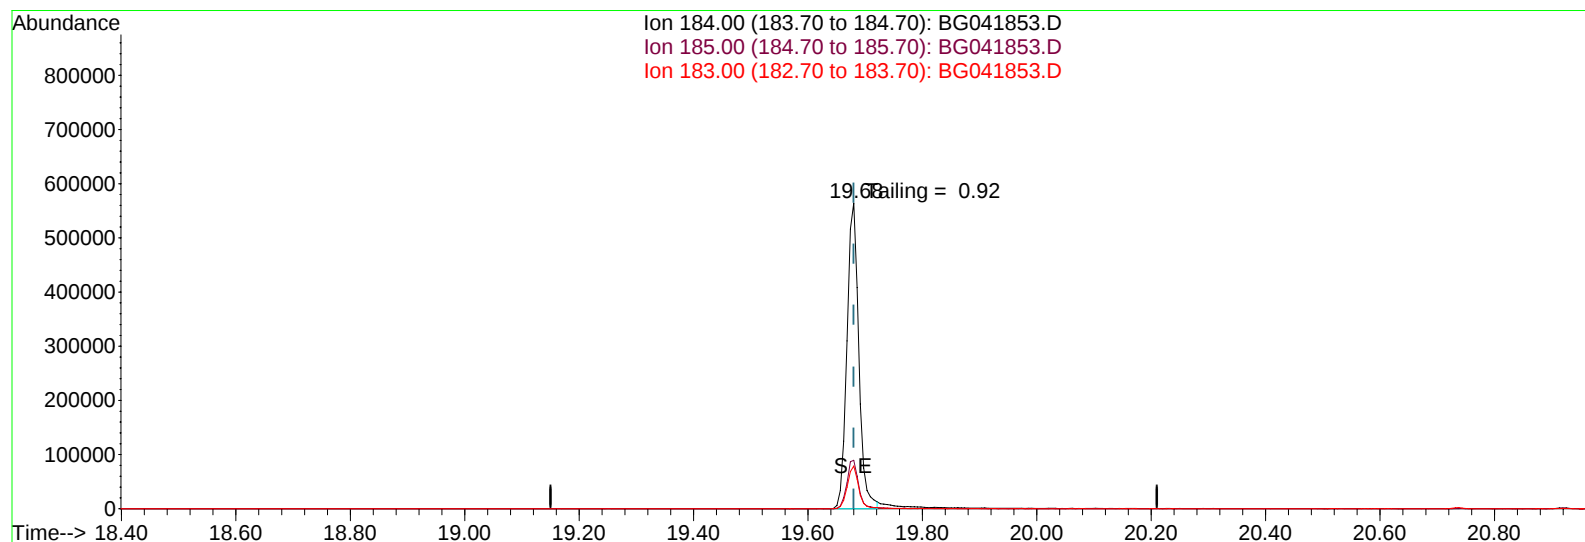

(77) Benzidine

19.680min (-0.000) 474291.82ng

response 835971

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.85
183.00	14.70	13.98
0.00	0.00	0.00