

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080119\
 Data File : BG041874.D
 Acq On : 1 Aug 2019 21:58
 Operator : HP/JU
 Sample : K4044-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-1

Quant Time: Aug 02 03:55:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 08:57:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	78930	20.00	ng	0.00
21) Naphthalene-d8	10.87	136	296400	20.00	ng	0.00
39) Acenaphthene-d10	14.70	164	196091	20.00	ng	0.00
64) Phenanthrene-d10	17.45	188	459357	20.00	ng	0.00
76) Chrysene-d12	21.73	240	622072	20.00	ng	0.00
87) Perylene-d12	25.00	264	741892	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	514694	126.87	ng	0.00
7) Phenol-d6	7.19	99	622985	113.91	ng	0.00
23) Nitrobenzene-d5	9.20	82	469780	109.07	ng	0.00
42) 2,4,6-Tribromophenol	16.18	330	330952	148.59	ng	0.00
45) 2-Fluorobiphenyl	13.32	172	1130090	101.64	ng	0.00
79) Terphenyl-d14	20.06	244	2226183	81.89	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080119\
Data File : BG041874.D
Acq On : 1 Aug 2019 21:58
Operator : HP/JU
Sample : K4044-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-1

Quant Time: Aug 02 03:55:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

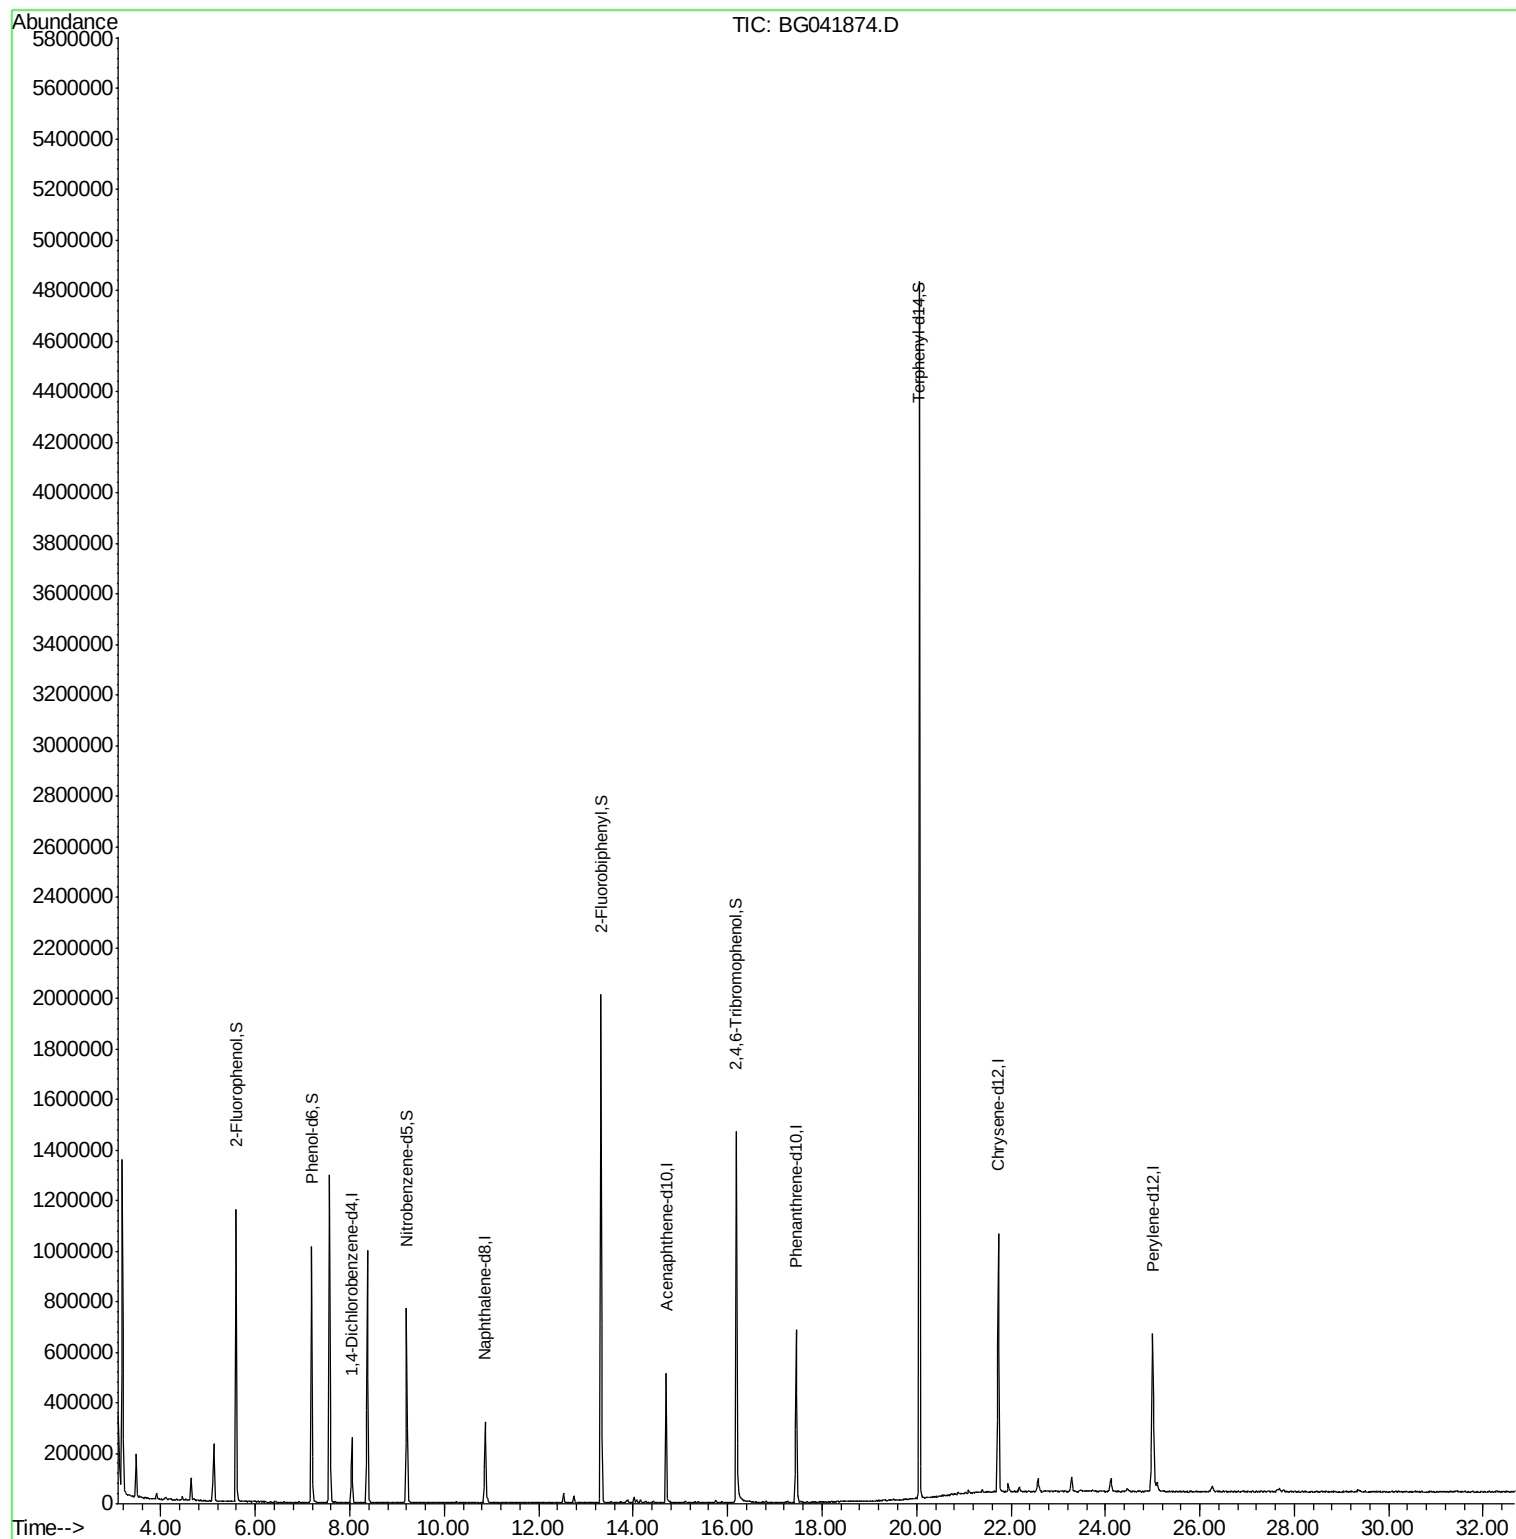

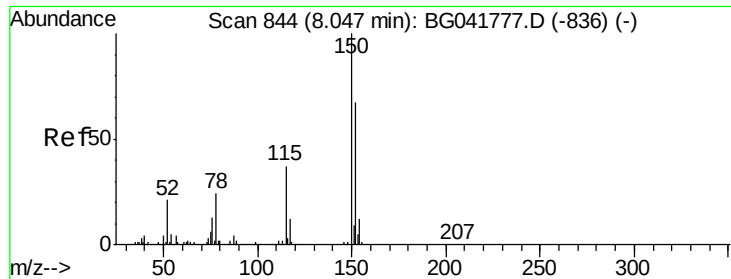


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.01 min
Lab File: BG041874.D
Acq: 1 Aug 2019 21:58

Instrument :
BNA_G
ClientSampleId :
TP-1

Tot Ion	Ratio	Lower	Upper
152	100		
150	148.2	126.9	190.3
115	54.1	45.0	67.6

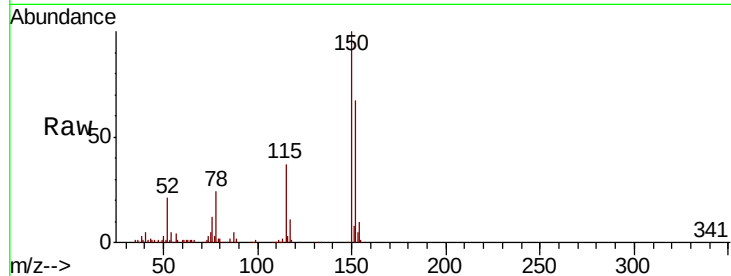


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

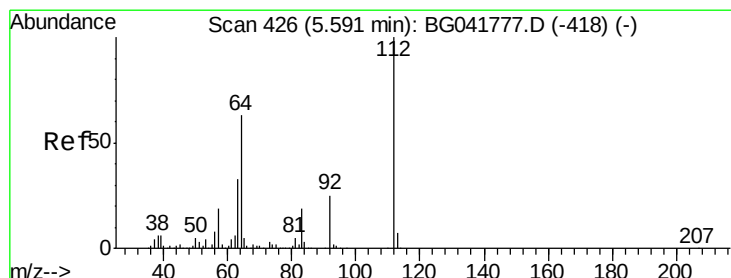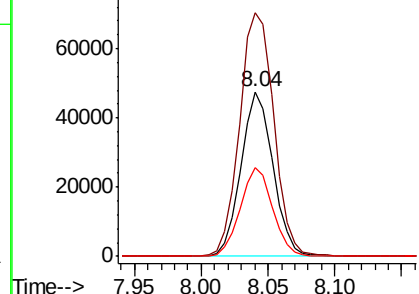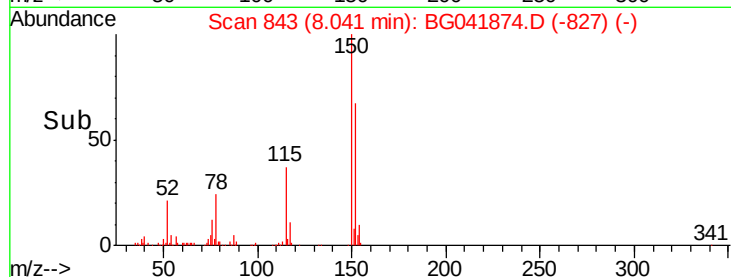



#5


2-Fluorophenol
Concen: 126.872 ng
RT: 5.59 min Scan# 426
Delta R.T. -0.00 min
Lab File: BG041874.D
Acq: 1 Aug 2019 21:58

Tgt Ion	Ratio	Lower	Upper
112	100		
64	65.0	55.4	83.2
63	32.9	29.1	43.7

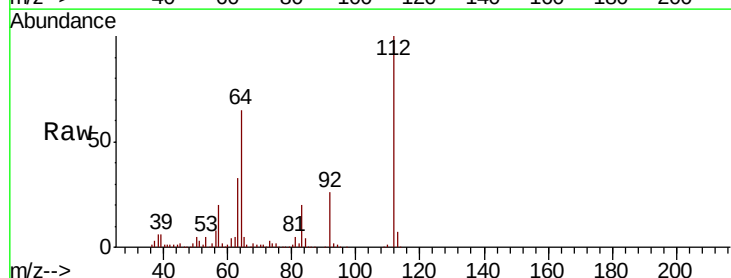

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

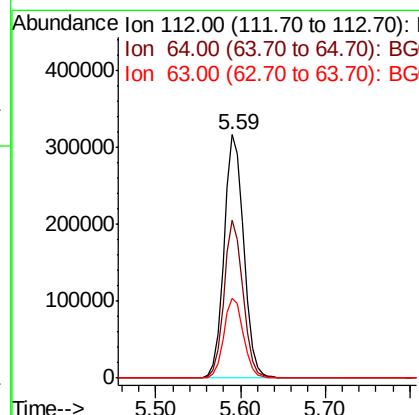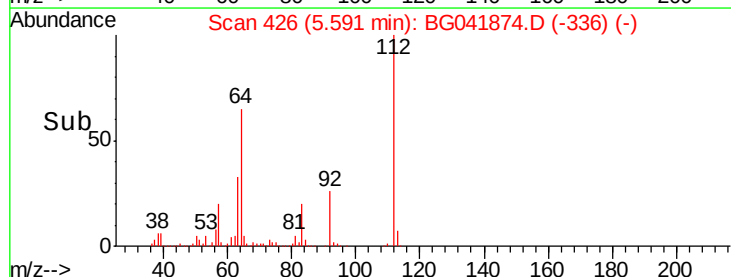

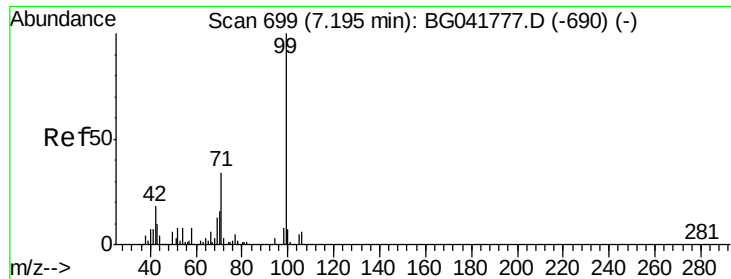

#7

Phenol-d6

Concen: 113.907 ng

RT: 7.19 min Scan# 698

Delta R.T. -0.01 min

Lab File: BG041874.D

Acq: 1 Aug 2019 21:58

Instrument :

BNA_G

ClientSampleId :

TP-1





Tot Ion: 99 Resp: 622985

Ion Ratio Lower Upper

99 100

42 17.5 17.6 26.4#

71 35.2 27.8 41.6

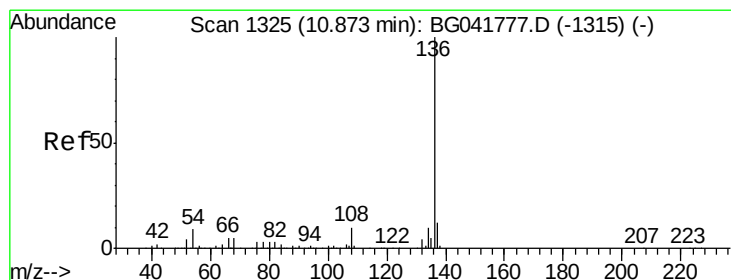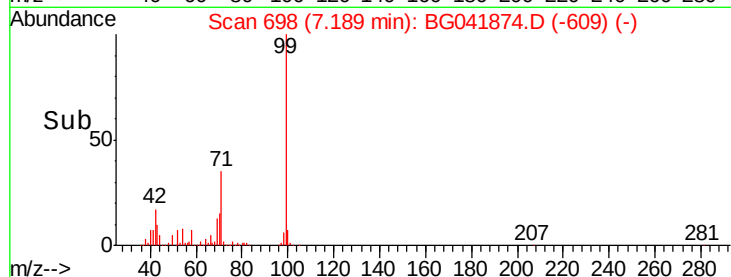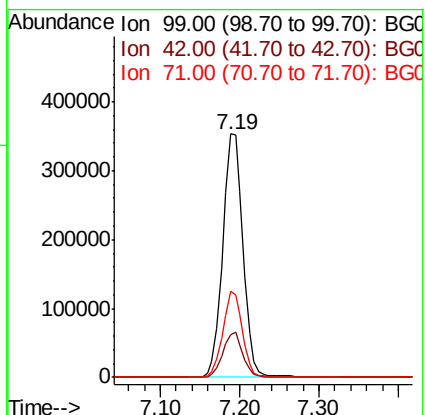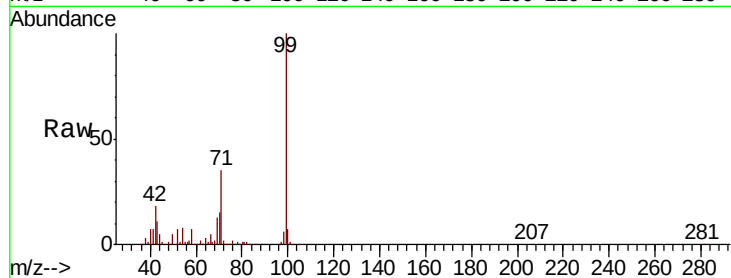

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.87 min Scan# 1324

Delta R.T. -0.01 min

Lab File: BG041874.D

Acq: 1 Aug 2019 21:58

Tgt Ion: 136 Resp: 296400




Ion Ratio Lower Upper


136 100

137 10.8 9.2 13.8

54 8.1 8.7 13.1#

68 5.1 5.5 8.3#


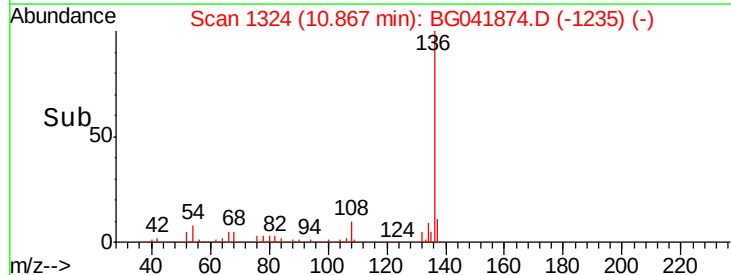
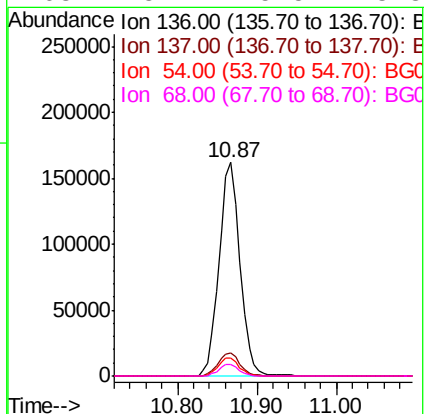
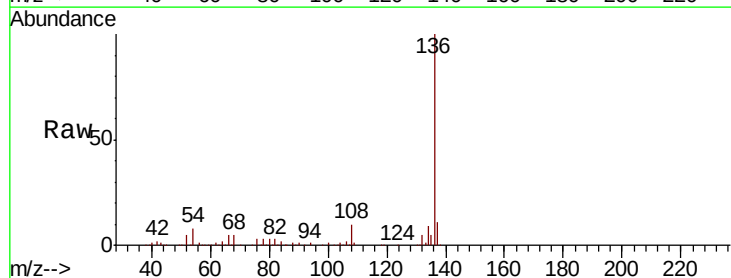


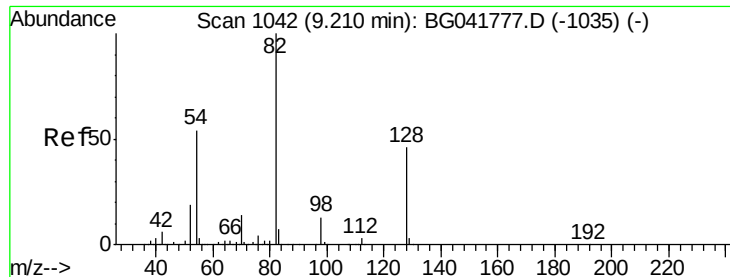

#23
Nitrobenzene-d5
Concen: 109.070 ng
RT: 9.20 min Scan# 1041
Delta R.T. -0.01 min
Lab File: BG041874.D
Acq: 1 Aug 2019 21:58




Instrument :
BNA_G
ClientSampleId :
TP-1


Tot Ion	82	Resp	469780
Ion Ratio	Lower	Upper	
82	100		
128	45.8	35.1	52.7
54	54.0	48.7	73.1

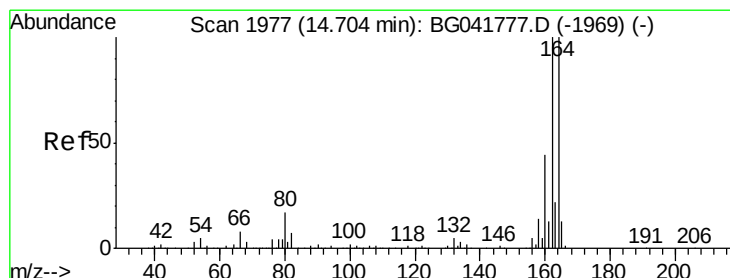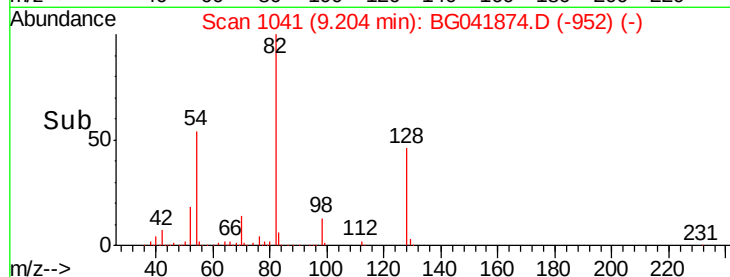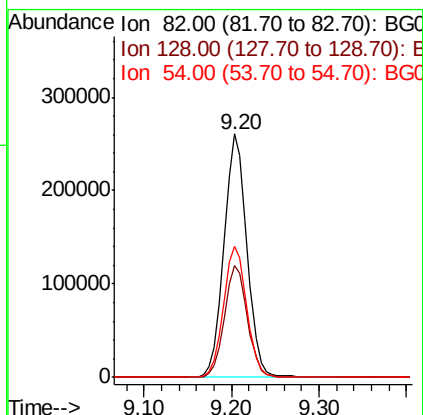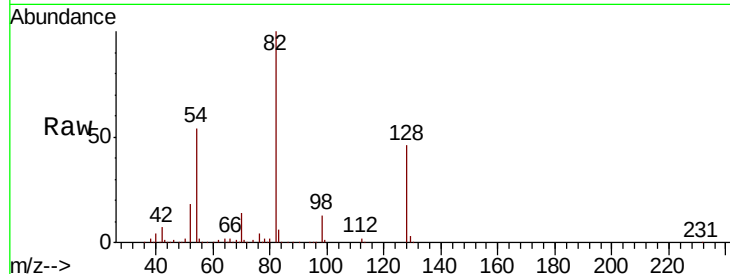

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.70 min Scan# 1976
Delta R.T. -0.01 min
Lab File: BG041874.D
Acq: 1 Aug 2019 21:58

Tgt Ion	164	Resp	196091
Ion Ratio	Lower	Upper	
164	100		
162	99.7	79.6	119.4
160	43.7	35.4	53.0

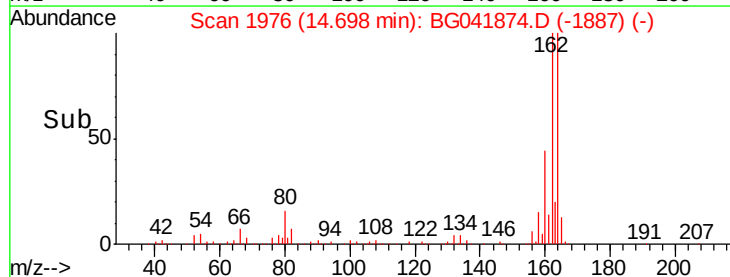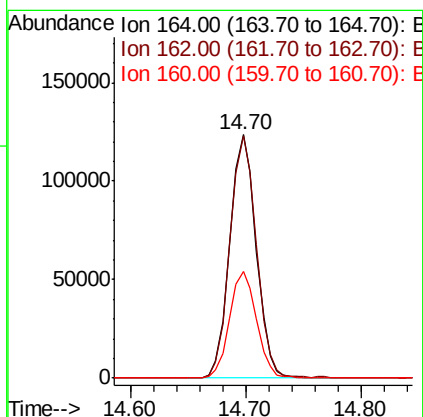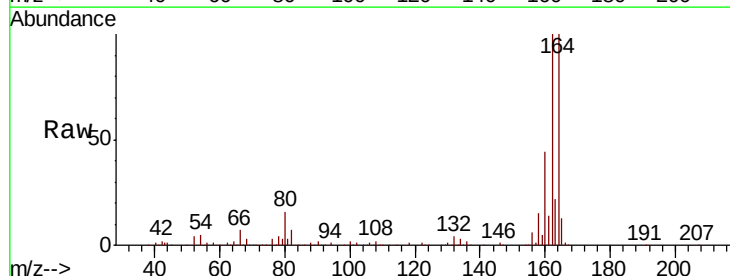

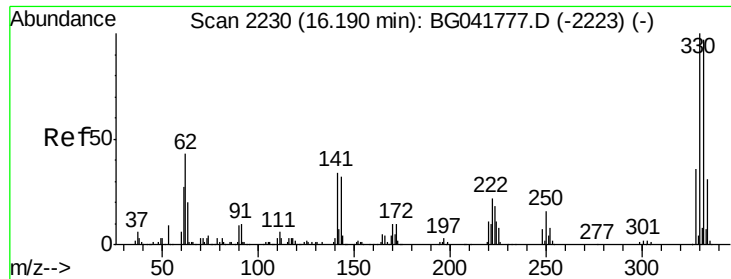

#42

2,4,6-Tribromophenol

Concen: 148.587 ng

RT: 16.18 min Scan# 2229

Delta R.T. -0.01 min

Lab File: BG041874.D

Acq: 1 Aug 2019 21:58

Instrument :

BNA_G

ClientSampled :

TP-1


Tot Ion:330 Resp: 330952

Ion Ratio Lower Upper

330 100

332 97.9 77.4 116.0




141 33.7 31.9 47.9

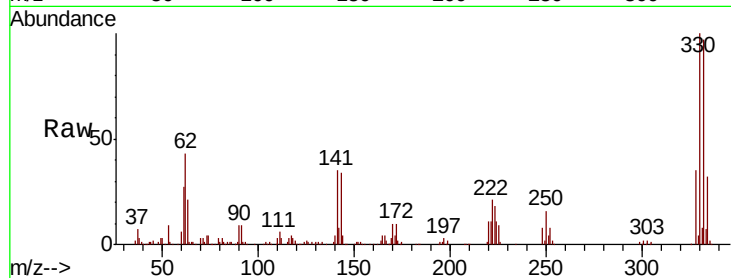

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

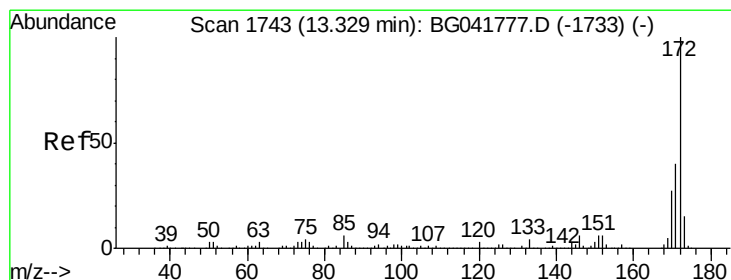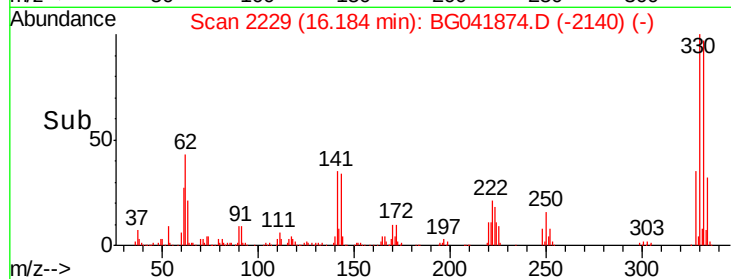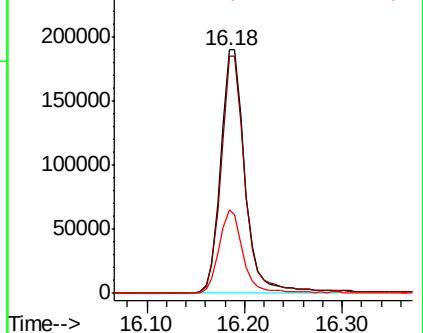

#45

2-Fluorobiphenyl

Concen: 101.645 ng

RT: 13.32 min Scan# 1742

Delta R.T. -0.01 min

Lab File: BG041874.D

Acq: 1 Aug 2019 21:58


Tgt Ion:172 Resp: 1130090

Ion Ratio Lower Upper

172 100

171 40.0 35.0 52.4



170 25.7 23.5 35.3

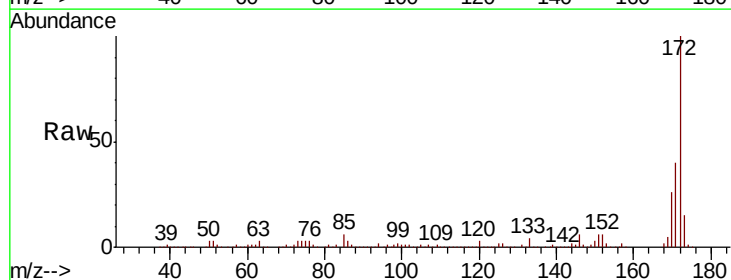


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

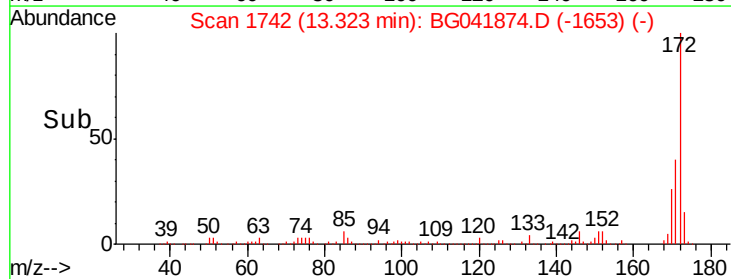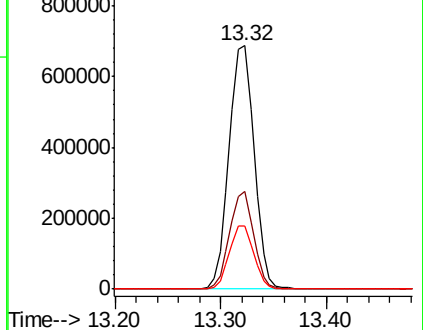

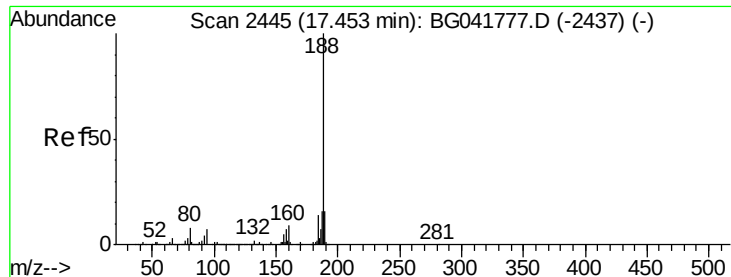

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.45 min Scan# 2444

Delta R.T. -0.01 min

Lab File: BG041874.D

Acq: 1 Aug 2019 21:58

Instrument :

BNA_G

ClientSampleId :

TP-1


Tot Ion:188 Resp: 459357

Ion Ratio Lower Upper

188 100

94 7.0 6.9 10.3




80 7.6 8.0 12.0#

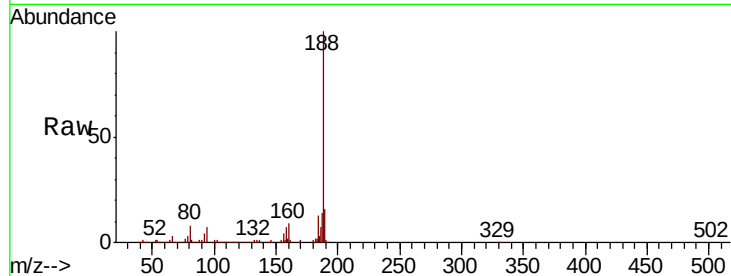

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

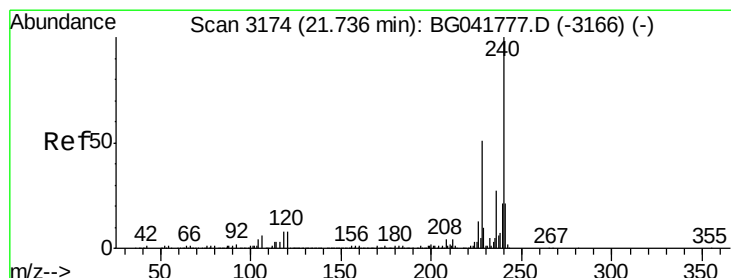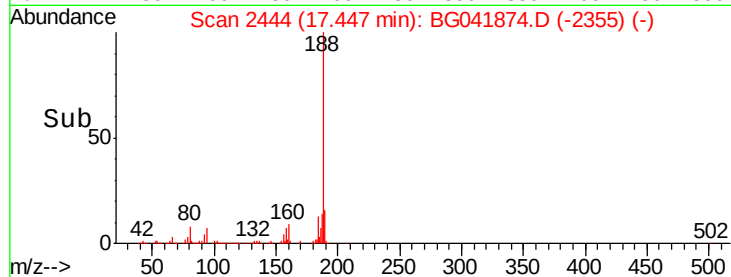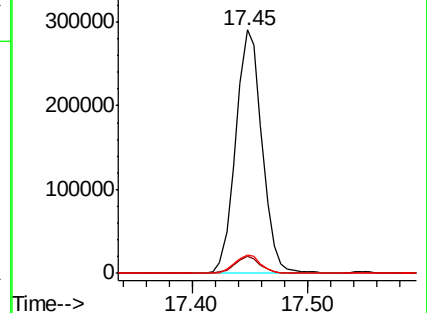

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.73 min Scan# 3173

Delta R.T. -0.01 min

Lab File: BG041874.D

Acq: 1 Aug 2019 21:58


Tgt Ion:240 Resp: 622072

Ion Ratio Lower Upper

240 100

120 8.0 8.0 12.0



236 27.1 22.6 33.8

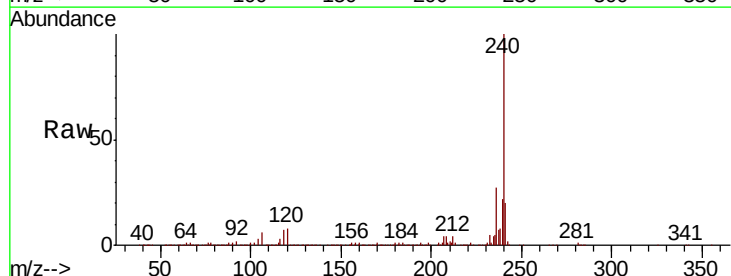


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

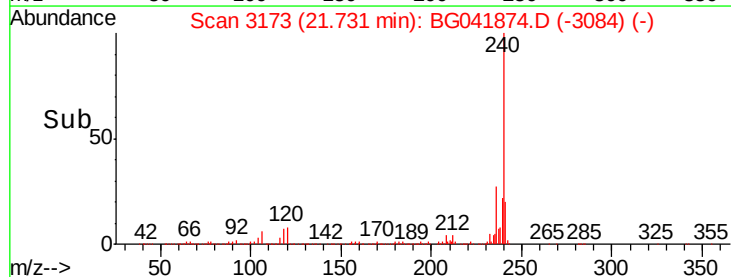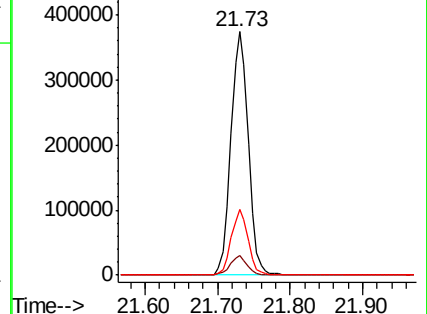

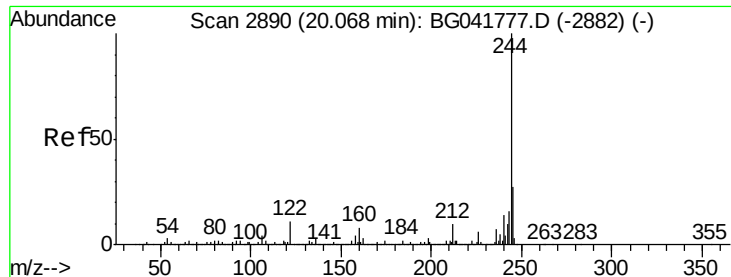

#79

Terphenyl-d14

Concen: 81.889 ng

RT: 20.06 min Scan# 2889

Delta R.T. -0.01 min

Lab File: BG041874.D

Acq: 1 Aug 2019 21:58

Instrument :

BNA_G

ClientSampleId :

TP-1


Tot Ion:244 Resp: 2226183

Ion Ratio Lower Upper




244 100

212 10.0 9.7 14.5

122 11.0 12.5 18.7#

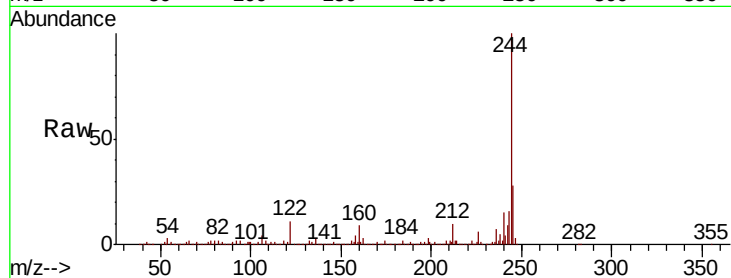

Abundance Ion 244.00 (243.70 to 244.70): E
2000000 Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

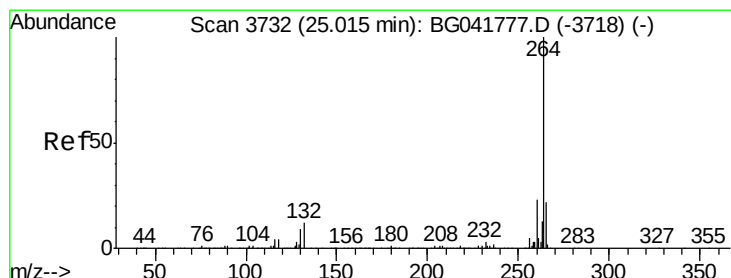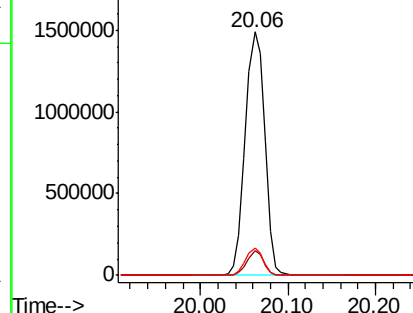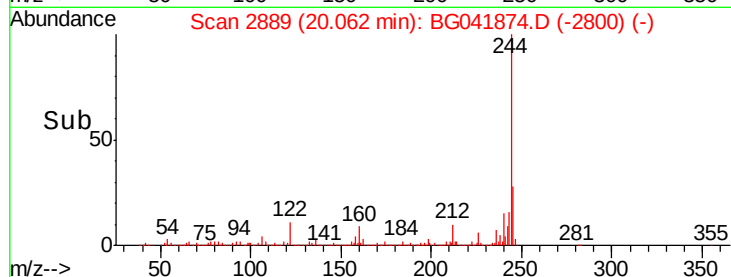

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.00 min Scan# 3730

Delta R.T. -0.01 min

Lab File: BG041874.D

Acq: 1 Aug 2019 21:58


Tgt Ion:264 Resp: 741892

Ion Ratio Lower Upper

264 100

260 23.3 19.5 29.3

265 22.7 18.0 27.0

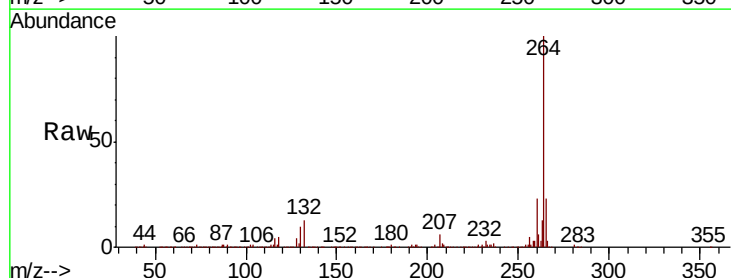

Abundance Ion 264.00 (263.70 to 264.70): E
300000 Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

