


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG080119\
 Data File : BG041864.D
 Acq On : 1 Aug 2019 15:33
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 31 08:57:26 2019

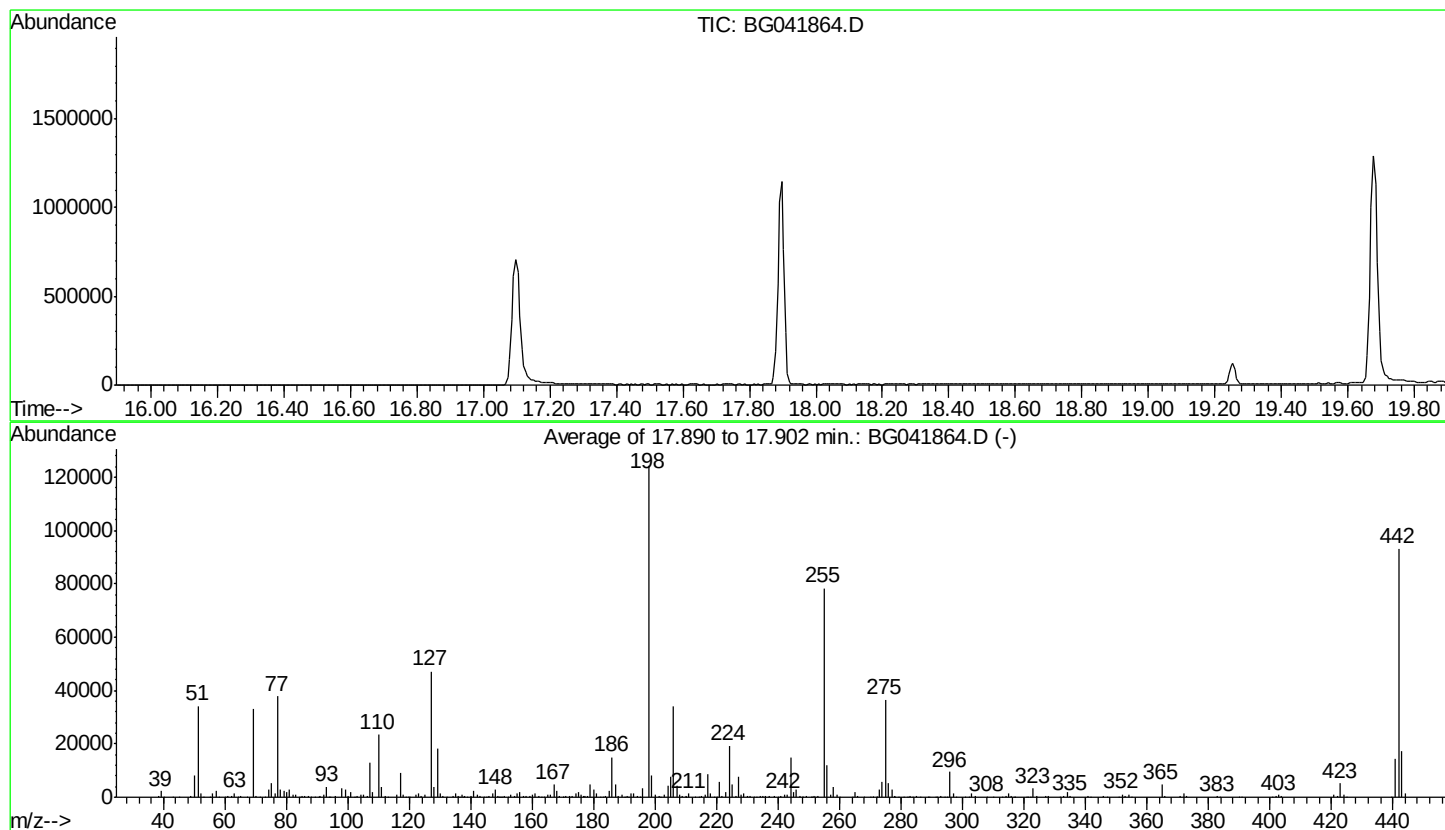

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	34112	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.6	33090	PASS
70	69	0.00	2	0.8	263	PASS
127	198	10	80	37.9	47042	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	124264	PASS
199	198	5	9	6.7	8318	PASS
275	198	10	60	29.5	36664	PASS
365	198	1	100	3.8	4751	PASS
441	198	0.01	100	11.4	14224	PASS
442	198	50	100	75.0	93208	PASS
443	442	15	24	18.6	17374	PASS