


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080122\
Data File : BG054458.D
Acq On : 1 Aug 2022 10:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 28 04:30:50 2022

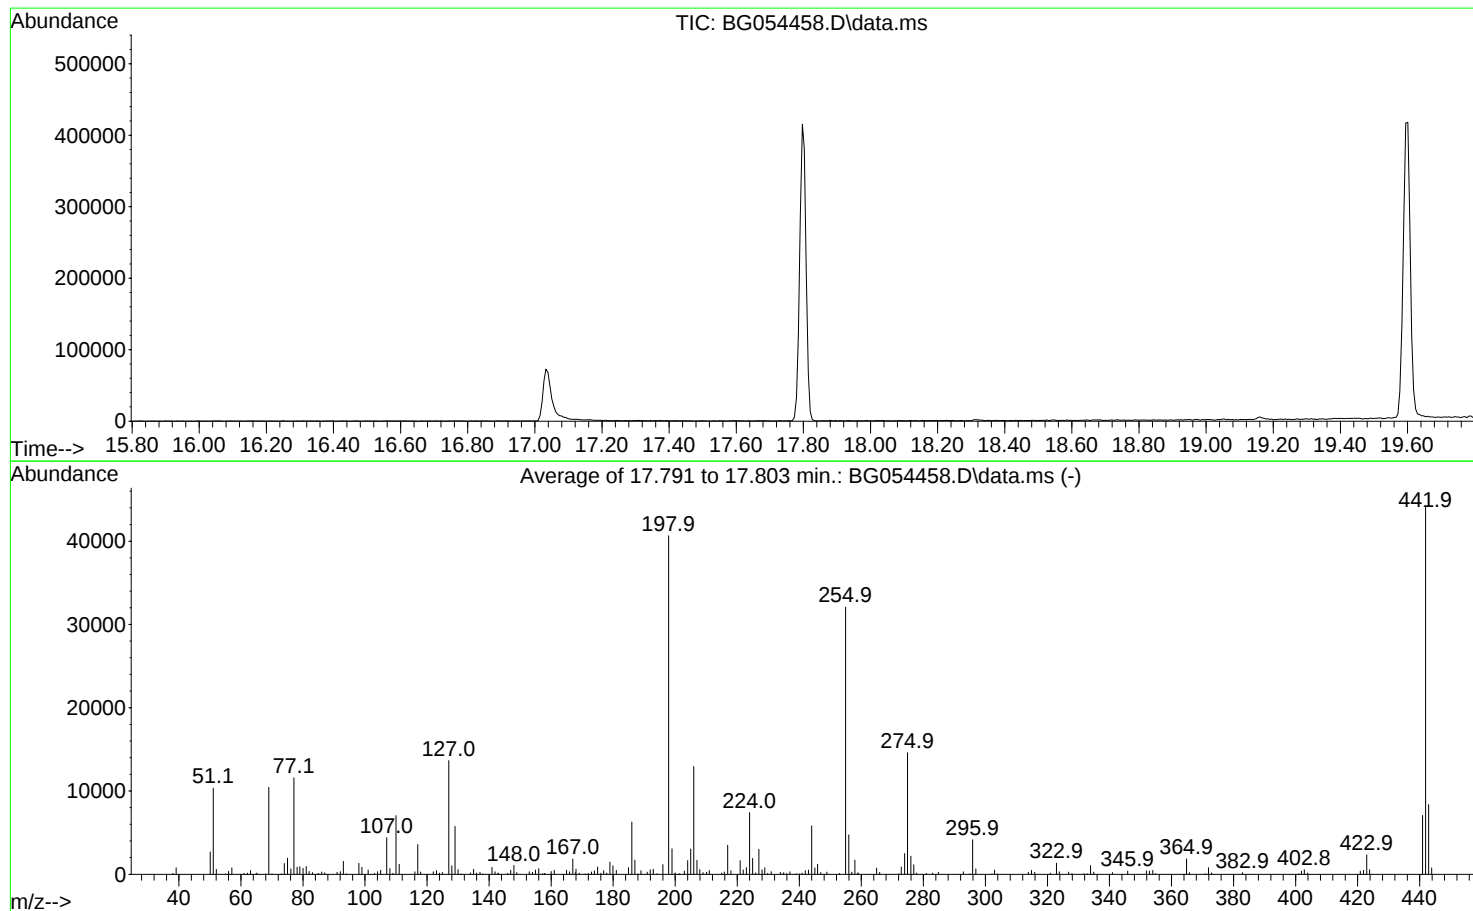




AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	10337	PASS
68	69	0.00	2	0.5	54	PASS
69	198	0.00	100	25.7	10441	PASS
70	69	0.00	2	0.5	56	PASS
127	198	10	80	33.6	13642	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40645	PASS
199	198	5	9	7.6	3074	PASS
275	198	10	60	35.9	14592	PASS
365	198	1	100	4.6	1860	PASS
441	198	0.01	100	17.4	7070	PASS
442	442	50	100	100.0	44171	PASS
443	442	15	24	18.9	8367	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080122\
Data File : BG054458.D
Acq On : 1 Aug 2022 10:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 01 11:00:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

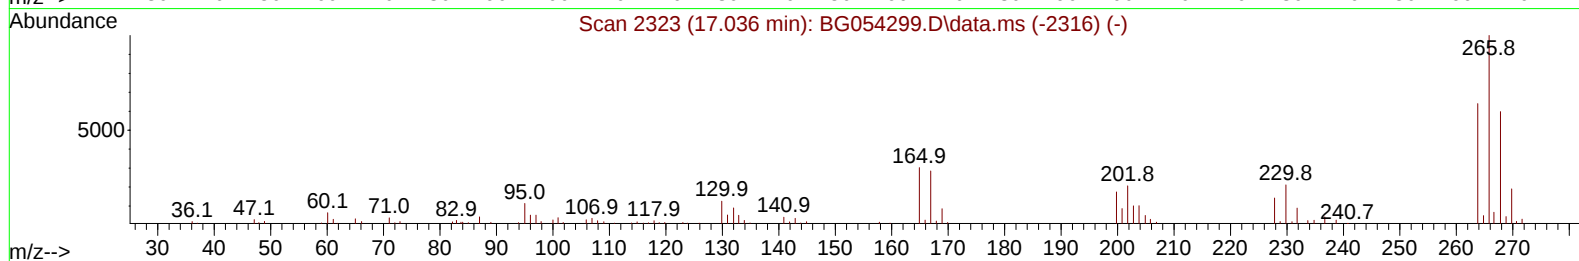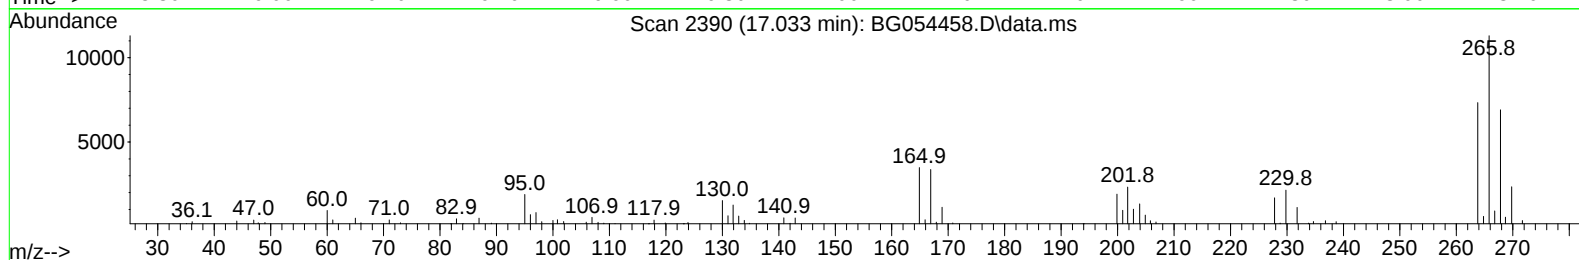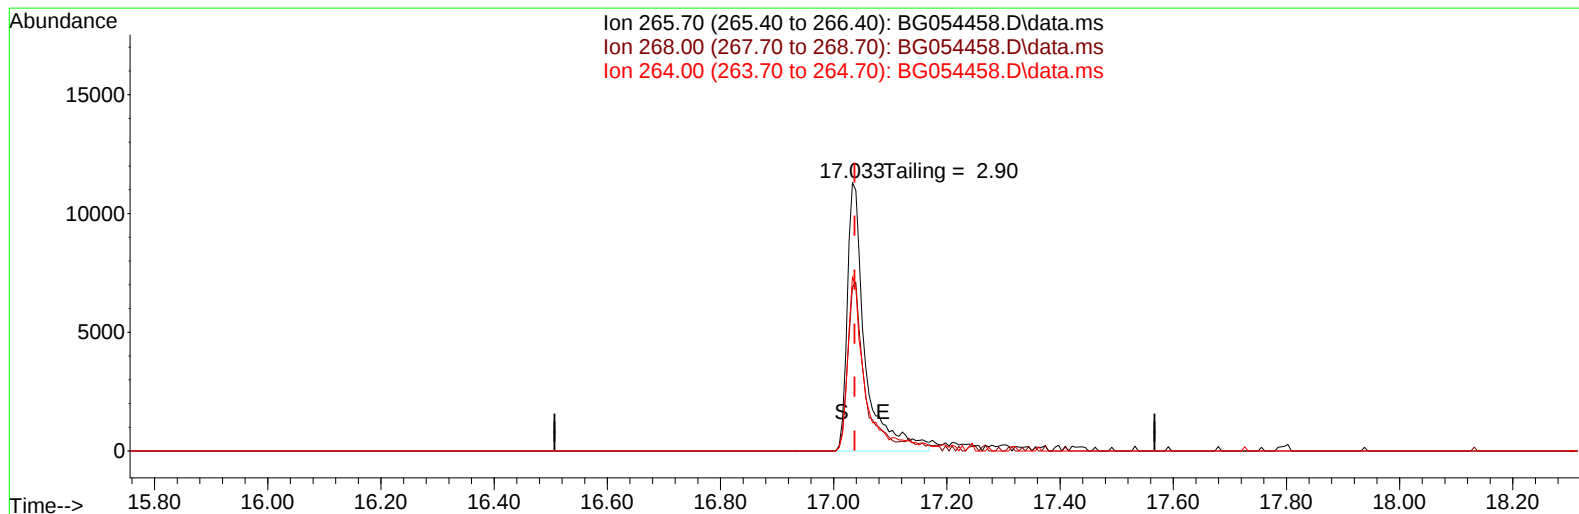

TIC: BG054458.D\data.ms

(70) Pentachlorophenol (C)

17.033min (-0.004) 60148.53 ng




response 23308

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.99
264.00	66.20	64.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080122\
Data File : BG054458.D
Acq On : 1 Aug 2022 10:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 01 11:00:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

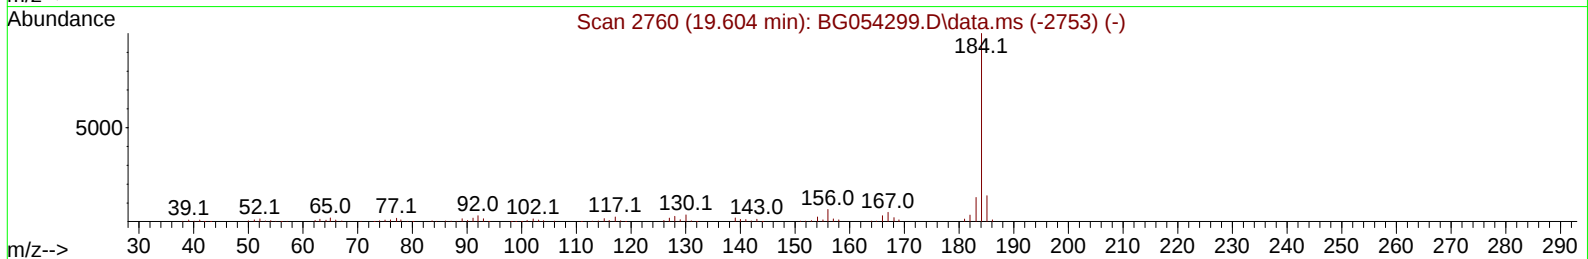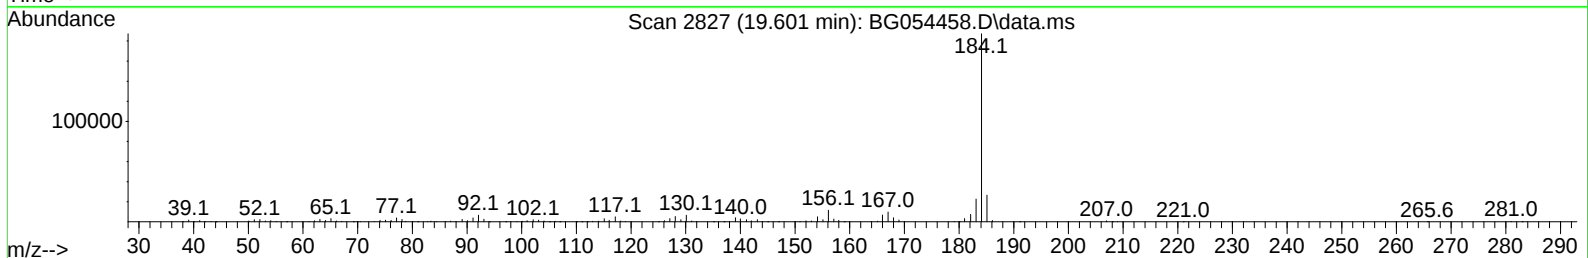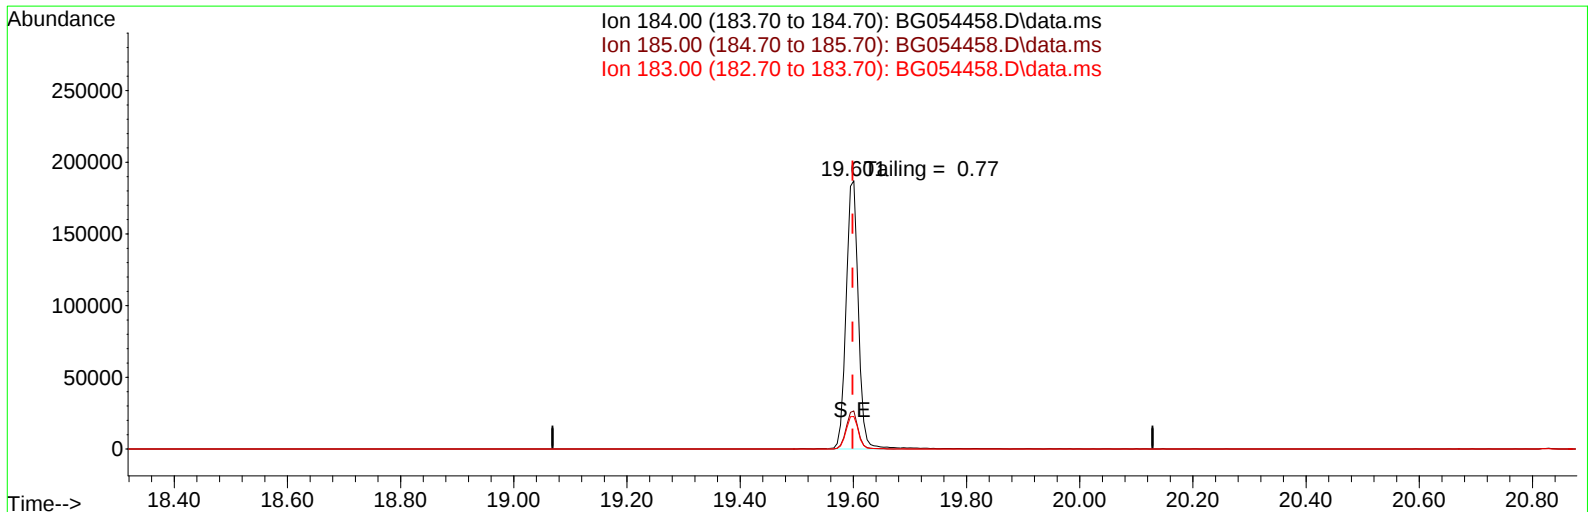

TIC: BG054458.D\data.ms

(77) Benzidine

19.601min (+ 0.002) 0.00 ng

response 280992

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.20
183.00	11.10	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/1/2022	BNA_G	BG054458.D
Compound Name	Response	Retention Time
DDT	152585	20.829
DDD	6279	20.394
DDE	303	19.889
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6582	159167	4.14

Instrument :
BNA_G
ClientSampleId :
DFTPP