
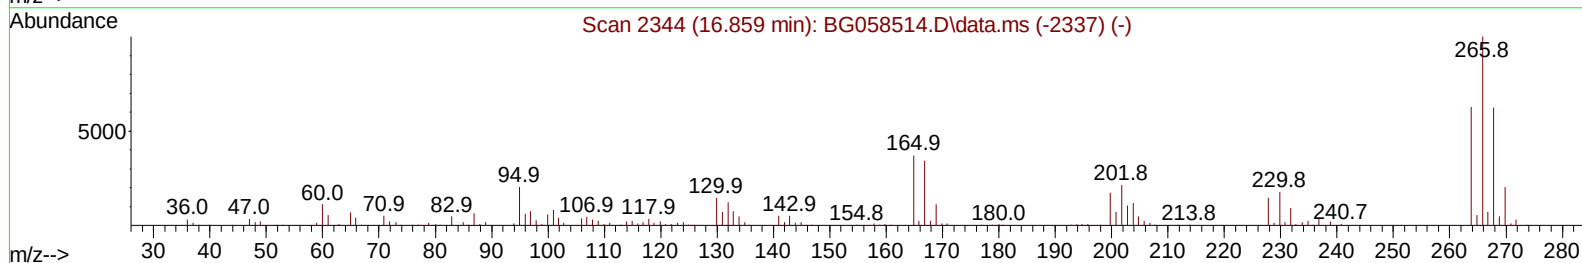
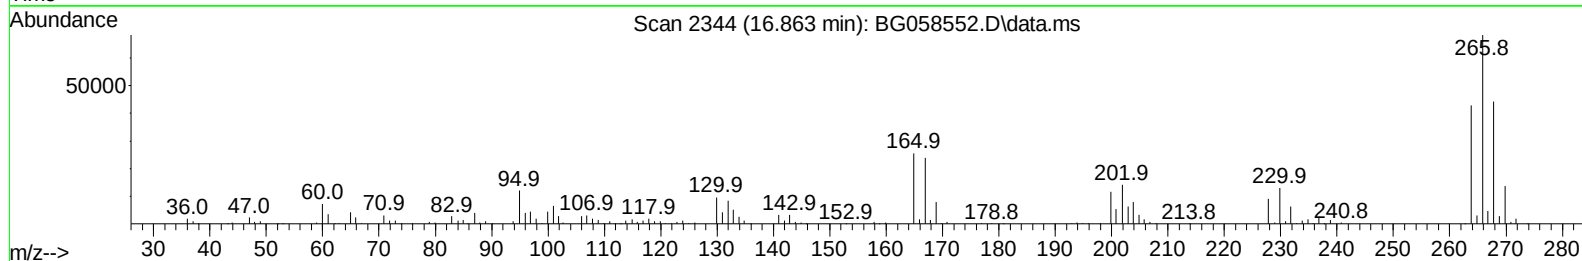


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080123\
Data File : BG058552.D
Acq On : 1 Aug 2023 6:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 18:42:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration



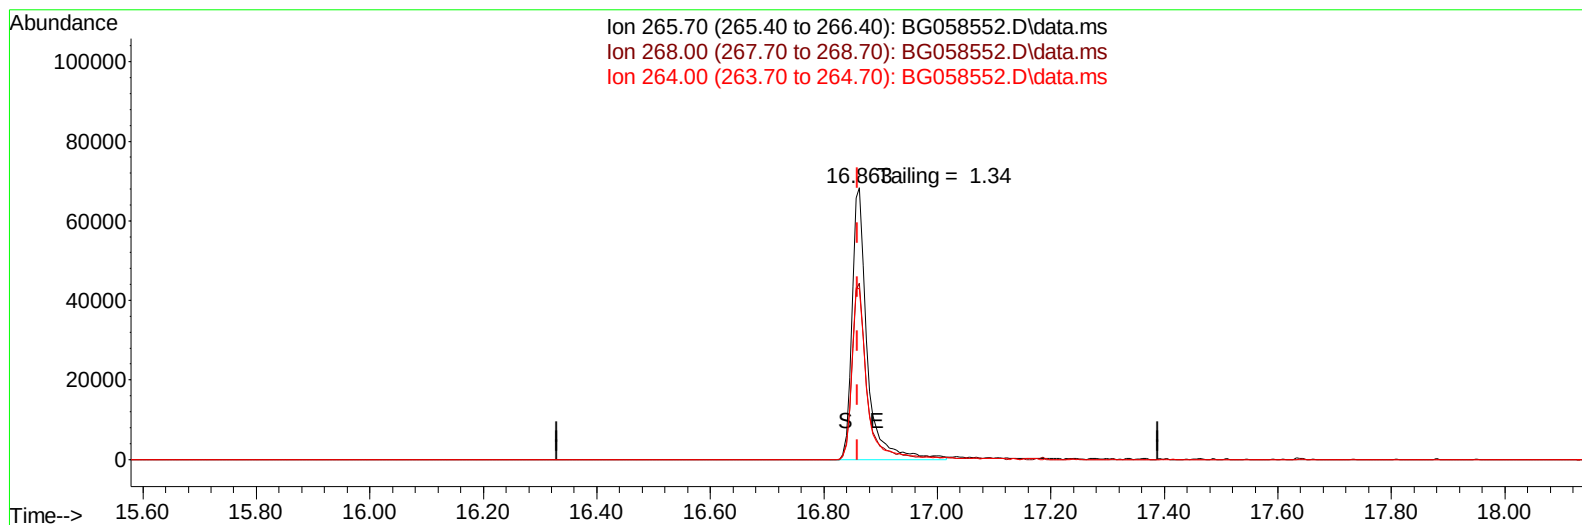


TIC: BG058552.D\data.ms

(70) Pentachlorophenol (C)**16.863min (+ 0.004) 26662.68 ng****response 124912**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.95
264.00	62.80	62.80
0.00	0.00	0.00

Quant Time: Aug 01 18:42:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

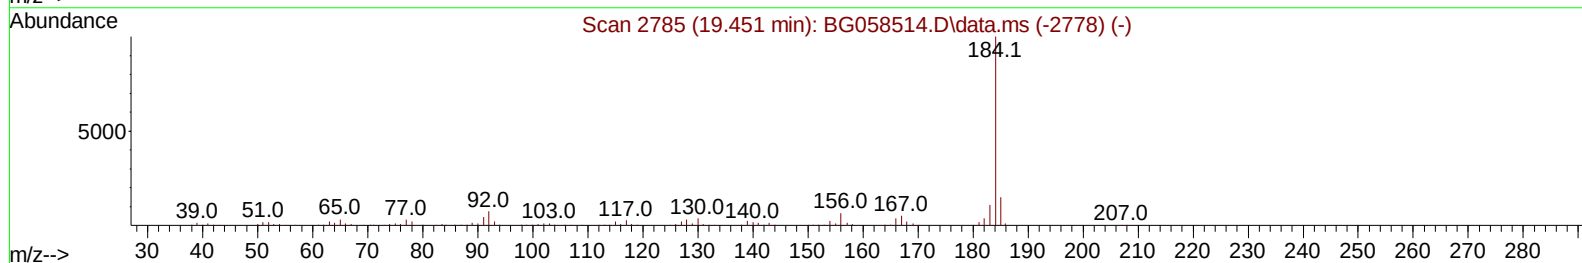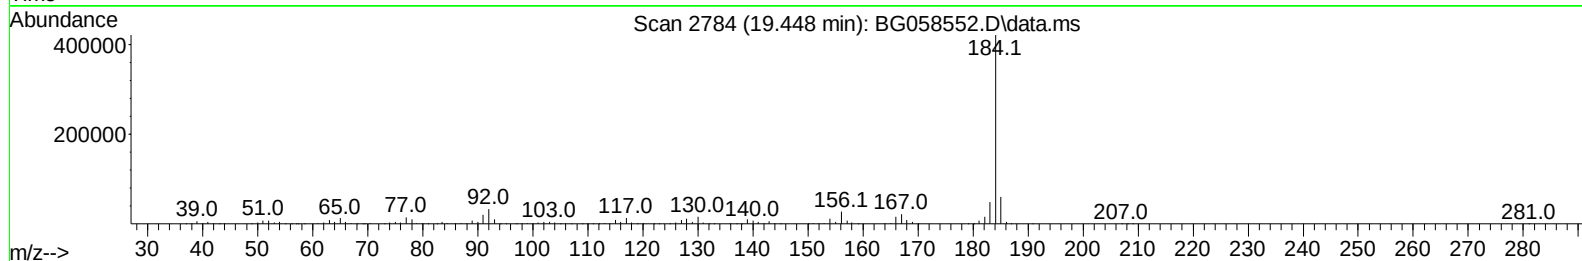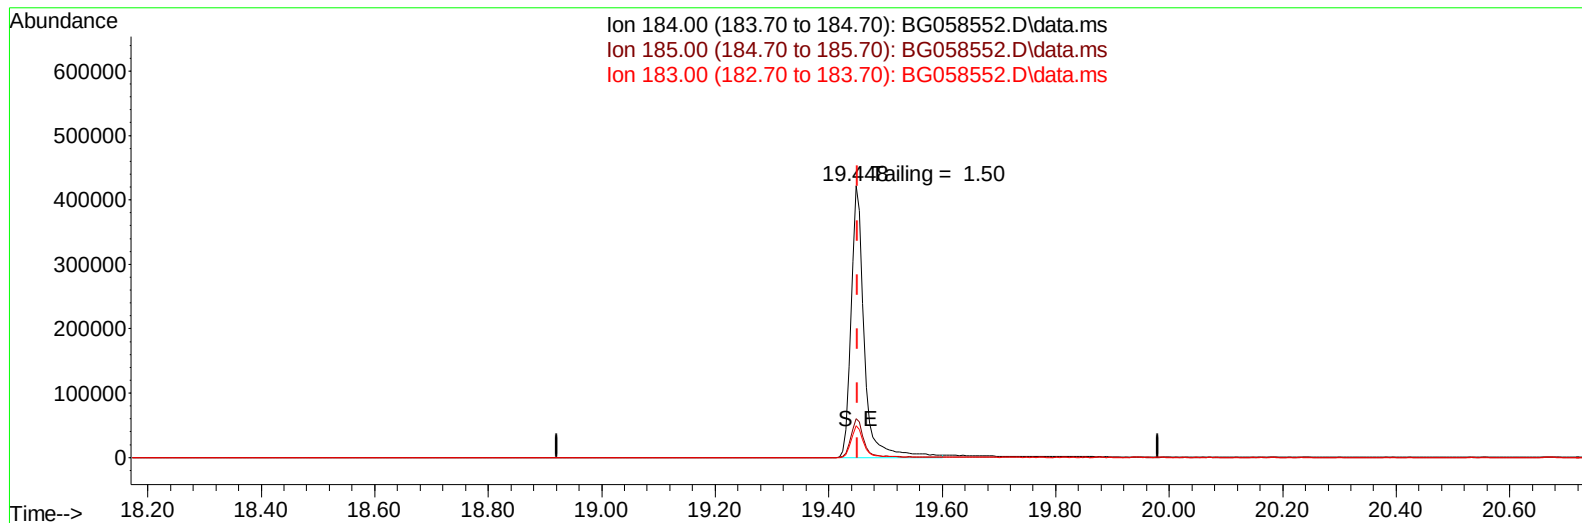

TIC: BG058552.D\data.ms

(77) Benzidine

19.448min (-0.002) 143339.20 ng

response **678164**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.24
183.00	10.90	11.66
0.00	0.00	0.00