
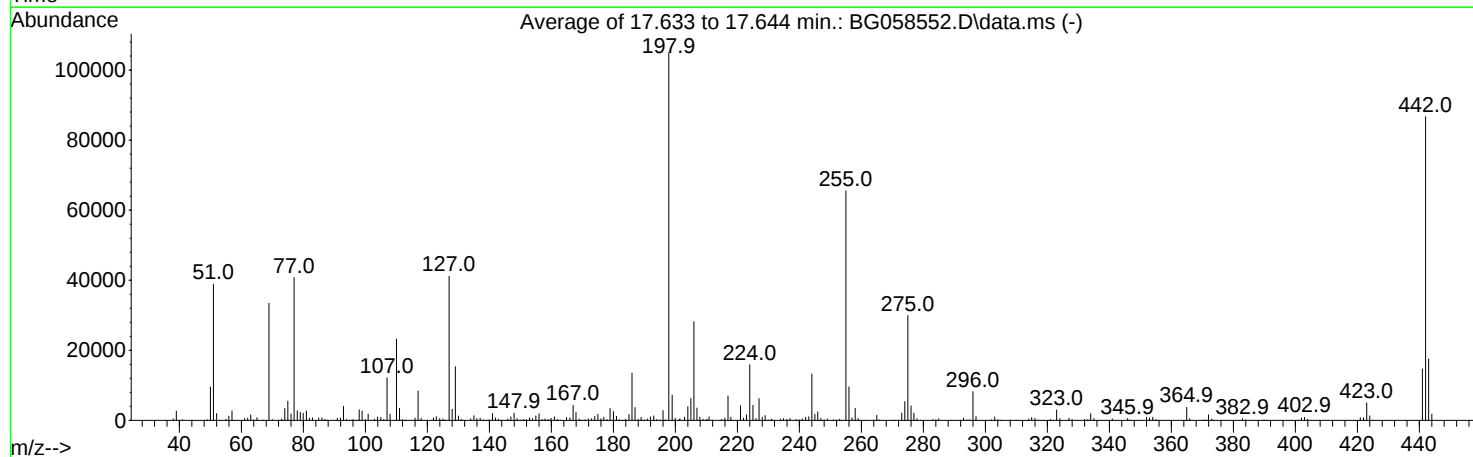


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080123\
Data File : BG058552.D
Acq On : 1 Aug 2023 6:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

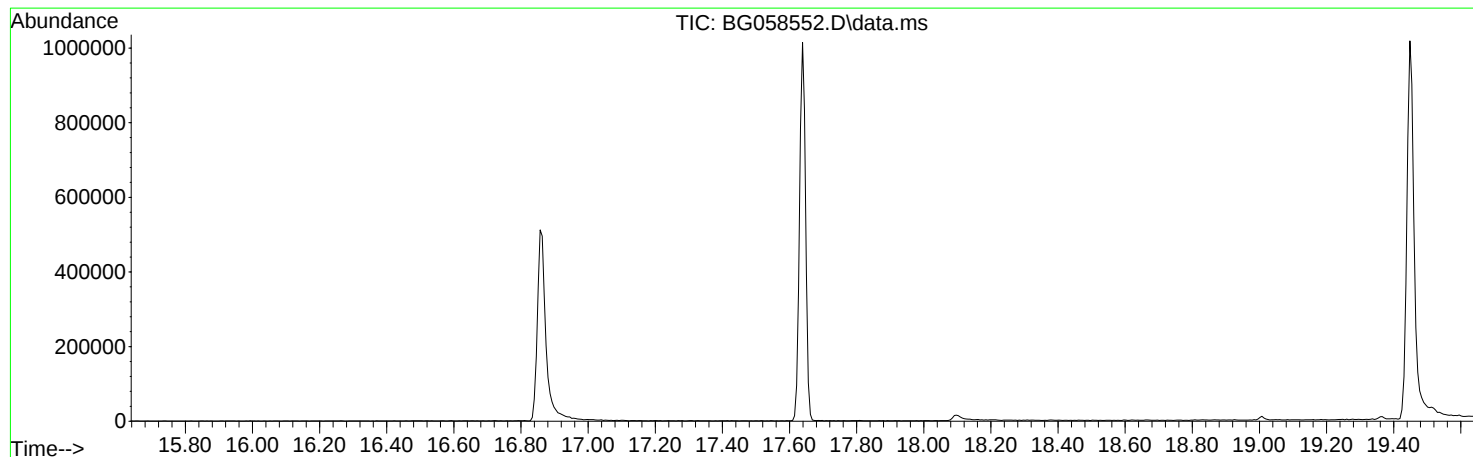

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	38891	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.8	33432	PASS
70	69	0.00	2	0.7	219	PASS
127	198	10	80	39.2	41155	PASS
197	198	0.00	2	0.2	176	PASS
198	198	100	100	100.0	105016	PASS
199	198	5	9	6.8	7178	PASS
275	198	10	60	28.5	29917	PASS
365	198	1	100	3.5	3713	PASS
441	198	0.01	100	14.0	14651	PASS
442	442	50	100	100.0	86715	PASS
443	442	15	24	20.2	17541	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/1/2023	BNA_G	<u>BG058552.D</u>
Compound Name	Response	Retention Time
DDT	267445	20.674
DDD	67697	20.239
DDE	756	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
68453	335898	20.38

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080123\
Data File : BG058552.D
Acq On : 1 Aug 2023 6:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 01 18:42:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

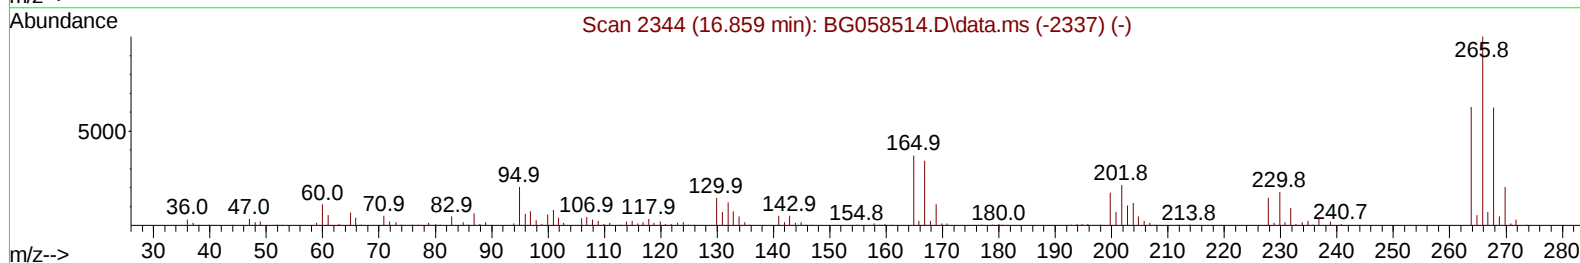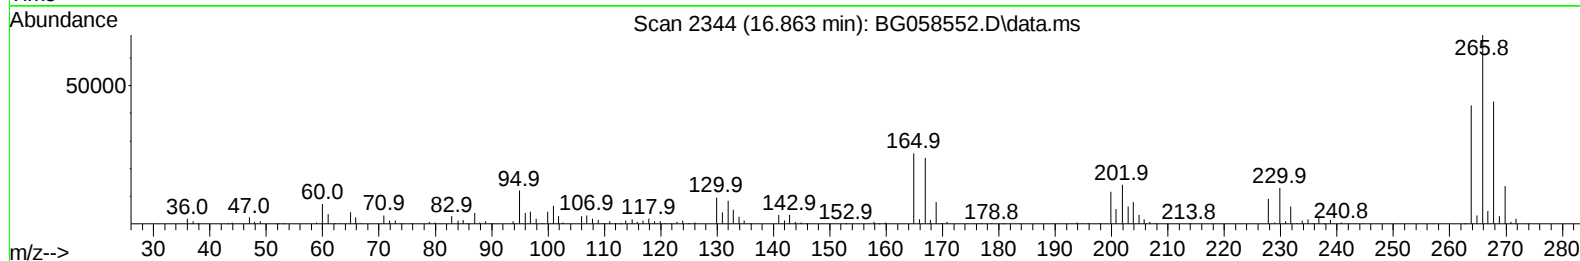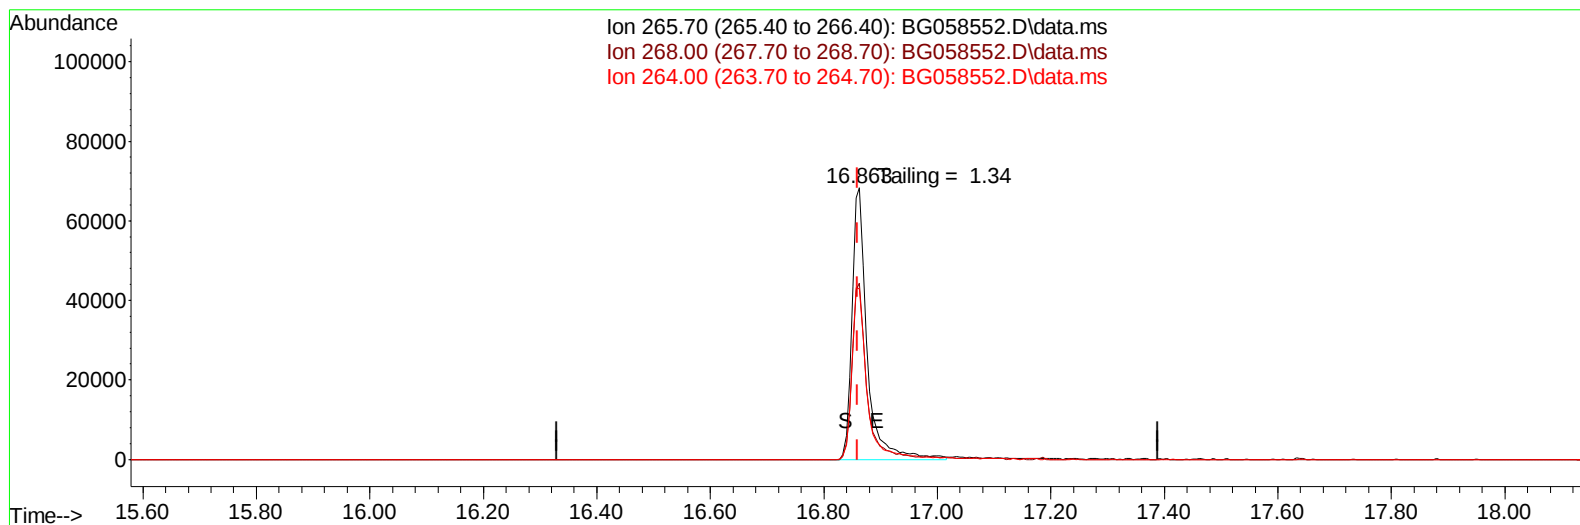

TIC: BG058552.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.004) 26662.68 ng




response 124912

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.95
264.00	62.80	62.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080123\
 Data File : BG058552.D
 Acq On : 1 Aug 2023 6:51
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 01 18:42:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 28 22:29:07 2023
 Response via : Initial Calibration

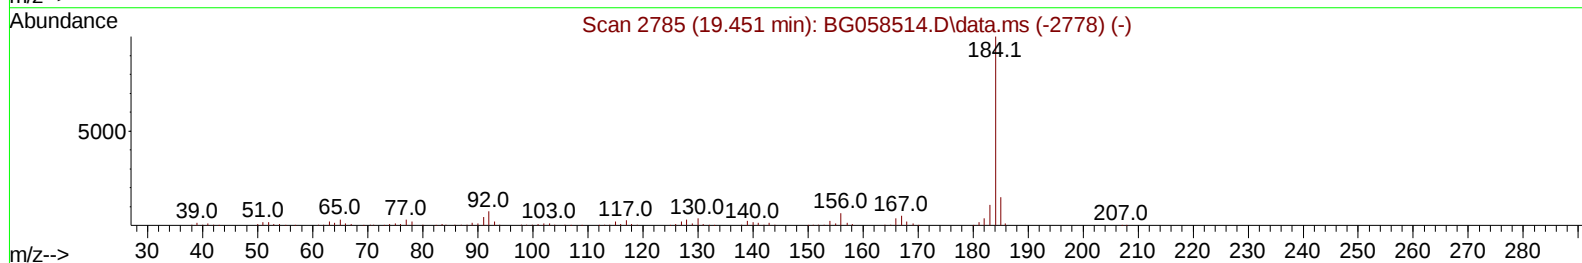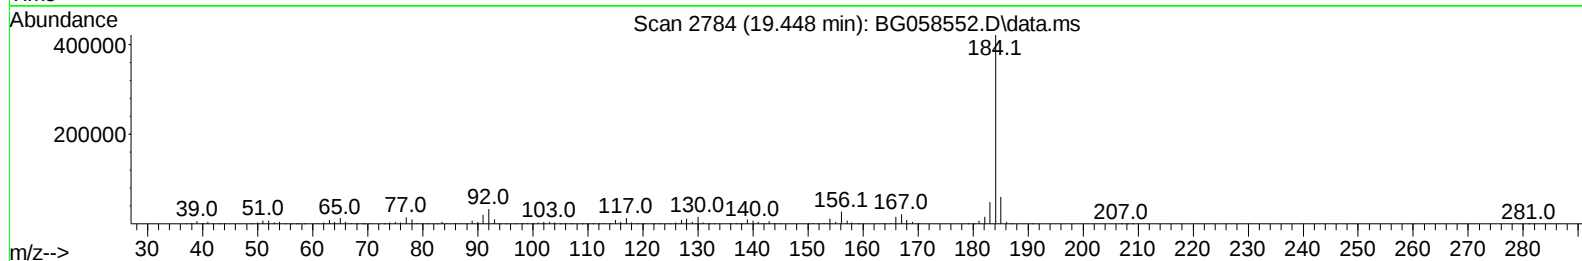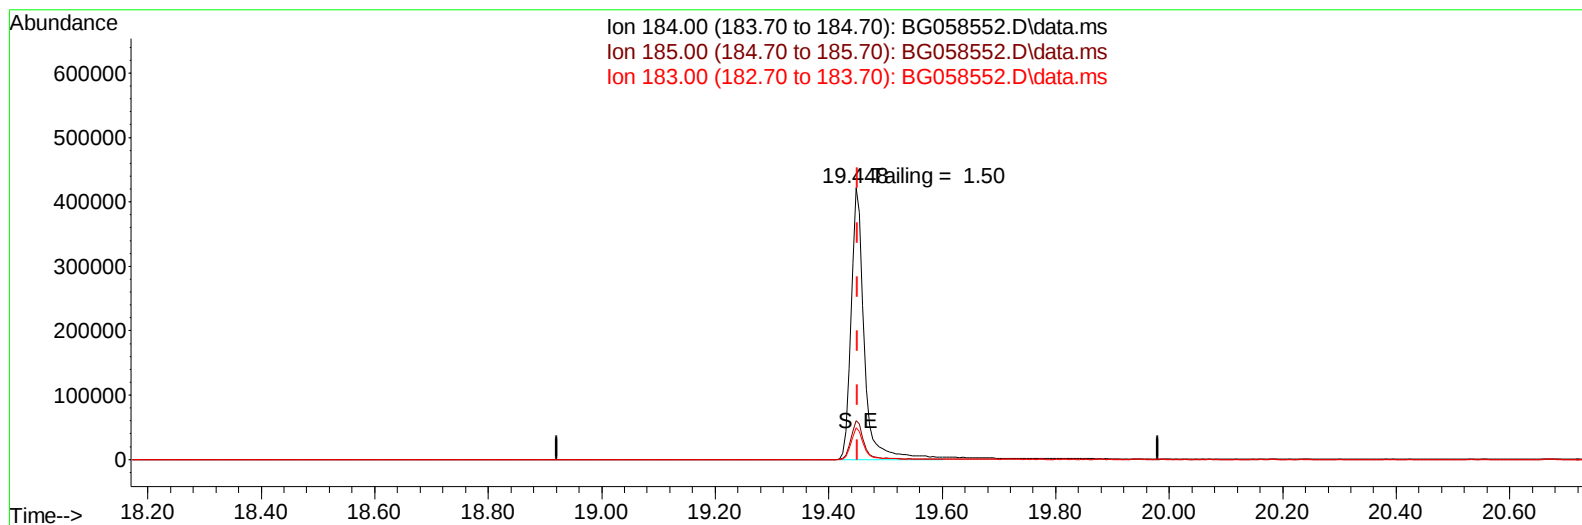

TIC: BG058552.D\data.ms

(77) Benzidine

19.448min (-0.002) 143339.20 ng

response 678164

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.24
183.00	10.90	11.66
0.00	0.00	0.00