
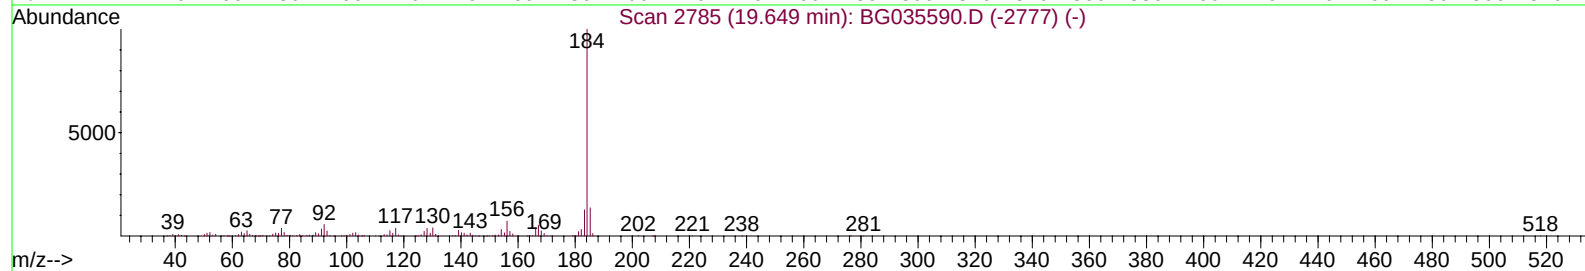
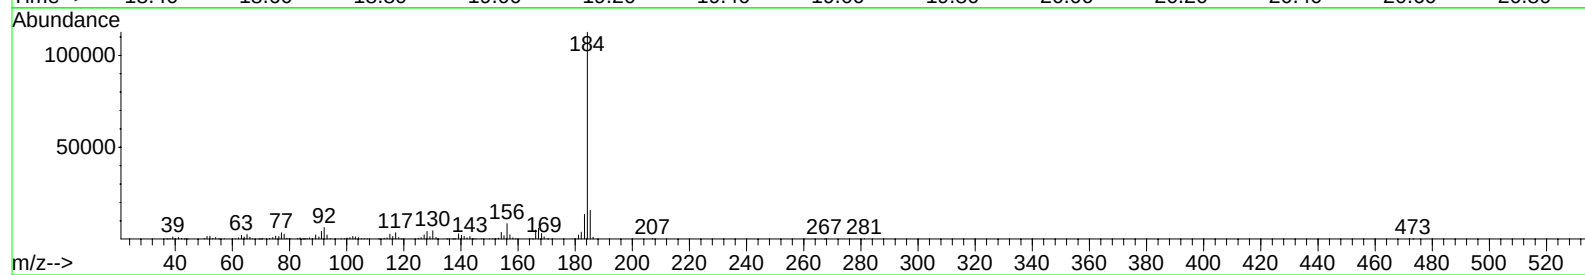


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080218\
Data File : BG036051.D
Acq On : 2 Aug 2018 8:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 11:57:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

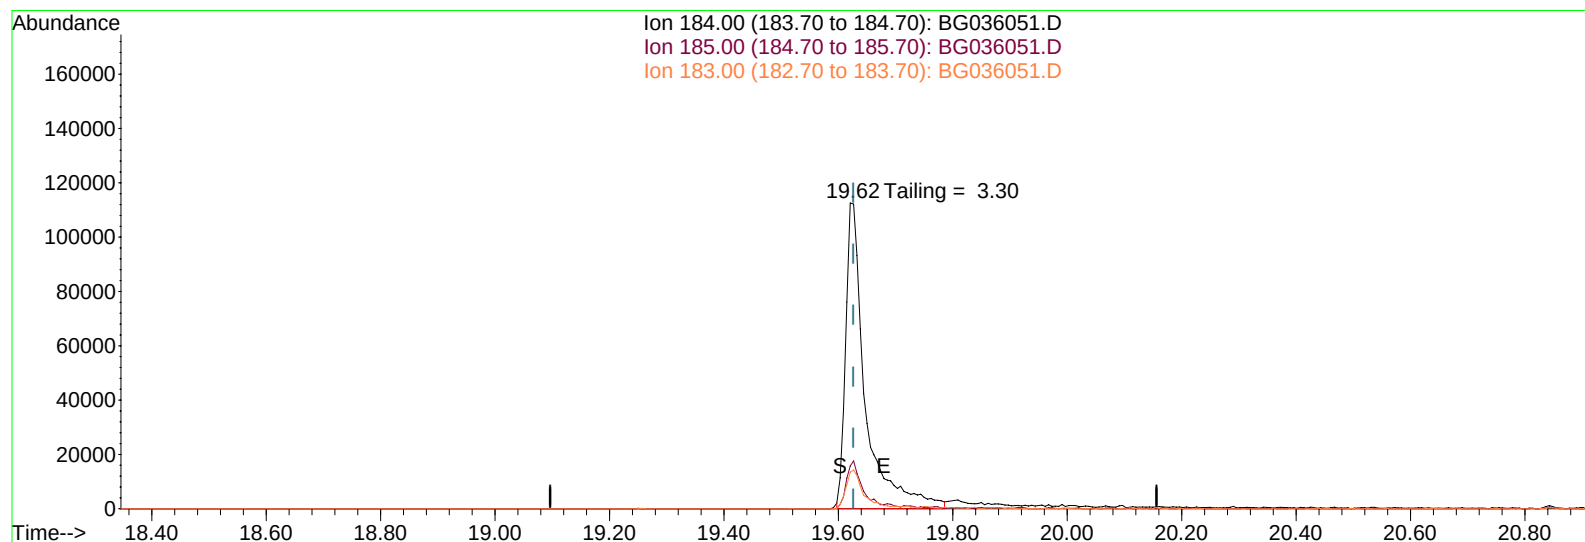

TIC: BG036051.D

(76) Benzidine




19.621min (-0.005) 124571.33ng

response 271826

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.97
183.00	13.30	11.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080218\
Data File : BG036051.D
Acq On : 2 Aug 2018 8:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 11:57:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

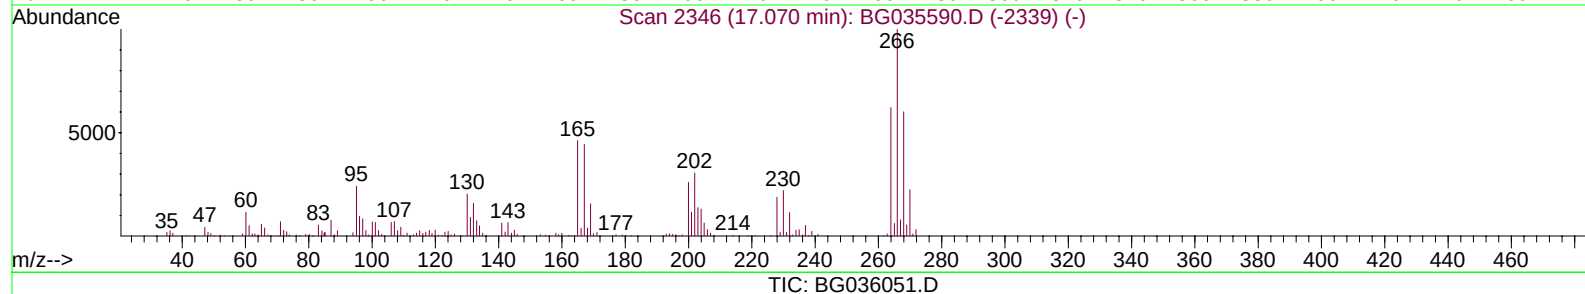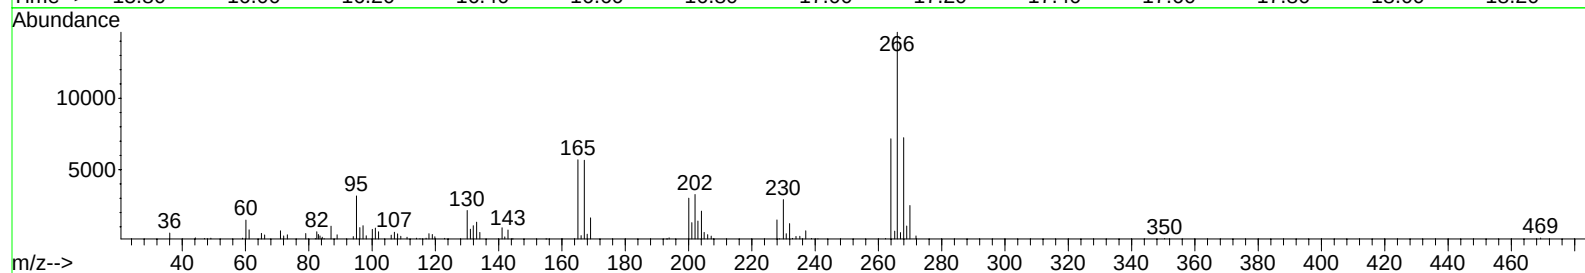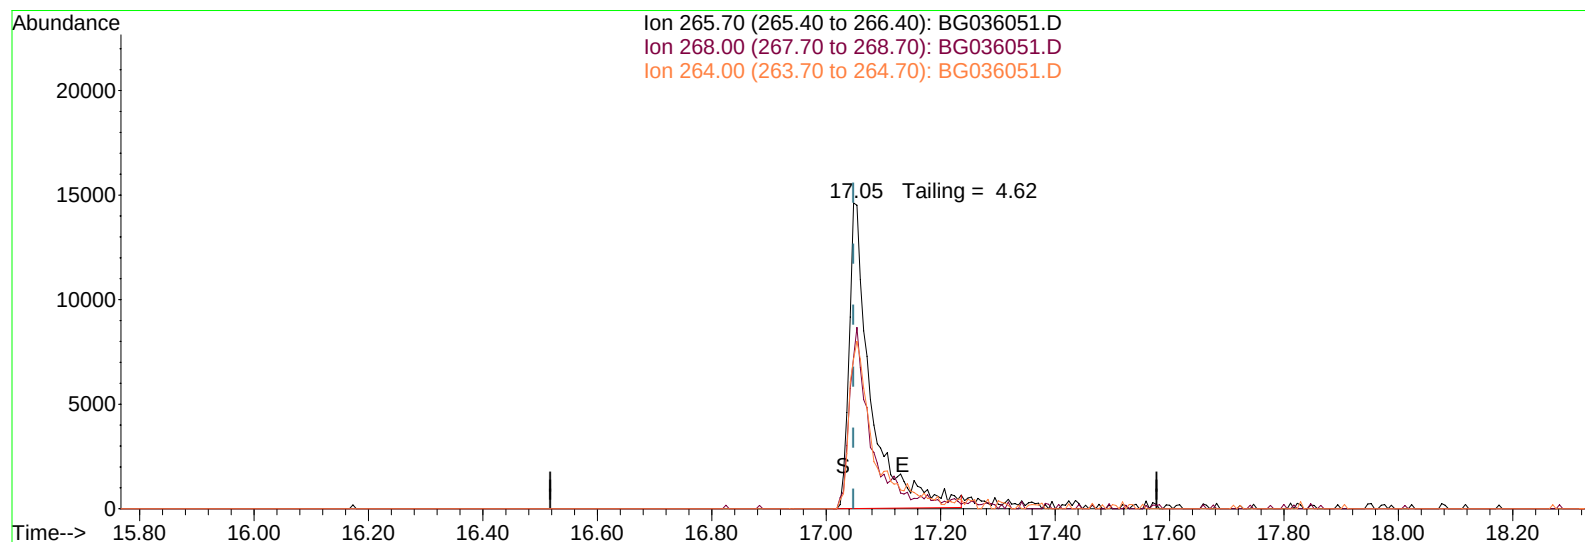

(69) Pentachlorophenol (C)

17.048min (+0.001) 33572.58ng

response 33471

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	49.56#
264.00	62.00	48.97#
0.00	0.00	0.00