
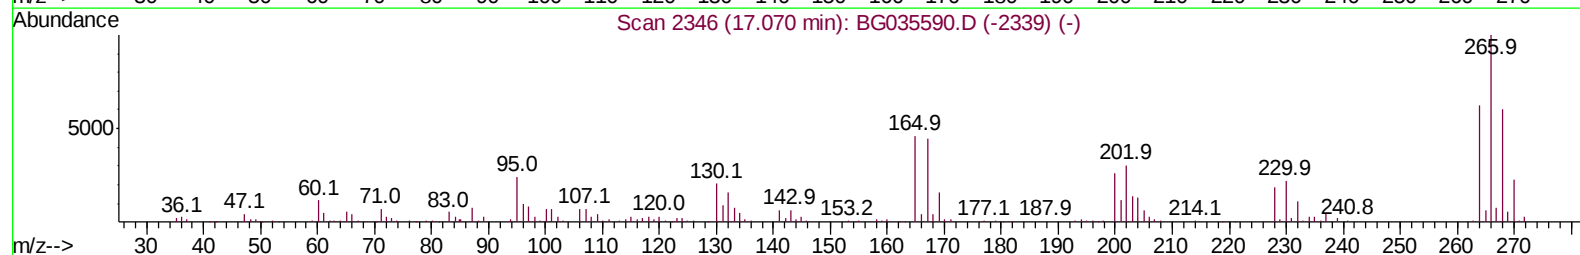
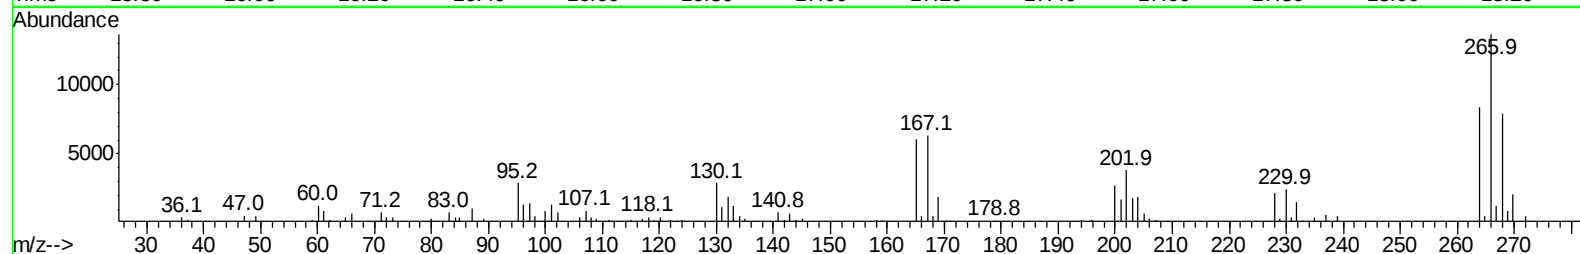


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080218\
Data File : BG036069.D
Acq On : 2 Aug 2018 22:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 23:15:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

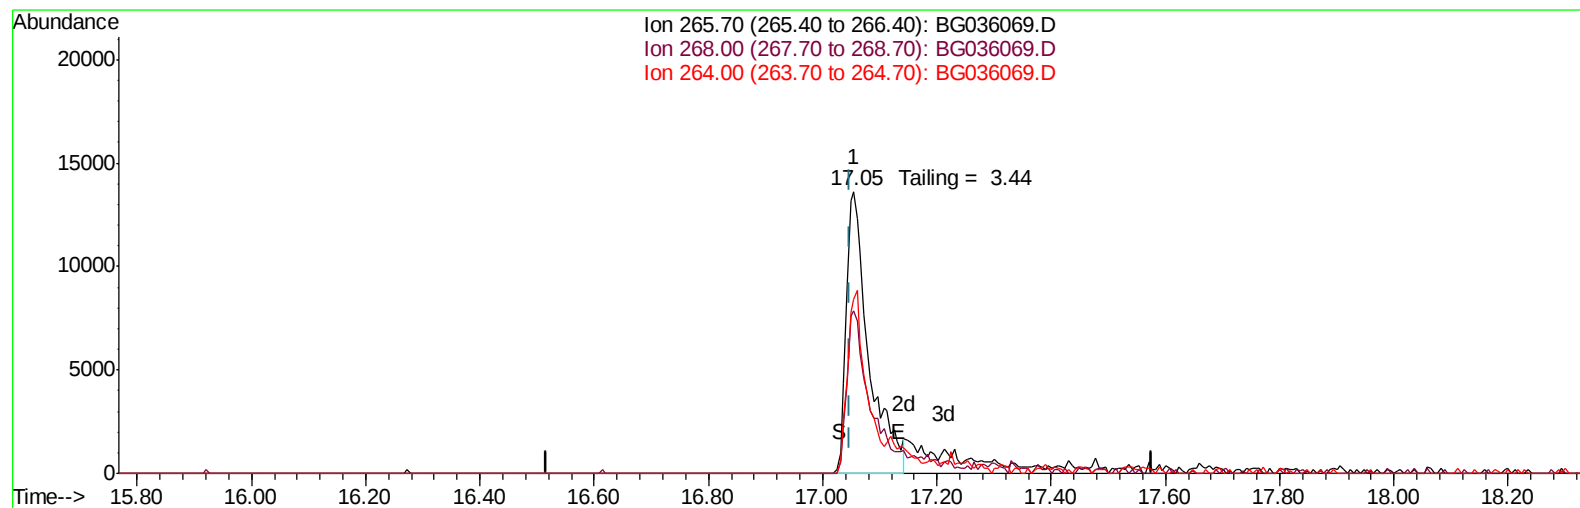

TIC: BG036069.D

(69) Pentachlorophenol (C)




17.054min (+0.007) 51997.85ng

response 37083

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.76
264.00	62.00	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080218\
Data File : BG036069.D
Acq On : 2 Aug 2018 22:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 23:15:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

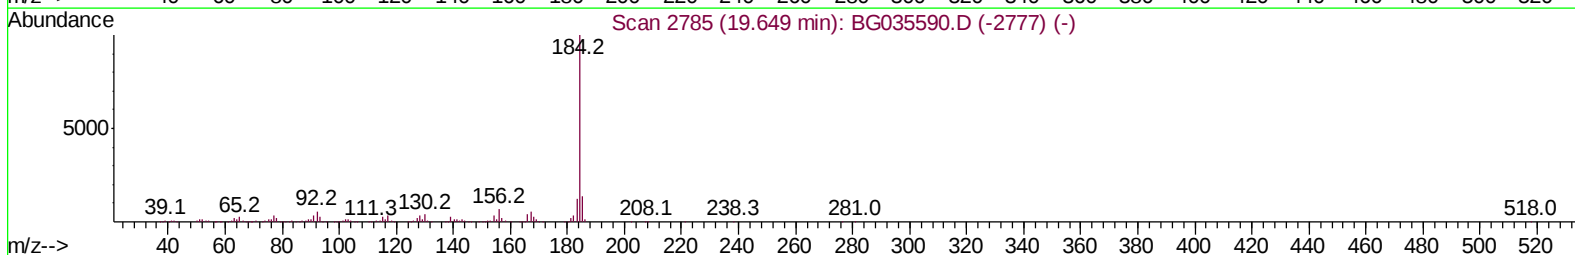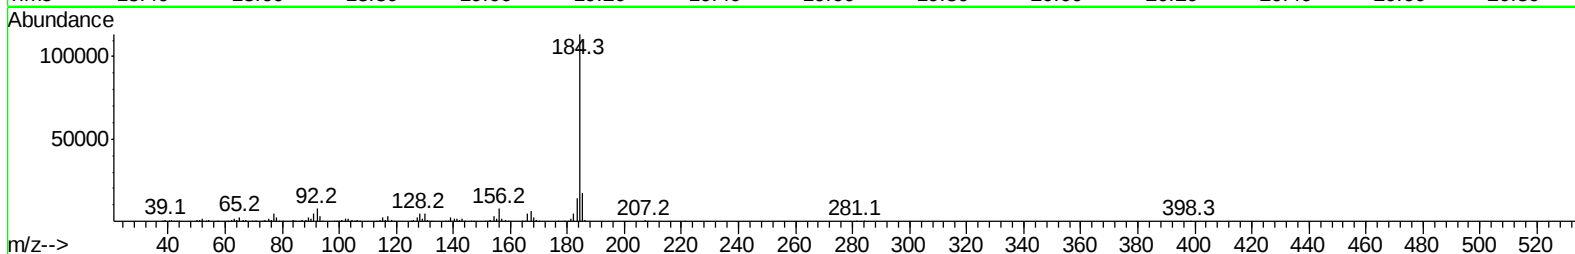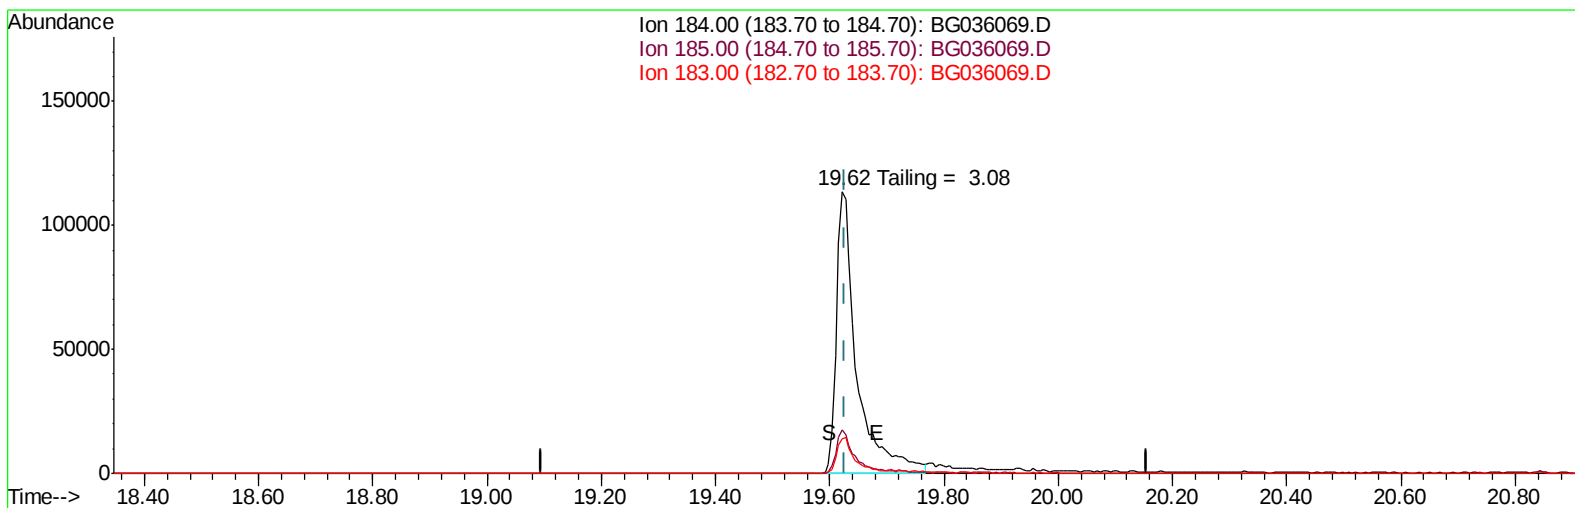

TIC: BG036069.D

(76) Benzidine

19.621min (-0.005) 33206.57ng

response 281109

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.25
183.00	13.30	12.37
0.00	0.00	0.00