

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080223\
Data File : BG058570.D
Acq On : 2 Aug 2023 9:14
Operator : MA/JU
Sample : PB154374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154374BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG058570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	385	392	402	rBV	868480	1377285	35.81%	9.659%
2	6.989	656	664	679	rBV	805666	1354968	35.23%	9.502%
3	7.811	797	804	813	rBV	136483	232618	6.05%	1.631%
4	8.981	995	1003	1018	rBV	443550	806501	20.97%	5.656%
5	10.620	1272	1282	1296	rBV	170359	336141	8.74%	2.357%
6	13.082	1694	1701	1718	rBV	1135734	1816290	47.22%	12.738%
7	14.462	1929	1936	1952	rBV	278859	461313	11.99%	3.235%
8	15.955	2183	2190	2206	rBV	932897	1530618	39.79%	10.734%
9	17.206	2397	2403	2419	rBV	382848	635298	16.52%	4.455%
10	19.833	2843	2850	2860	rBV	2710468	3846451	100.00%	26.975%
11	21.454	3119	3126	3136	rBV	515530	867716	22.56%	6.085%
12	24.527	3638	3649	3663	rBV	345869	994109	25.84%	6.972%




Sum of corrected areas: 14259308

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080223\
Data File : BG058570.D
Acq On : 2 Aug 2023 9:14
Operator : MA/JU
Sample : PB154374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154374BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

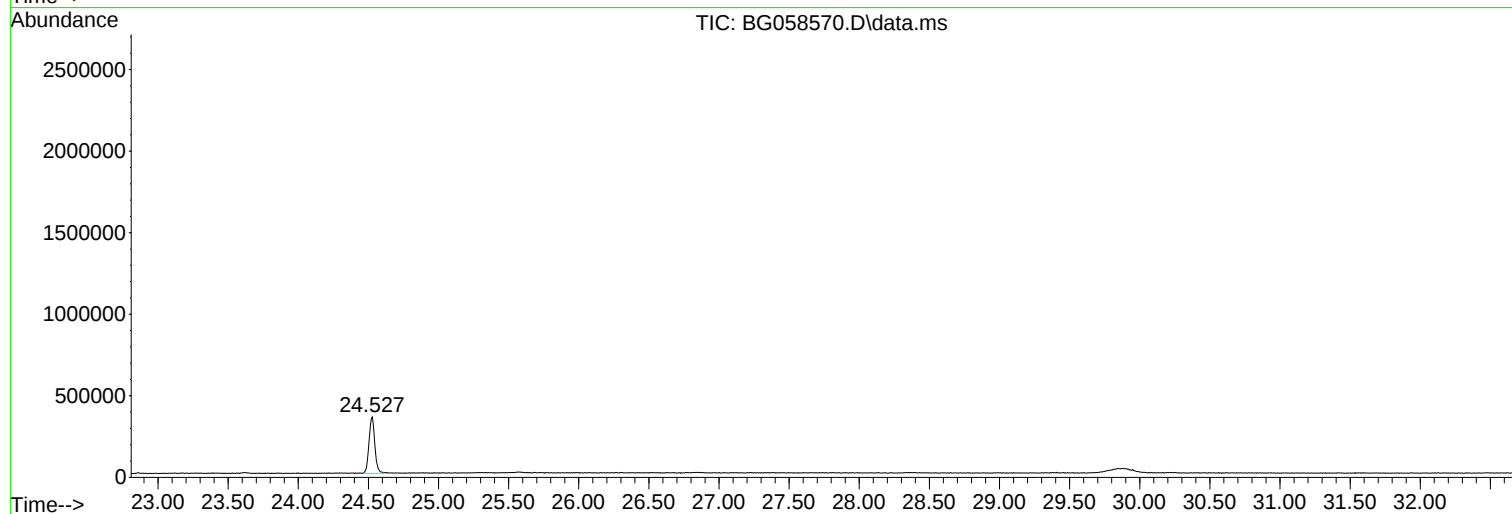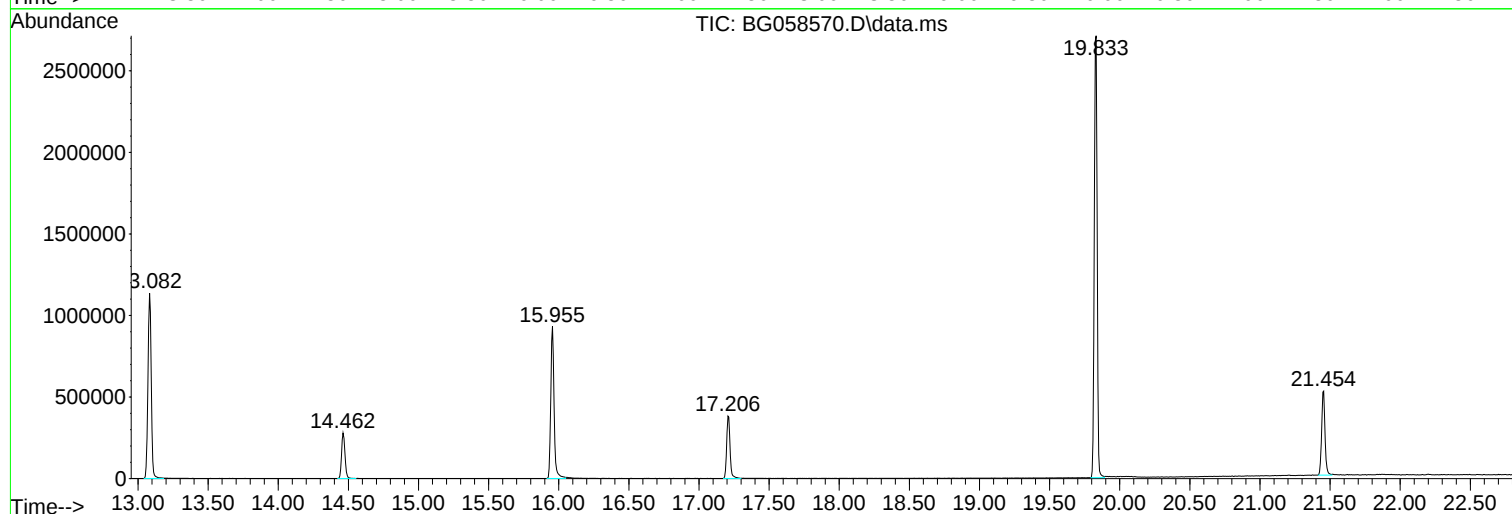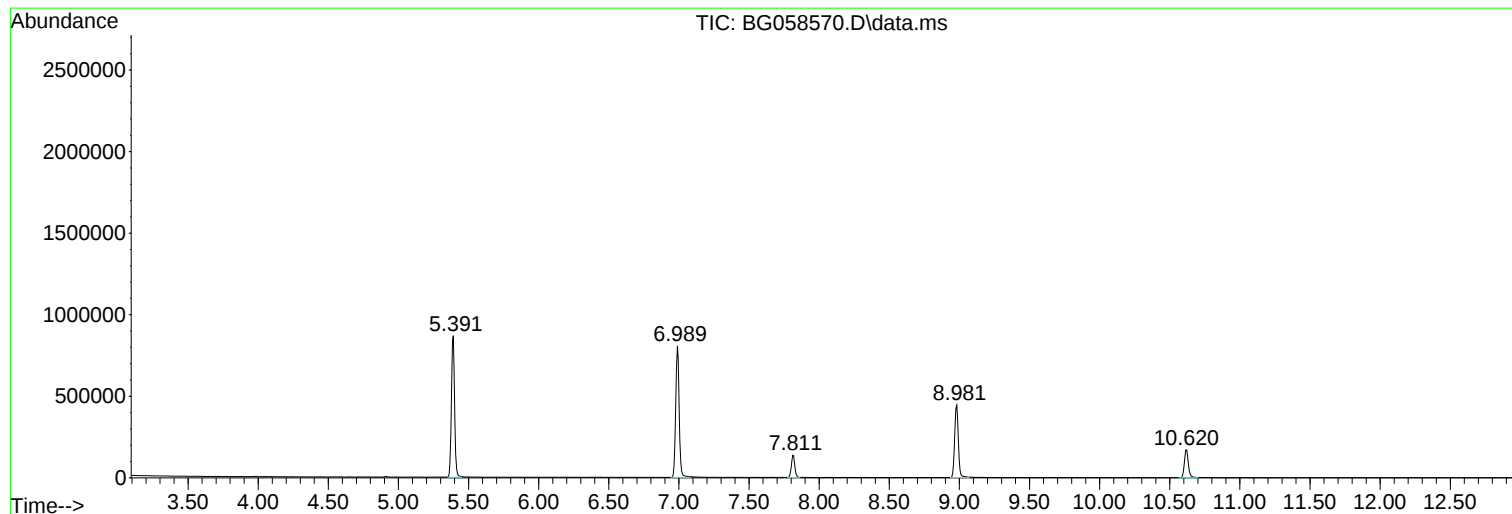

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080223\
Data File : BG058570.D
Acq On : 2 Aug 2023 9:14
Operator : MA/JU
Sample : PB154374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154374BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080223\
Data File : BG058570.D
Acq On : 2 Aug 2023 9:14
Operator : MA/JU
Sample : PB154374BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154374BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------