

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080323\
 Data File : BG058586.D
 Acq On : 3 Aug 2023 9:59
 Operator : MA/JU
 Sample : PB154586BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB154586BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG058586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	384	391	407	rBV	962980	1491506	40.68%	10.070%
2	6.984	655	663	677	rBV	852660	1485617	40.52%	10.030%
3	7.812	796	804	815	rBV	153310	261604	7.14%	1.766%
4	8.975	994	1002	1020	rBV	494264	889840	24.27%	6.008%
5	10.615	1274	1281	1296	rBV	189792	363657	9.92%	2.455%
6	13.082	1694	1701	1718	rBV	1212164	1972503	53.80%	13.317%
7	14.457	1929	1935	1945	rBV	310736	518626	14.15%	3.501%
8	15.950	2183	2189	2208	rBV	1040374	1684528	45.95%	11.373%
9	17.207	2396	2403	2418	rBV	441245	695669	18.98%	4.697%
10	19.827	2843	2849	2859	rBV	2723550	3666062	100.00%	24.751%
11	21.449	3118	3125	3136	rBV2	481115	840347	22.92%	5.674%
12	24.516	3637	3647	3668	rVB2	328924	941813	25.69%	6.359%




Sum of corrected areas: 14811772

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080323\
Data File : BG058586.D
Acq On : 3 Aug 2023 9:59
Operator : MA/JU
Sample : PB154586BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154586BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

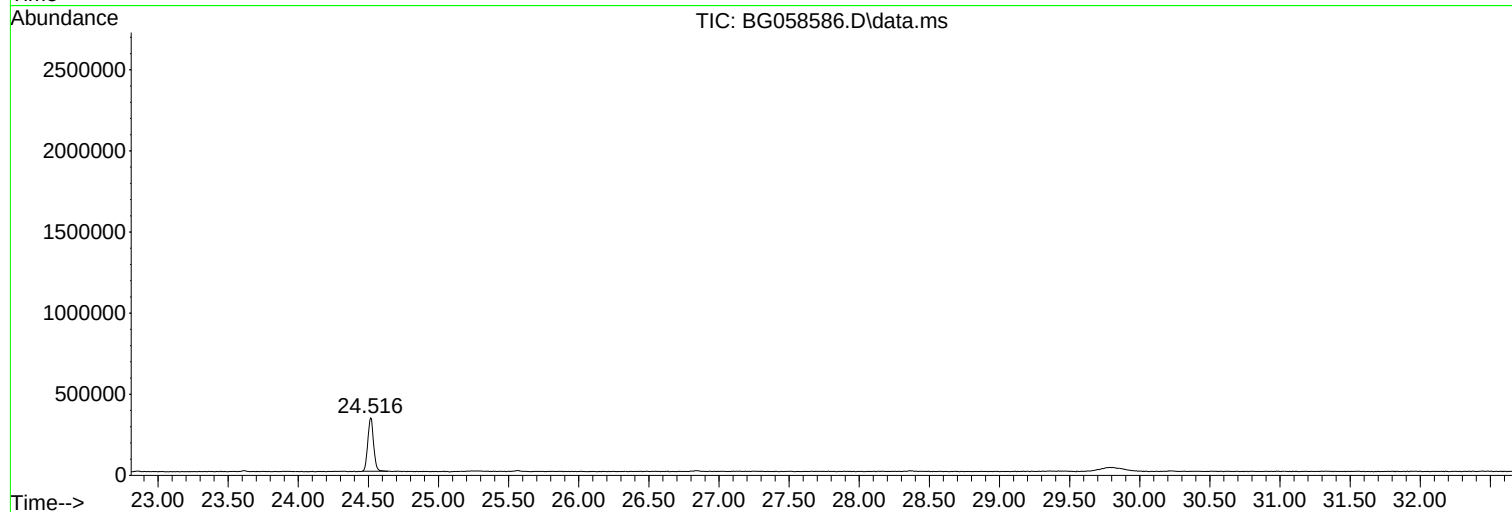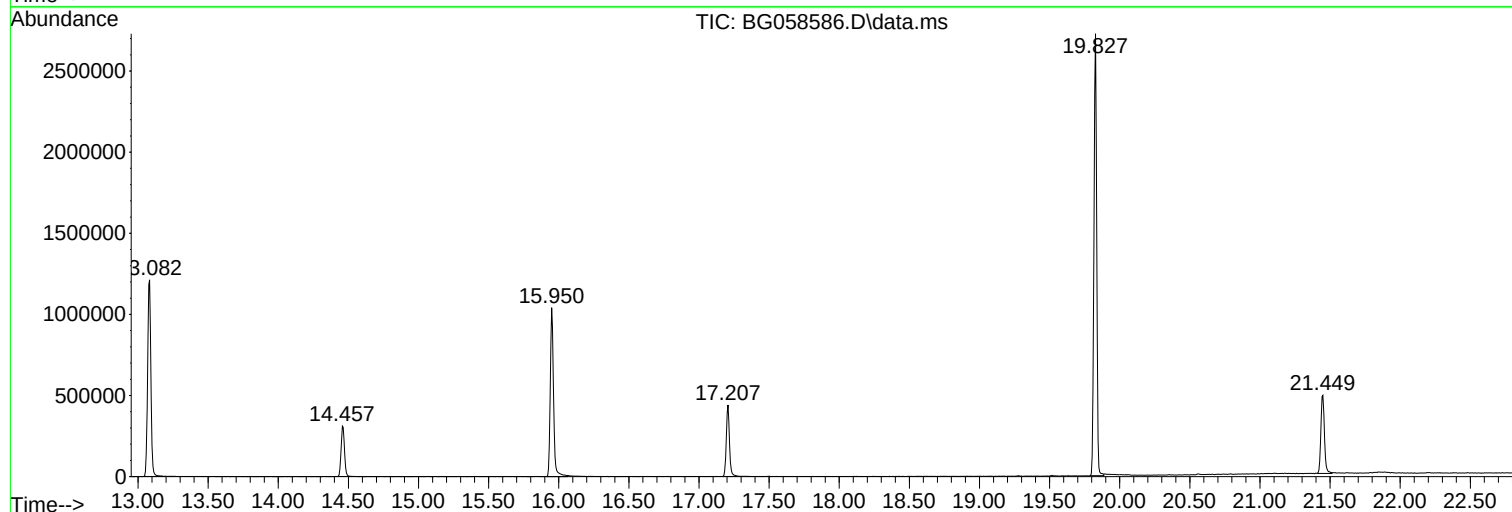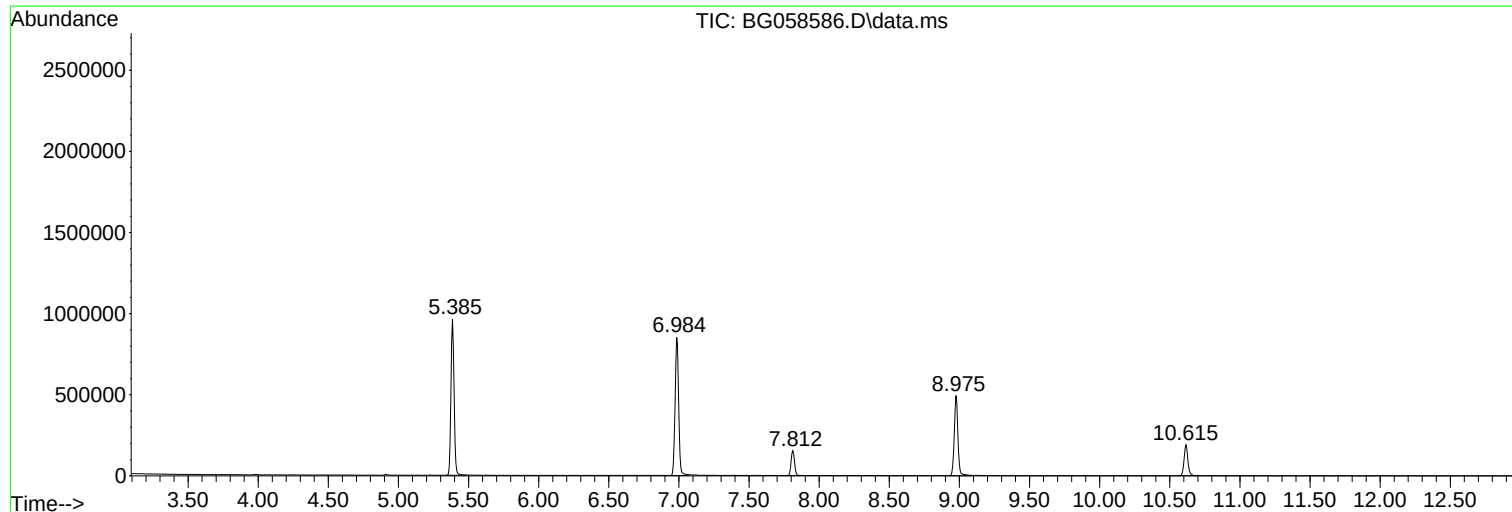

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080323\
Data File : BG058586.D
Acq On : 3 Aug 2023 9:59
Operator : MA/JU
Sample : PB154586BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154586BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080323\
Data File : BG058586.D
Acq On : 3 Aug 2023 9:59
Operator : MA/JU
Sample : PB154586BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154586BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------