


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080323\
Data File : BG058584.D
Acq On : 3 Aug 2023 8:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

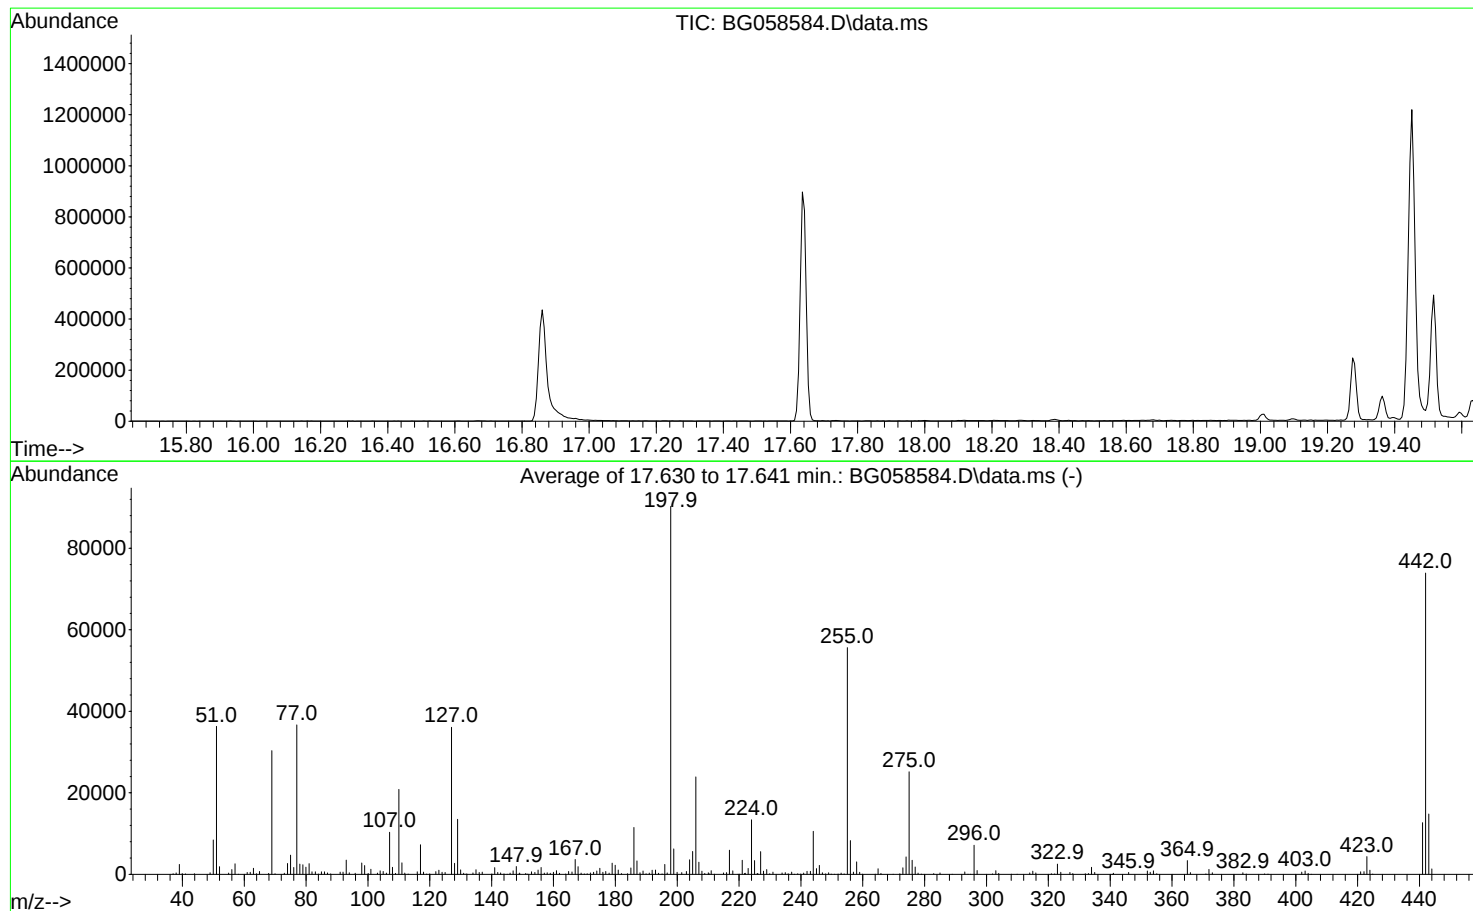




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	36293	PASS
68	69	0.00	2	0.7	227	PASS
69	198	0.00	100	33.6	30349	PASS
70	69	0.00	2	0.5	152	PASS
127	198	10	80	40.0	36077	PASS
197	198	0.00	2	0.4	345	PASS
198	198	100	100	100.0	90237	PASS
199	198	5	9	6.9	6260	PASS
275	198	10	60	27.9	25160	PASS
365	198	1	100	3.7	3374	PASS
441	198	0.01	100	14.1	12693	PASS
442	442	50	100	100.0	73915	PASS
443	442	15	24	20.0	14795	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080323\
Data File : BG058584.D
Acq On : 3 Aug 2023 8:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 03 12:50:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

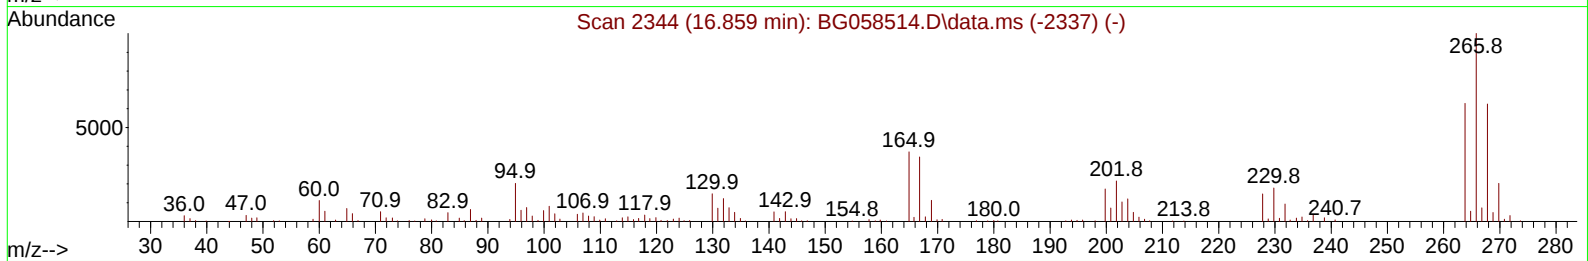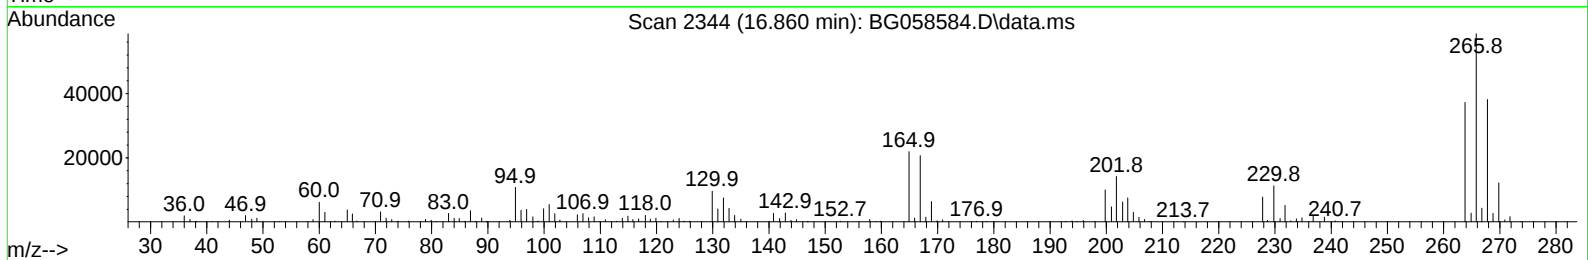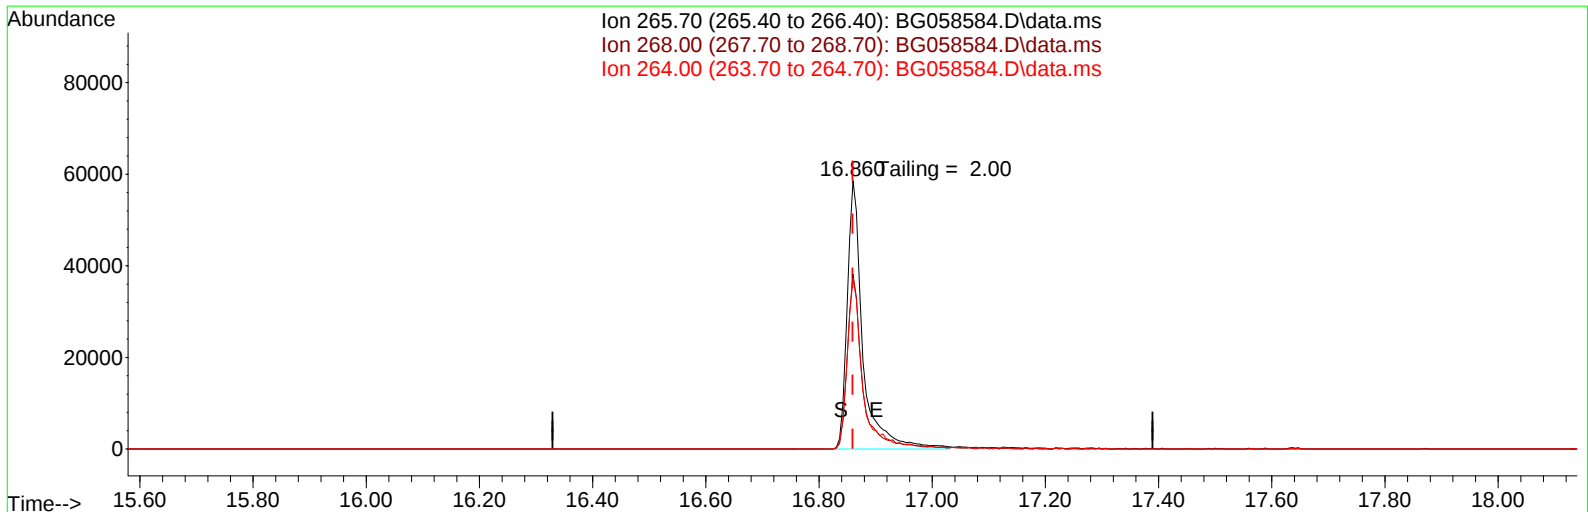

TIC: BG058584.D\data.ms

(70) Pentachlorophenol (C)

16.860min (+ 0.001) 32040.76 ng




response 113047

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	65.09
264.00	62.80	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080323\
Data File : BG058584.D
Acq On : 3 Aug 2023 8:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 03 12:50:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

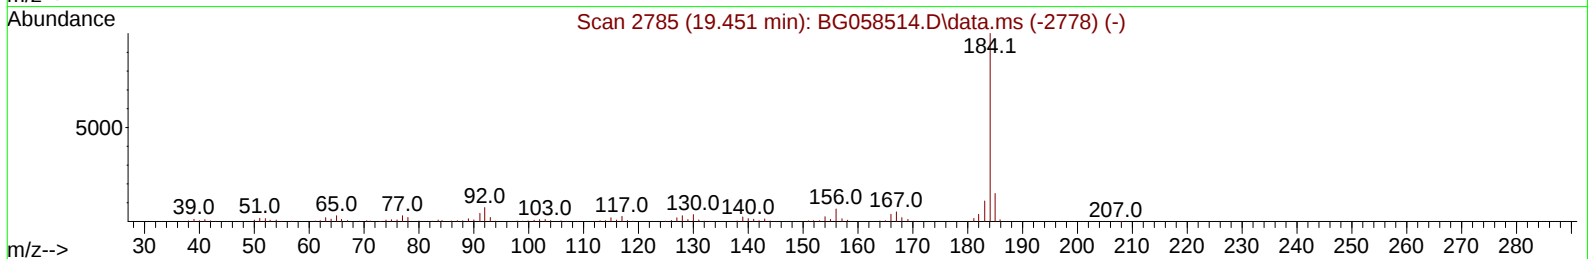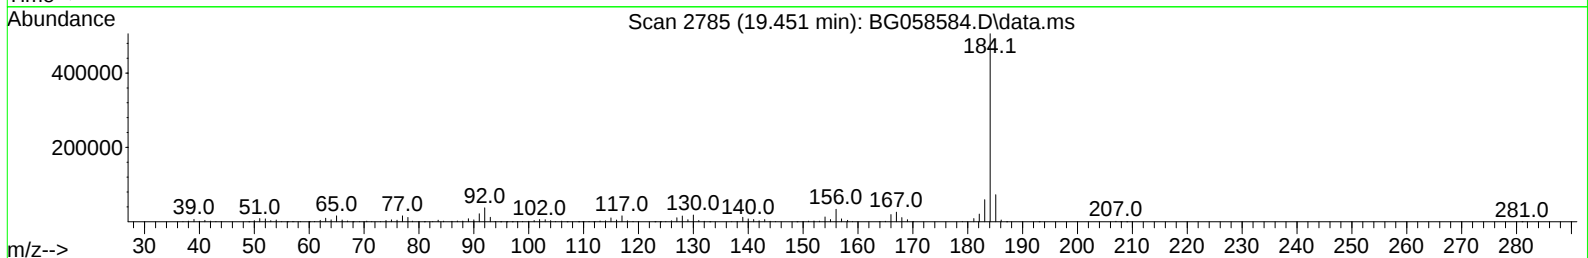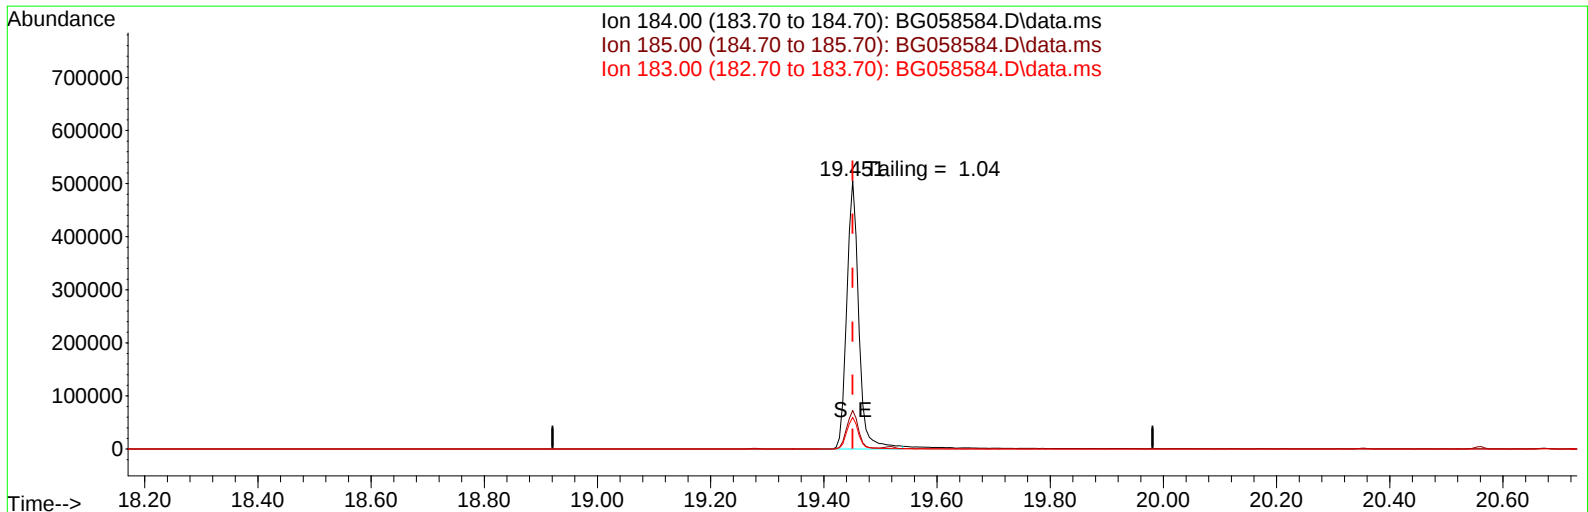

TIC: BG058584.D\data.ms

(77) Benzidine

19.451min (+ 0.000) 0.00 ng

response 764615

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.41
183.00	10.90	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2023	BNA_G	<u>BG058584.D</u>
Compound Name	Response	Retention Time
DDT	370398	20.673
DDD	10290	20.238
DDE	1733	19.093
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12023	382421	3.14

Instrument :
BNA_G
ClientSampleId :
DFTPP