
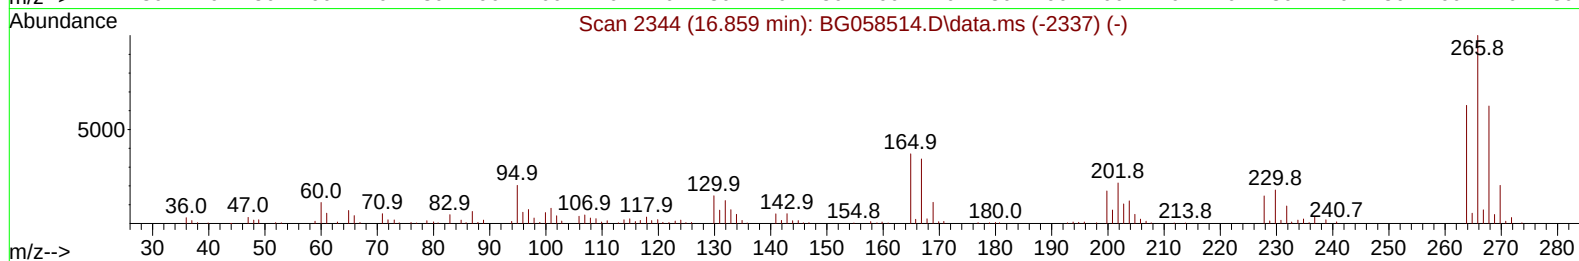
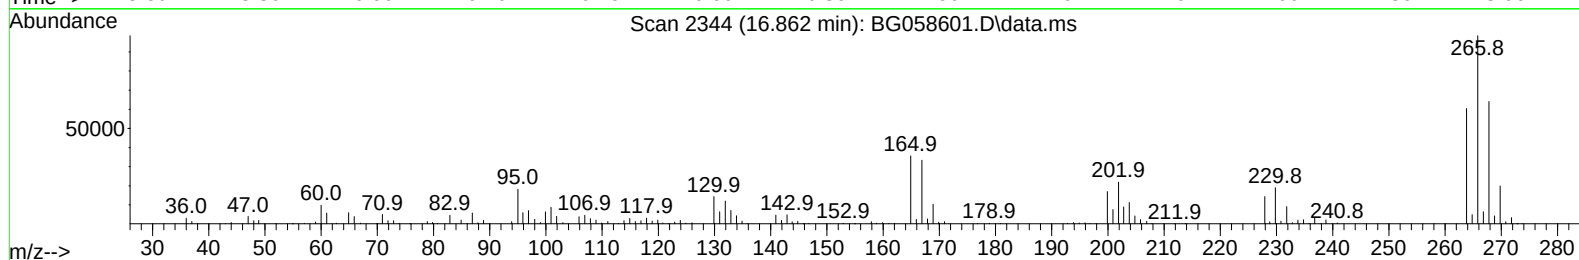


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080423\
Data File : BG058601.D
Acq On : 4 Aug 2023 7:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 08:33:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

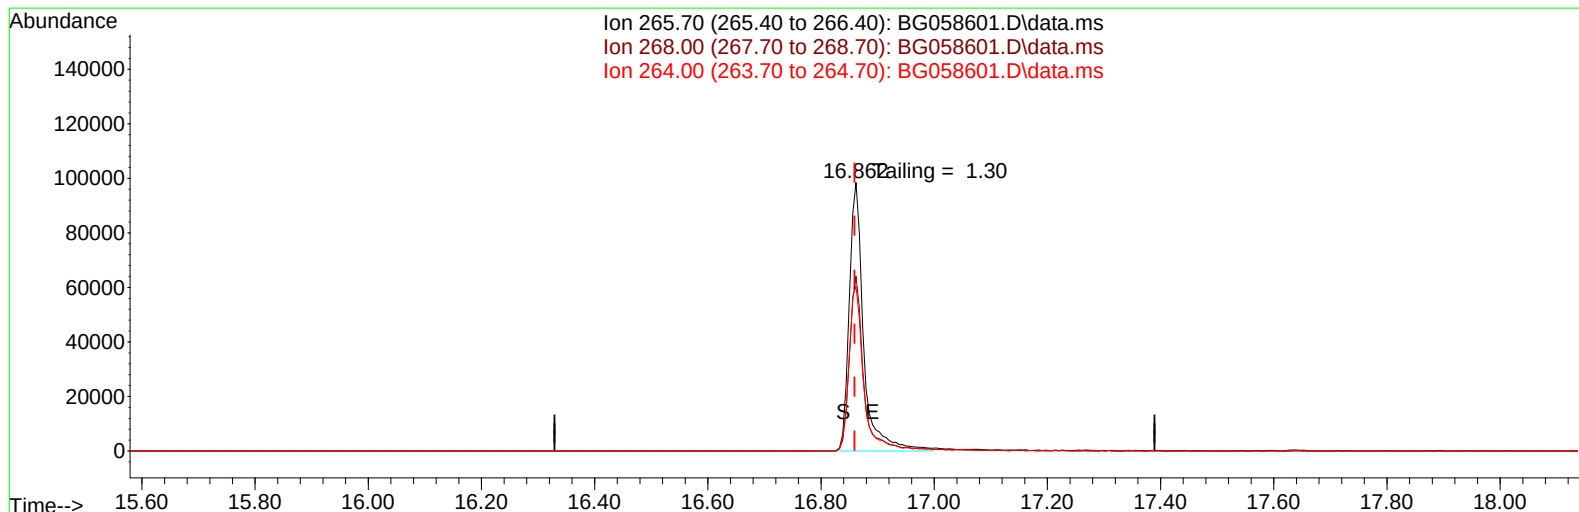

TIC: BG058601.D\data.ms

(70) Pentachlorophenol (C)




16.862min (+ 0.003) 27310.37 ng

response 177615

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	65.05
264.00	62.80	61.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080423\
Data File : BG058601.D
Acq On : 4 Aug 2023 7:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 08:33:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

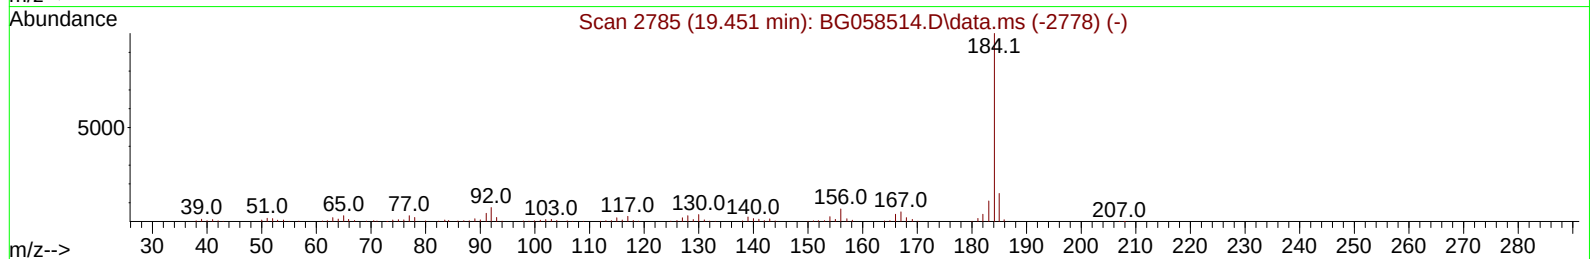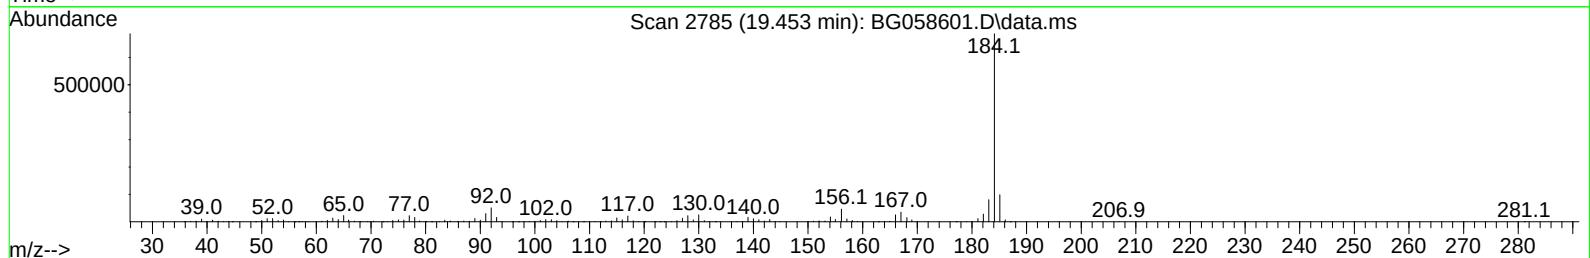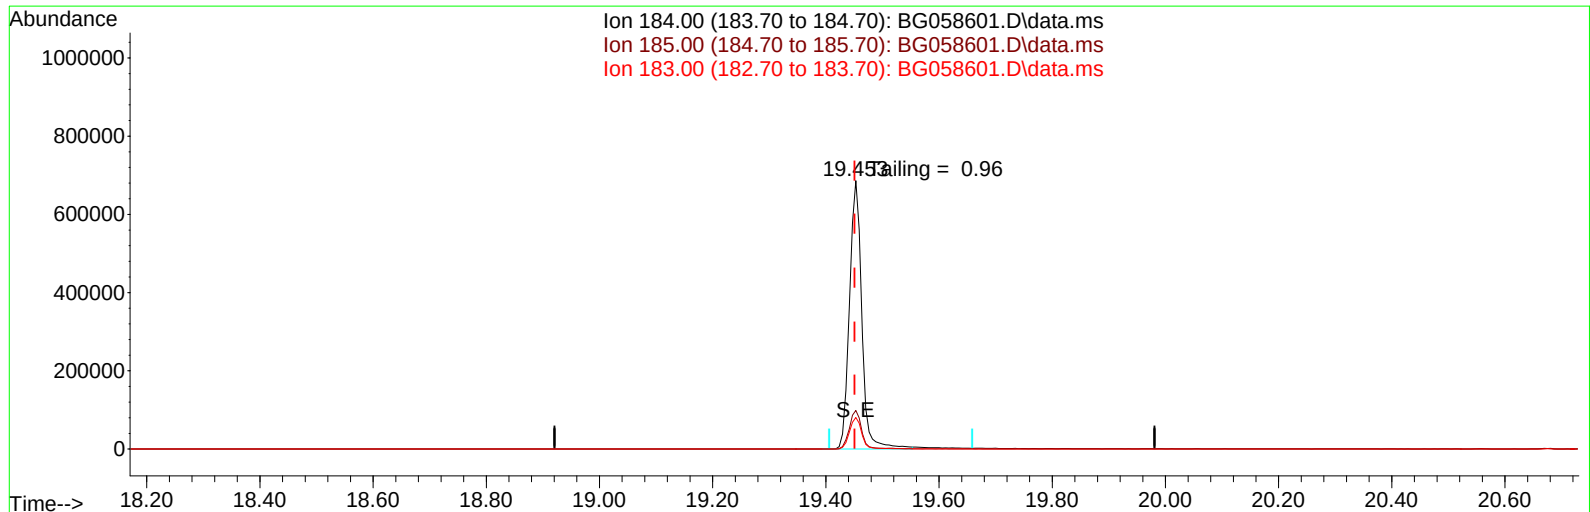

TIC: BG058601.D\data.ms

(77) Benzidine

19.453min (+ 0.002) 0.00 ng

response 1059697

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.41
183.00	10.90	11.78
0.00	0.00	0.00