
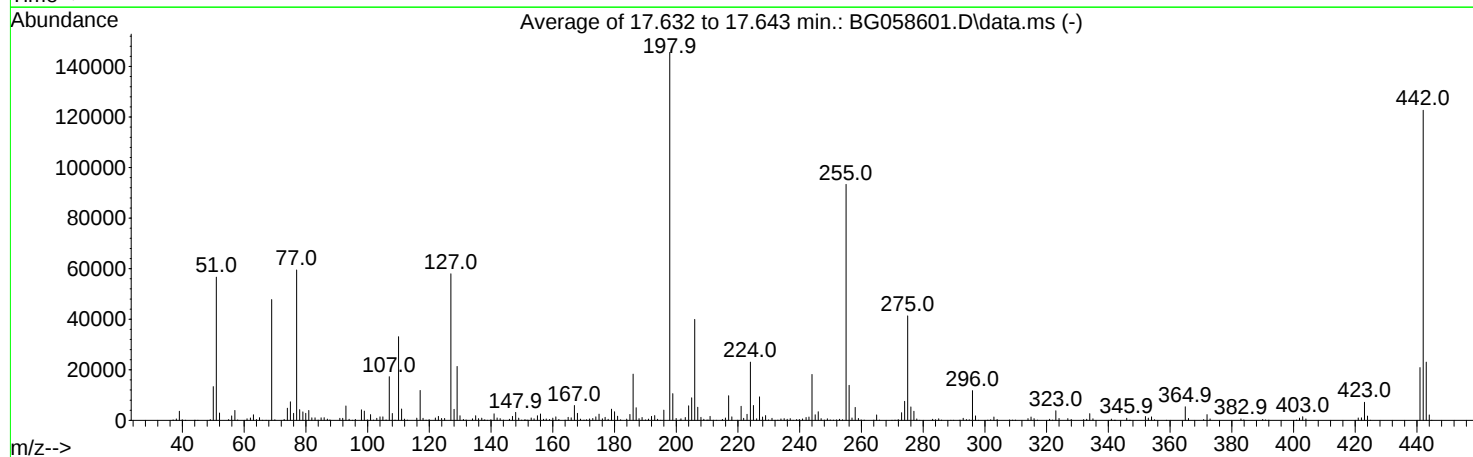


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080423\
Data File : BG058601.D
Acq On : 4 Aug 2023 7:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

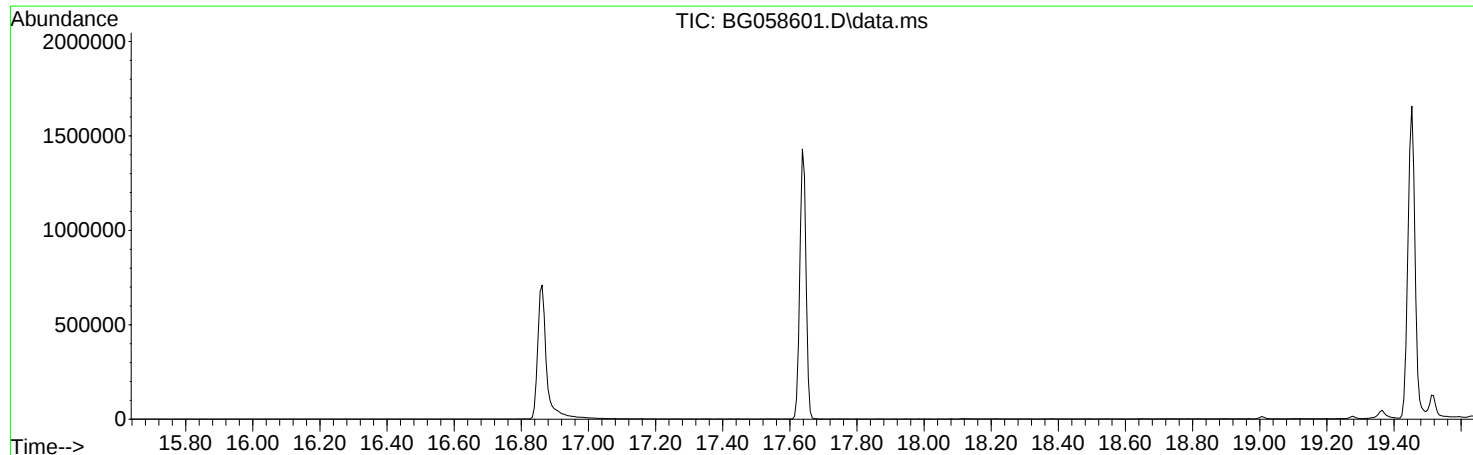




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	56667	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.8	47787	PASS
70	69	0.00	2	0.5	236	PASS
127	198	10	80	39.8	57979	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	145520	PASS
199	198	5	9	7.2	10550	PASS
275	198	10	60	28.4	41333	PASS
365	198	1	100	3.7	5408	PASS
441	198	0.01	100	14.4	20922	PASS
442	442	50	100	100.0	122651	PASS
443	442	15	24	18.8	23056	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080423\
Data File : BG058601.D
Acq On : 4 Aug 2023 7:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 04 08:33:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

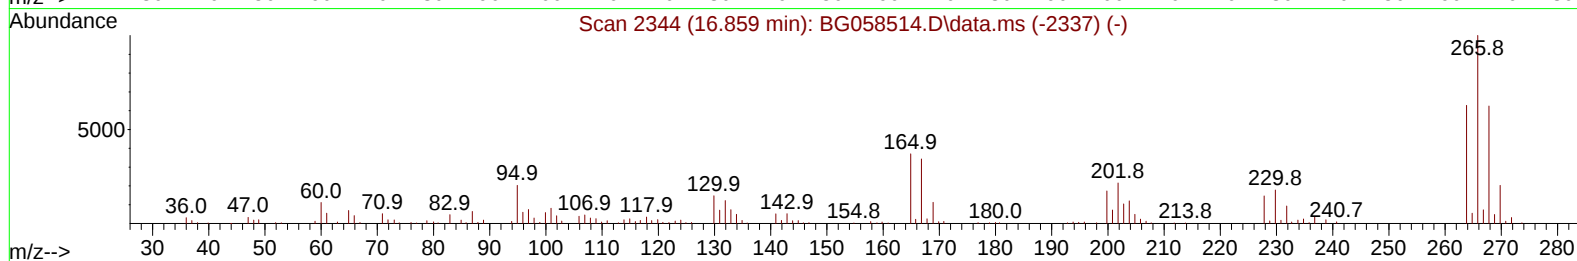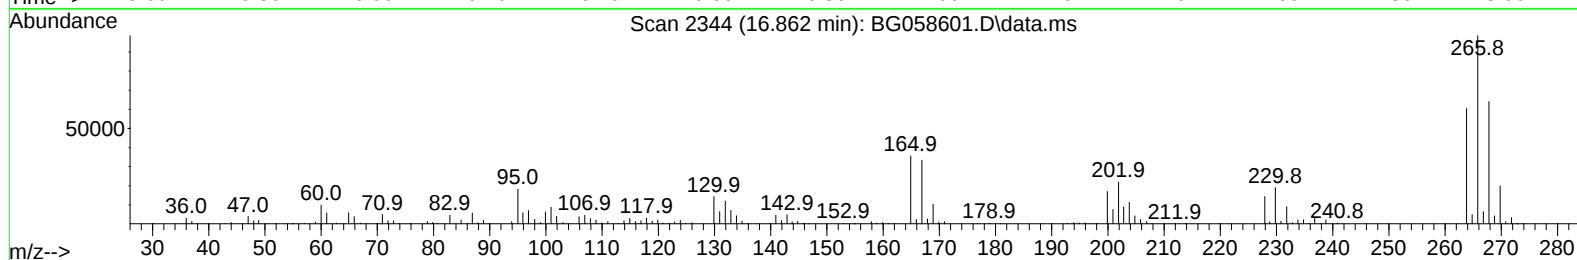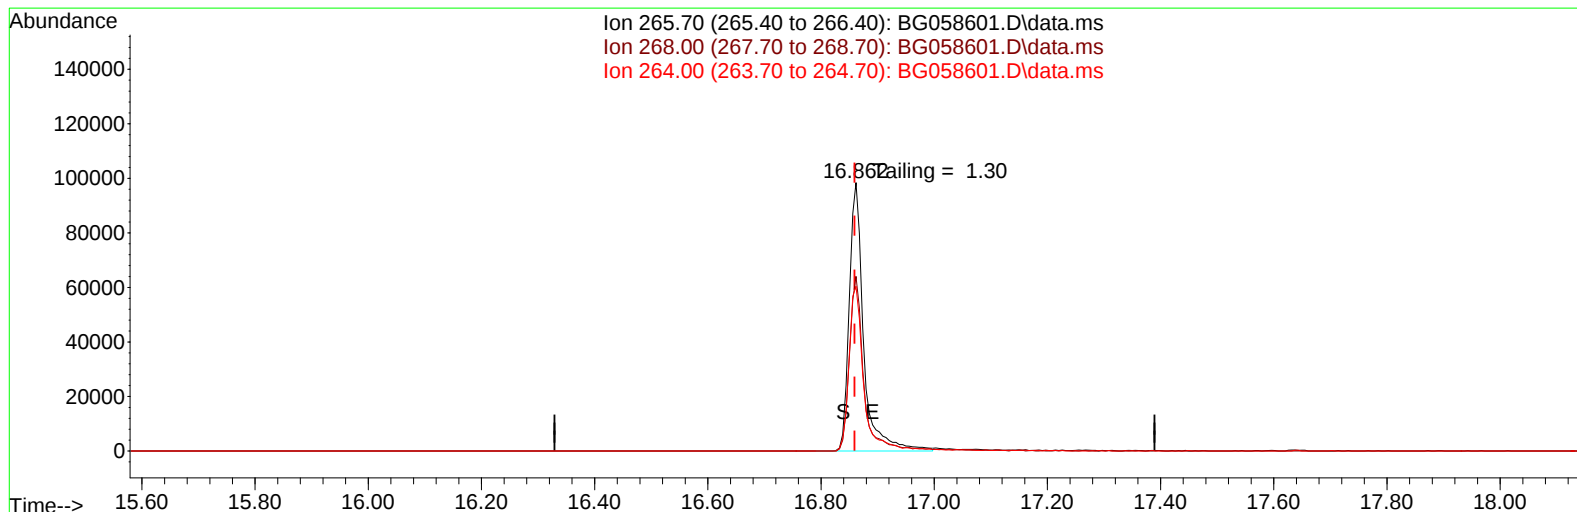

TIC: BG058601.D\data.ms

(70) Pentachlorophenol (C)

16.862min (+ 0.003) 27310.37 ng




response 177615

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	65.05
264.00	62.80	61.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080423\
Data File : BG058601.D
Acq On : 4 Aug 2023 7:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 04 08:33:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

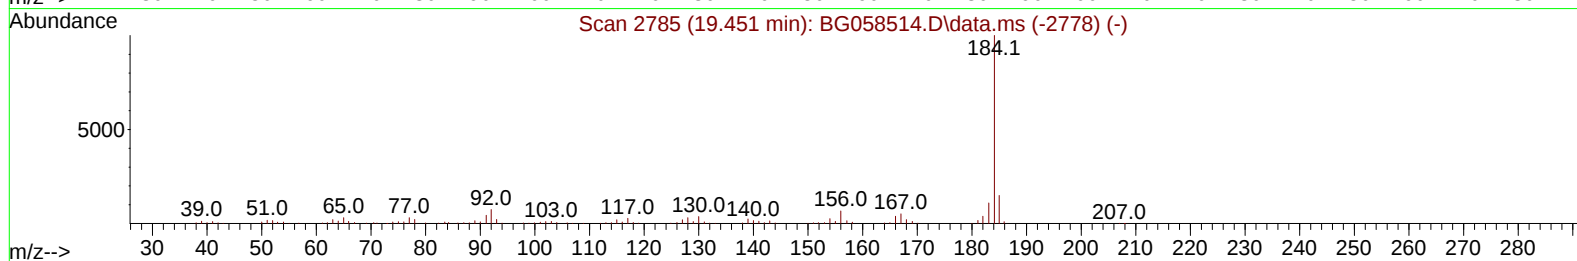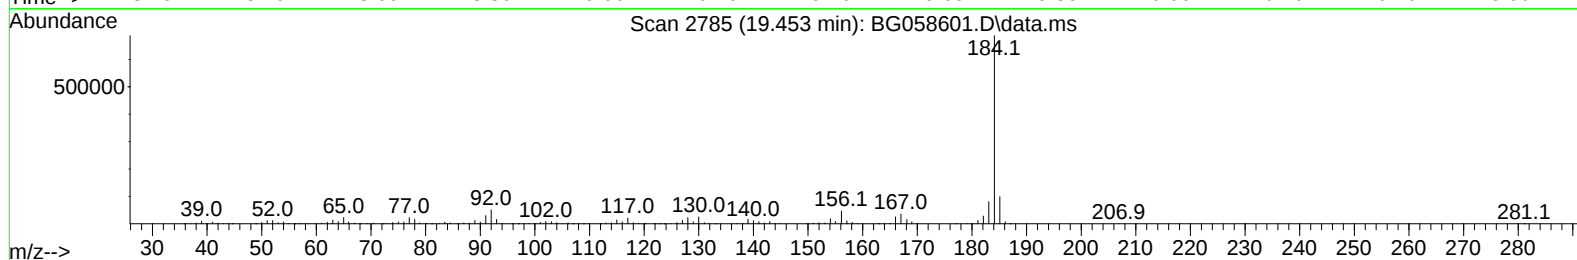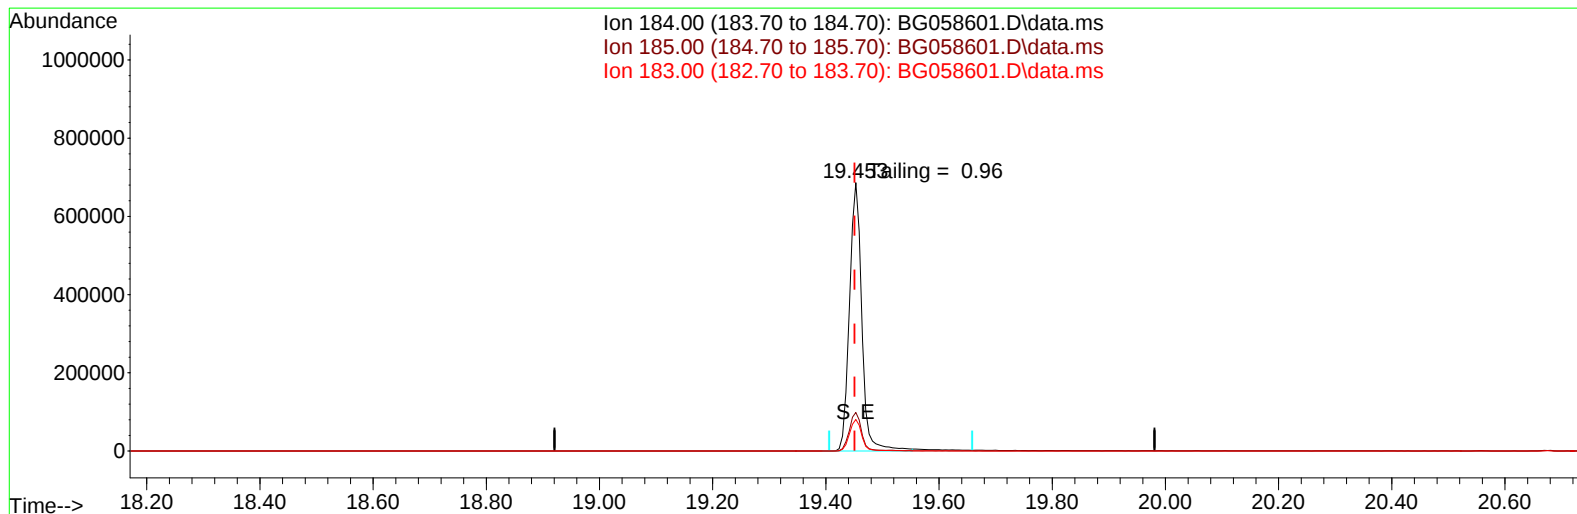

TIC: BG058601.D\data.ms

(77) Benzidine

19.453min (+ 0.002) 0.00 ng

response 1059697

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.41
183.00	10.90	11.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/4/2023	BNA_G	<u>BG058601.D</u>
Compound Name	Response	Retention Time
DDT	520480	20.675
DDD	13865	20.24
DDE	55	19.1
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13920	534400	2.60

Instrument :
BNA_G
ClientSampleId :
DFTPP