

Data File : BG041984.D
Acq On : 6 Aug 2019 3:04
Operator : HP/JU
Sample : PB121726BL
Misc : GCMS CONFIRMATION
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK26

Quant Time: Aug 06 07:01:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 06:57:43 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	149154	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	549491	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	370035	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	809984	20.00	ng/ul	0.00
77) Chrysene-d12	21.73	240	931883	20.00	ng/ul	0.00
85) Perylene-d12	25.00	264	1091965	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	10.86	131	406	0.04	ng/ul	-0.12
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	14.69	160	163640	4.99	ng/ul	0.31
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.70	176	666	0.03	ng/ul	0.02
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.54	188	5232	0.13	ng/ul	0.00
78) Pyrene-d10	0.00	212	0	0.00	ng/ul	
89) Benzo(a)pyrene-d12	25.00	264	1091965	19.14	ng/ul	0.23


Target Compounds					Qvalue	
44) Dimethylphthalate	14.69	163	82569	2.898	ng/ul#	1
45) 2,6-Dinitrotoluene	14.69	165	49287	7.952	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG041984.D
Acq On : 6 Aug 2019 3:04
Operator : HP/JU
Sample : PB121726BL
Misc : GCMS CONFIRMATION
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK26

Quant Time: Aug 06 07:01:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 06:57:43 2019
Response via : Initial Calibration




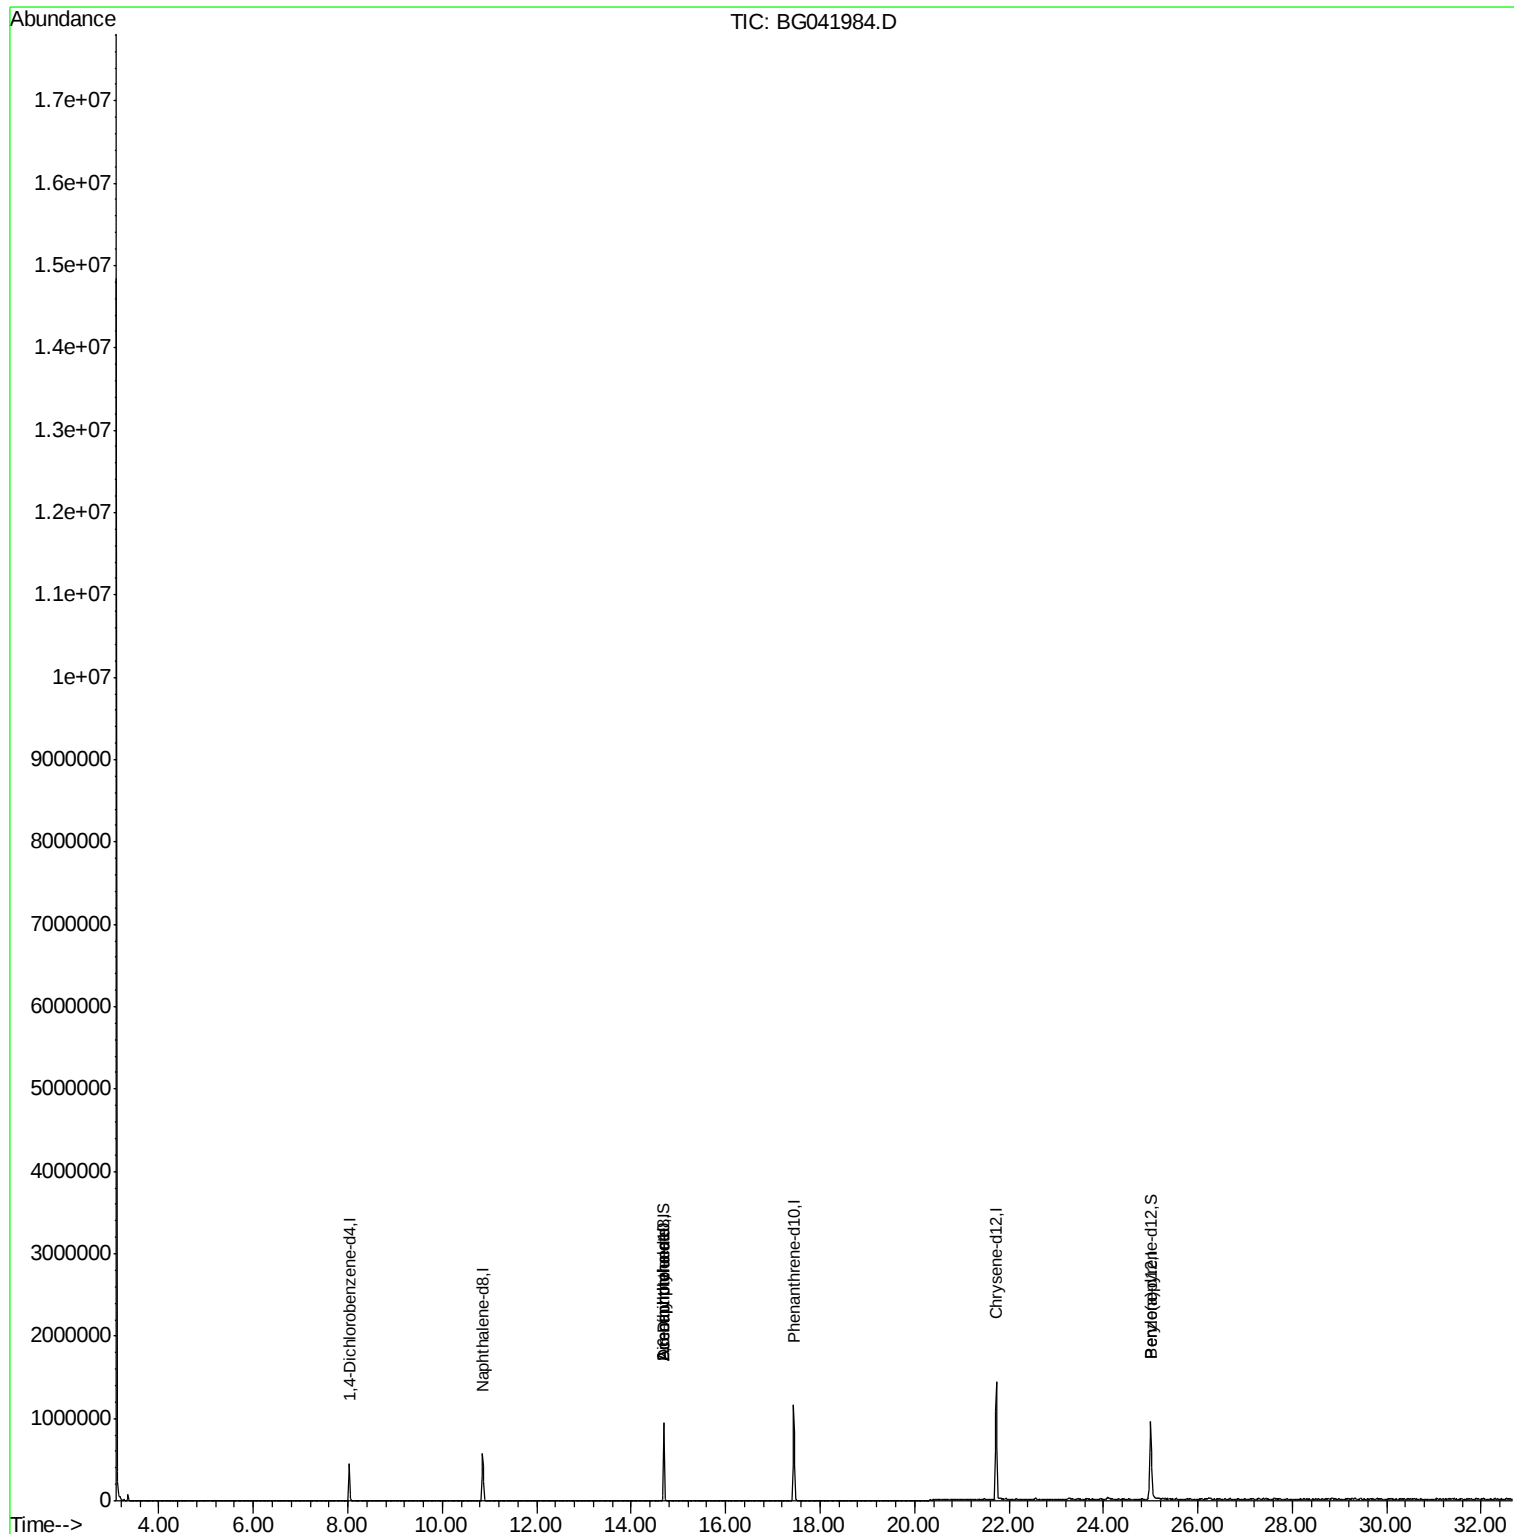


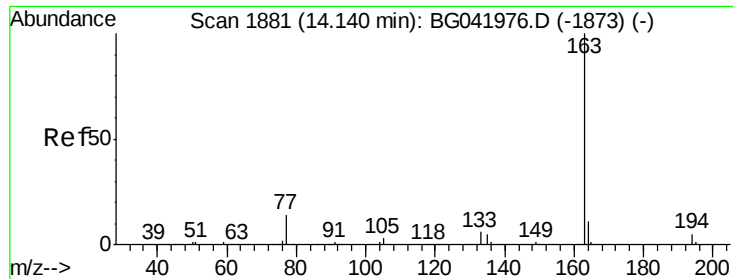

#44
Dimethylphthalate
Concen: 2.898 ng/ul
RT: 14.69 min Scan# 1975
Delta R.T. 0.55 min
Lab File: BG041984.D
Acq: 6 Aug 2019 3:04

Instrument :
BNA_G
ClientSampleId :
SBLK26

Tgt Ion	Resp	Ratio	Lower	Upper
163	82569	100		
194		0.0	4.2	6.2#
164		461.5	7.8	11.8#

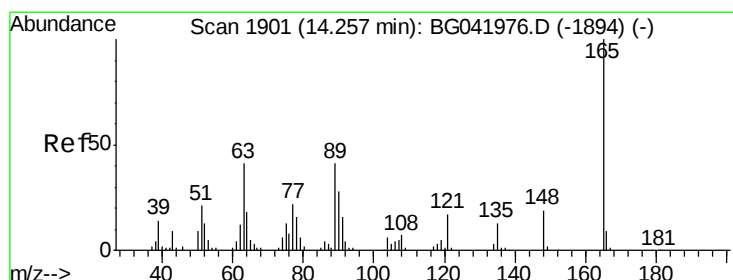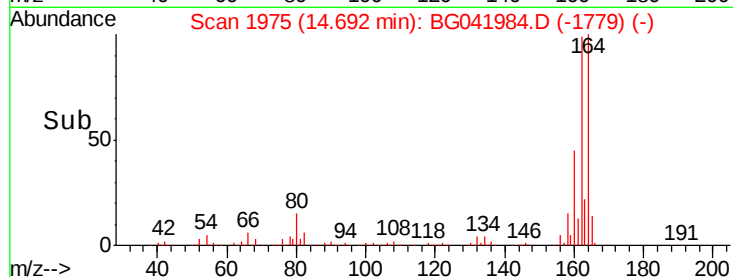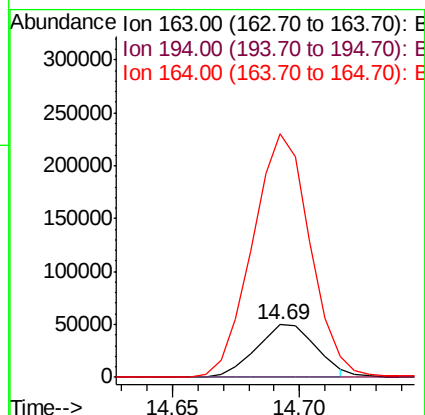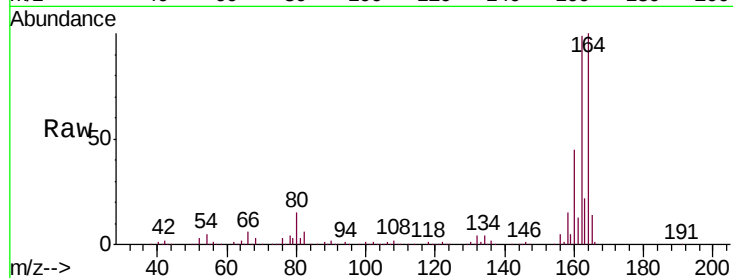

#45
2,6-Dinitrotoluene
Concen: 7.952 ng/ul
RT: 14.69 min Scan# 1975
Delta R.T. 0.44 min
Lab File: BG041984.D
Acq: 6 Aug 2019 3:04

Tgt Ion	Resp	Ratio	Lower	Upper
165	49287	100		
89		1.9	36.8	55.2#
121		0.7	15.6	23.4#

