

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080519\
 Data File : BG041974.D
 Acq On : 5 Aug 2019 20:40
 Operator : HP/JU
 Sample : K3976-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0CA9

Quant Time: Aug 06 04:54:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 04:50:21 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	77714	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	325909	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	219009	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	491640	20.00	ng/ul	0.00
77) Chrysene-d12	21.73	240	500130	20.00	ng/ul	0.00
85) Perylene-d12	25.00	264	482303	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.40	96	215101	121.10	ng/uL	-0.02
5) Phenol-d5	7.19	99	48533	7.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.35	67	98433	28.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.56	132	136421	26.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	92162	18.00	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	83742	34.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.93	143	102099	35.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	181553	31.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.99	131	26716	4.19	ng/ul	0.00
43) Dimethylphthalate-d6	14.10	166	597307	35.17	ng/ul	0.00
46) Acenaphthylene-d8	14.38	160	683655	35.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.88	143	22293	7.82	ng/ul	0.00
57) Fluorene-d10	15.69	176	543333	35.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.80	200	86667	27.48	ng/ul	0.00
70) Anthracene-d10	17.54	188	879341	37.28	ng/ul	0.00
78) Pyrene-d10	19.83	212	1003653	35.96	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.78	264	1056230	41.92	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.14	163	52732	3.127	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080519\
Data File : BG041974.D
Acq On : 5 Aug 2019 20:40
Operator : HP/JU
Sample : K3976-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0CA9

Quant Time: Aug 06 04:54:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 04:50:21 2019
Response via : Initial Calibration

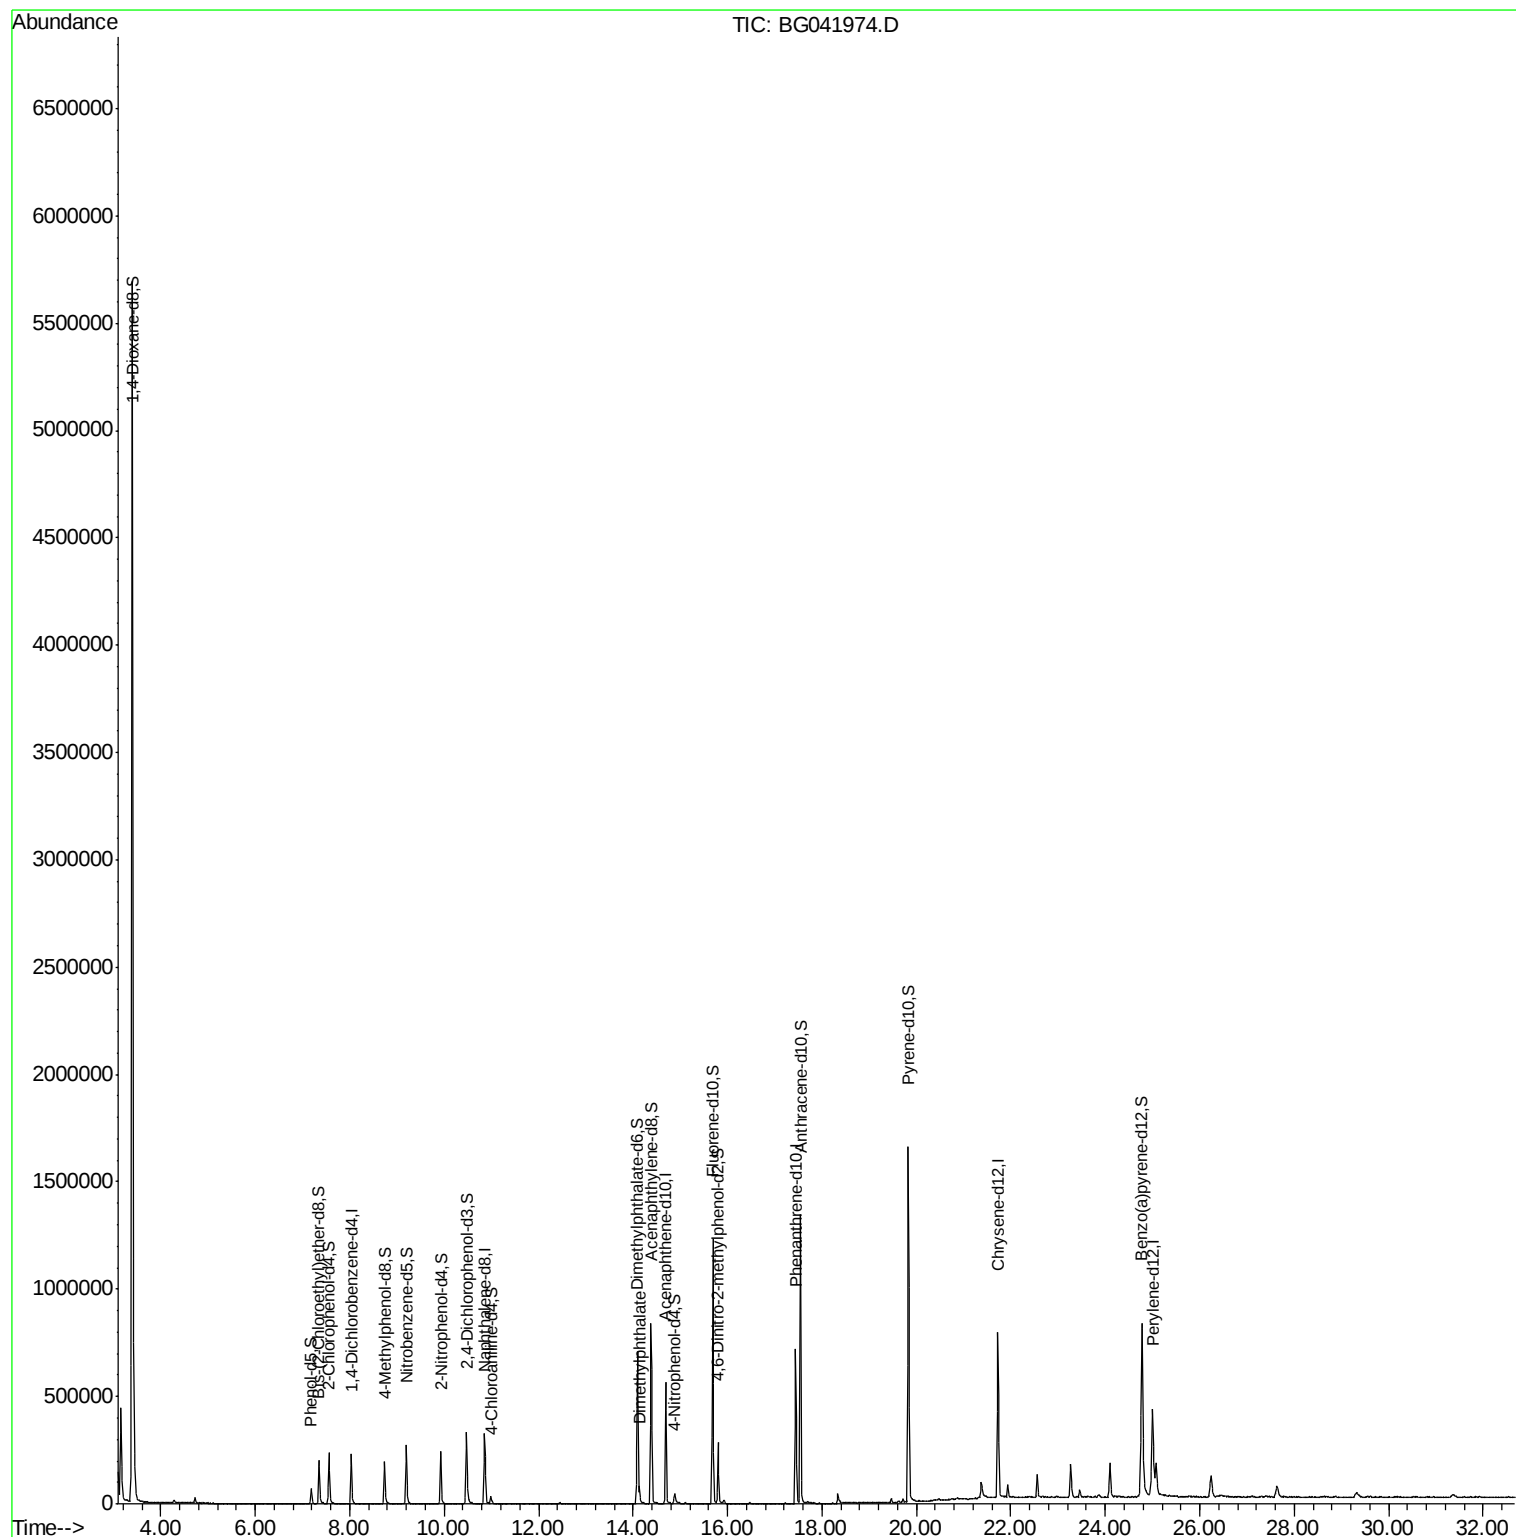

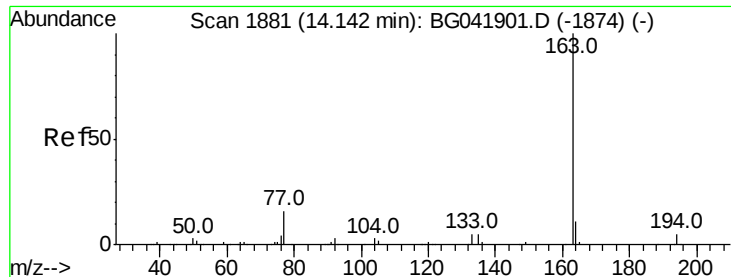

#44

Dimethylphthalate

Concen: 3.127 ng/ul

RT: 14.14 min Scan# 1880

Delta R.T. -0.00 min

Lab File: BG041974.D

Acq: 5 Aug 2019 20:40

Instrument :

BNA_G

ClientSampleId :

C0CA9

Tot Ion:163 Resp: 52732

Ion Ratio Lower Upper

163 100

194 5.1 4.2 6.2

164 11.8 7.8 11.8#

