

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080521\
 Data File : BG049659.D
 Acq On : 5 Aug 2021 21:25
 Operator : CG/JU
 Sample : M3162-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGEW6

Manual Integrations
 APPROVED

mohammad
 8/6/2021 2:48:26 PM

Quant Time: Aug 06 03:59:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 04 16:17:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.043	152	25014	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	104307	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.693	164	70728	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.442	188	152117	20.000	ng/ul	0.00
79) Chrysene-d12	21.724	240	144528	20.000	ng/ul	0.00
88) Perylene-d12	24.996	264	153318	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.420	96	2726m	5.095	ng/uL	0.00
4) Pyridine-d5	3.849	84	36912	22.991	ng/ul	0.00
7) Phenol-d5	7.191	99	60170	26.505	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.361	67	35042	26.873	ng/ul	0.00
11) 2-Chlorophenol-d4	7.567	132	44736	27.533	ng/ul	0.00
15) 4-Methylphenol-d8	8.748	113	47734	27.577	ng/ul	0.00
21) Nitrobenzene-d5	9.212	128	23333	28.398	ng/ul	0.00
24) 2-Nitrophenol-d4	9.940	143	27831	29.660	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	45528	25.732	ng/ul	0.00
31) 4-Chloroaniline-d4	10.992	131	62346	25.740	ng/ul	0.00
46) Dimethylphthalate-d6	14.088	166	157468	28.371	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	187050	28.326	ng/ul	0.00
54) 4-Nitrophenol-d4	14.881	143	21348m	23.789	ng/ul	0.00
60) Fluorene-d10	15.685	176	131323	27.525	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.797	200	23688m	23.137	ng/ul	-0.01
73) Anthracene-d10	17.542	188	206721	28.789	ng/ul	0.00
81) Pyrene-d10	19.827	212	235943	29.629	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.767	264	226656	26.980	ng/ul	-0.01
Target Compounds						
8) Phenol	7.220	94	2677	1.190	ng/ul#	Qvalue 86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080521\
Data File : BG049659.D
Acq On : 5 Aug 2021 21:25
Operator : CG/JU
Sample : M3162-15
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BGEW6

Manual Integrations
APPROVED

mohammad
8/6/2021 2:48:26 PM

Quant Time: Aug 06 03:59:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 04 16:17:29 2021
Response via : Initial Calibration

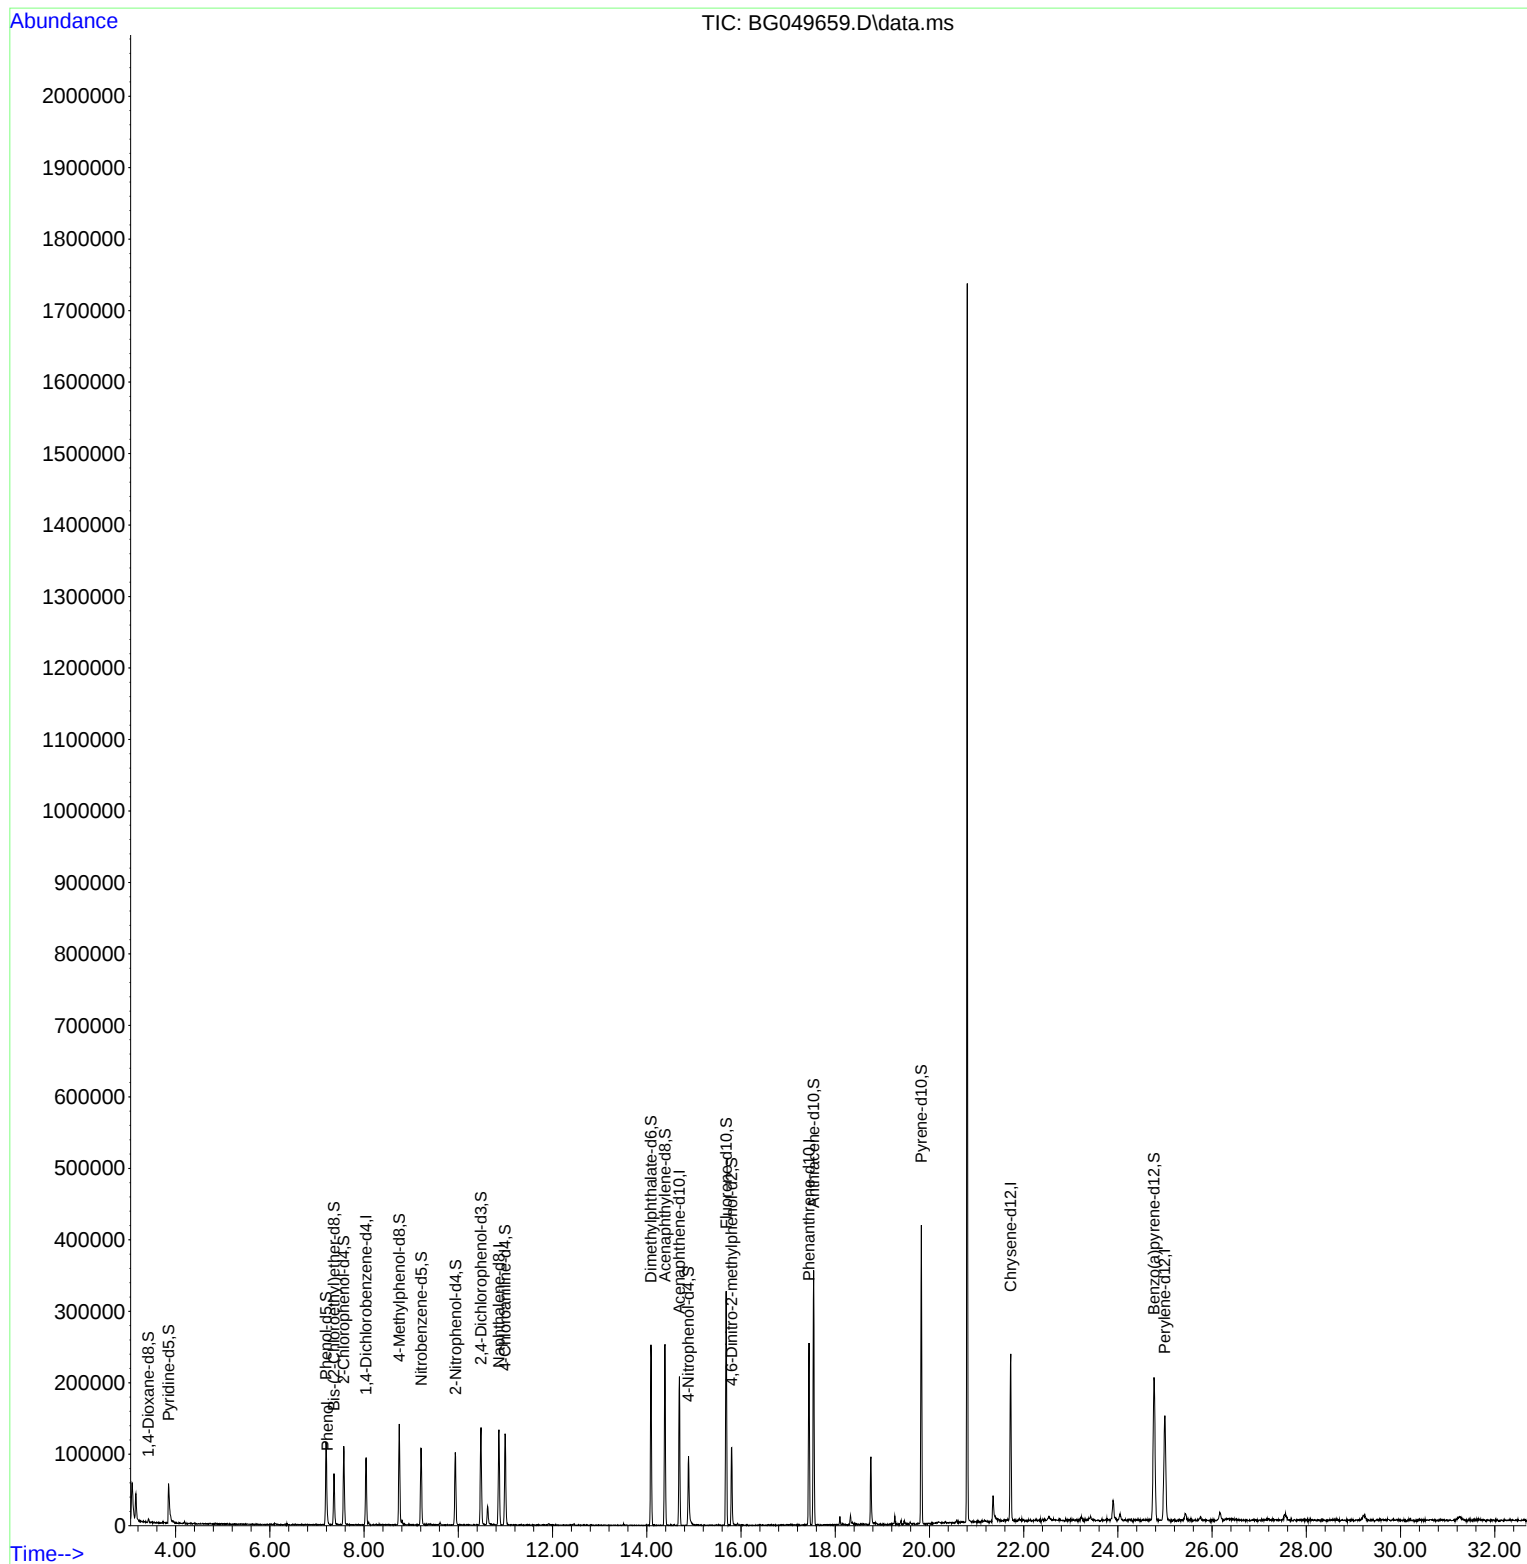

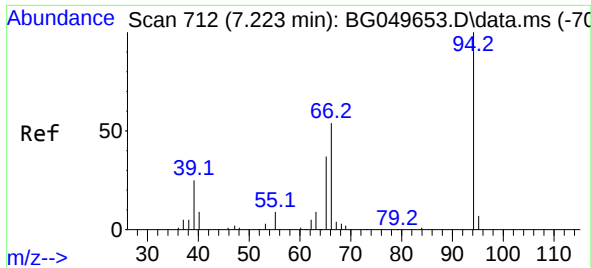

#8
Phenol
Concen: 1.190 ng/ul
RT: 7.220 min Scan# 712
Delta R.T. -0.006 min
Lab File: BG049659.D
Acq: 5 Aug 2021 21:25

Tgt Ion: 94 Resp: 2677
Ion Ratio Lower Upper
94 100
65 45.7 24.7 37.1#
66 59.1 43.7 65.5

Instrument :
BNA_G
ClientSampleId :
BGEW6

Manual Integrations
APPROVED

mohammad
8/6/2021 2:48:26 PM

