

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080521\
 Data File : BG049717.D
 Acq On : 7 Aug 2021 23:39
 Operator : CG/JU
 Sample : M3244-01
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JCE01

Quant Time: Aug 09 02:12:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 04 16:17:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.043	152	32750	20.000	ng/ul	0.00
20) Naphthalene-d8	10.862	136	137704	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.693	164	90520	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.448	188	173896	20.000	ng/ul	0.00
79) Chrysene-d12	21.730	240	153034	20.000	ng/ul	0.00
88) Perylene-d12	25.008	264	154016	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.443	96	926	1.322	ng/uL	0.02
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.203	99	39811	13.394	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.361	67	27737	16.246	ng/ul	0.00
11) 2-Chlorophenol-d4	7.579	132	34536	16.235	ng/ul	0.00
15) 4-Methylphenol-d8	8.754	113	29823	13.160	ng/ul	0.00
21) Nitrobenzene-d5	9.212	128	18943	17.463	ng/ul	0.00
24) 2-Nitrophenol-d4	9.934	143	21212	17.123	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.486	165	37650	16.118	ng/ul	0.00
31) 4-Chloroaniline-d4	0.000	131	0	0.000	ng/ul	
46) Dimethylphthalate-d6	14.093	166	124624	17.544	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	161189	19.073	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	5527	4.812	ng/ul	0.01
60) Fluorene-d10	15.685	176	113285	18.553	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.809	200	12502	10.682	ng/ul	0.00
73) Anthracene-d10	17.542	188	134781	16.420	ng/ul	0.00
81) Pyrene-d10	19.833	212	168735	20.012	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.785	264	136617	16.189	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.173	77	2538	1.602	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080521\
Data File : BG049717.D
Acq On : 7 Aug 2021 23:39
Operator : CG/JU
Sample : M3244-01
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JCE01

Quant Time: Aug 09 02:12:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 04 16:17:29 2021
Response via : Initial Calibration

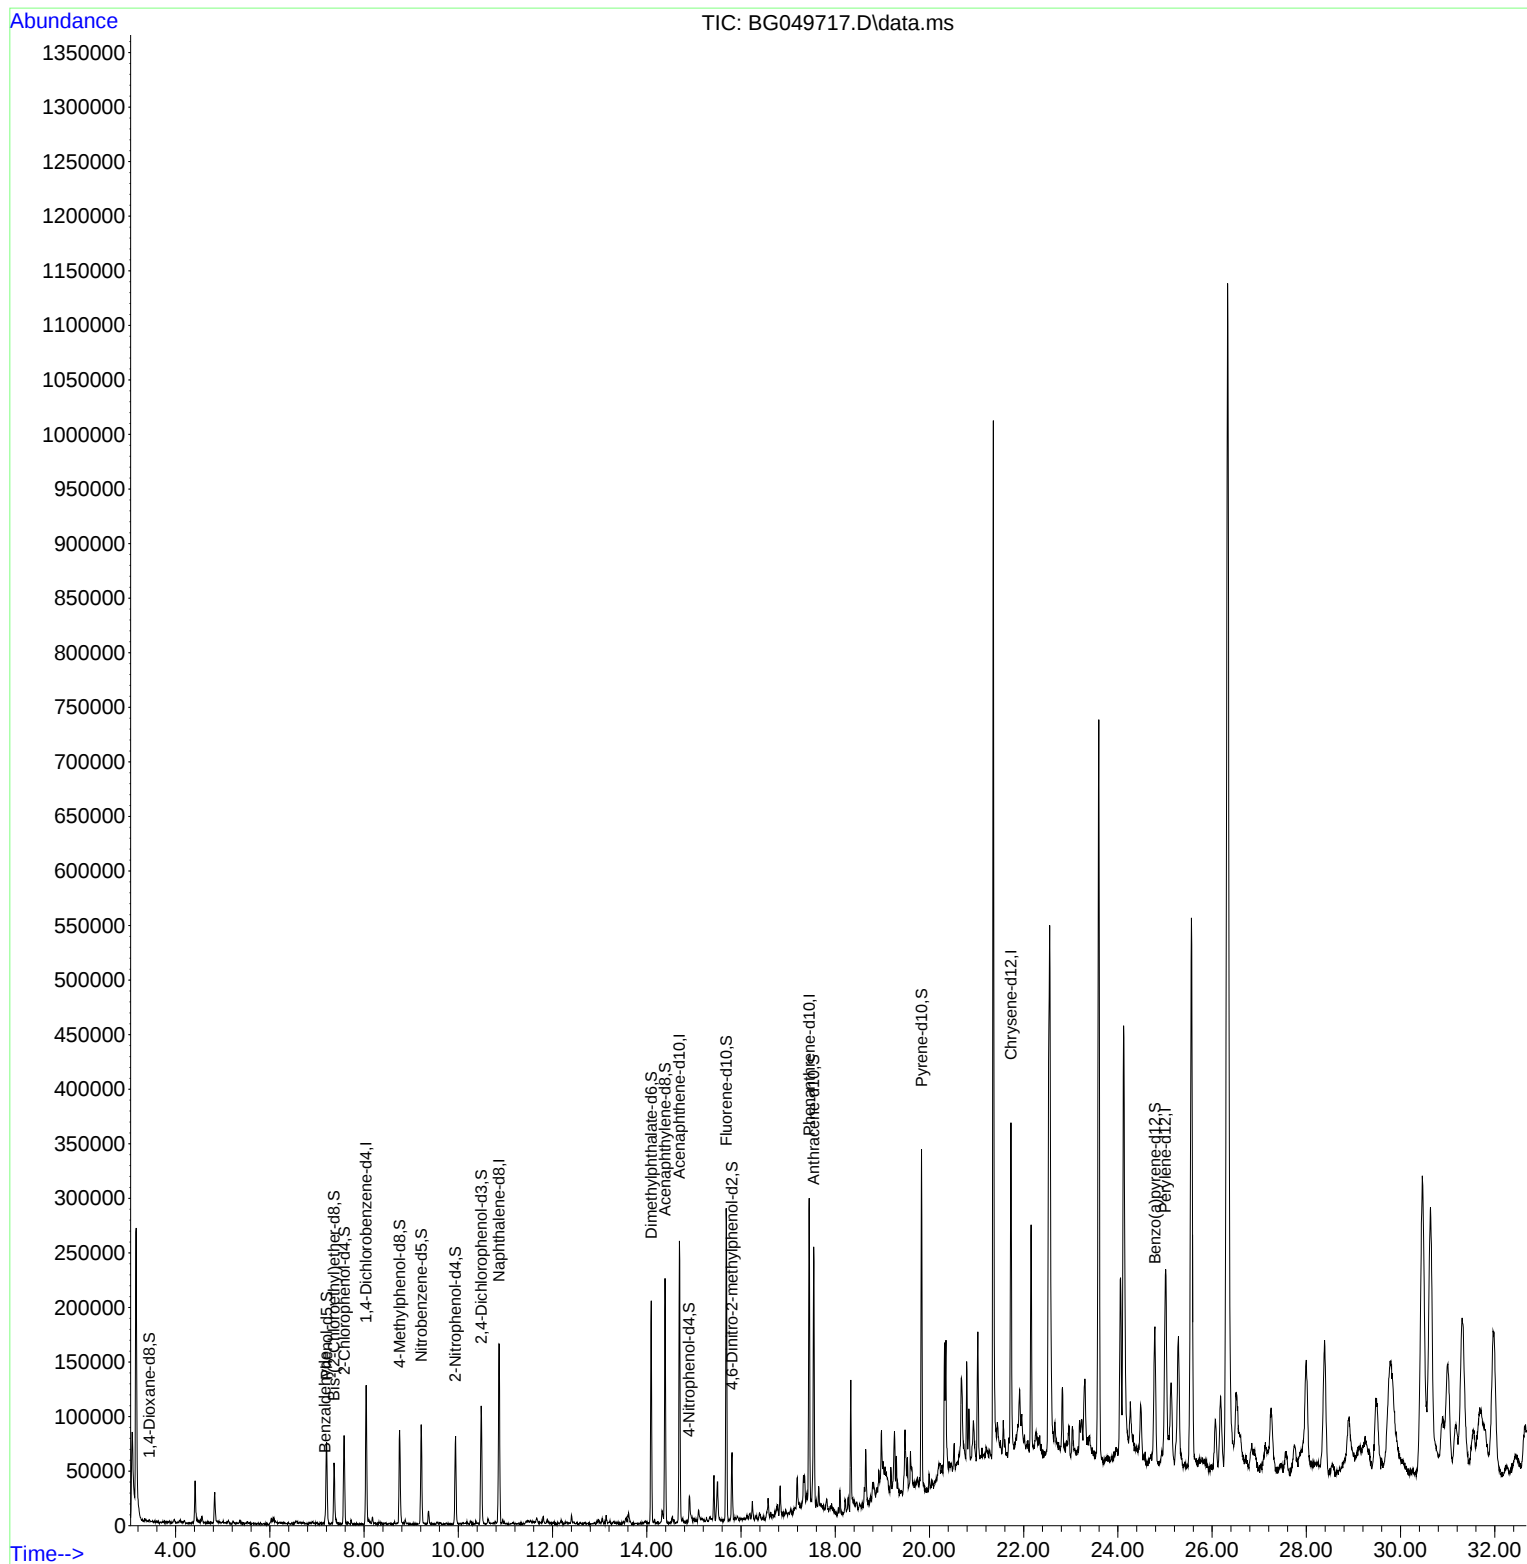

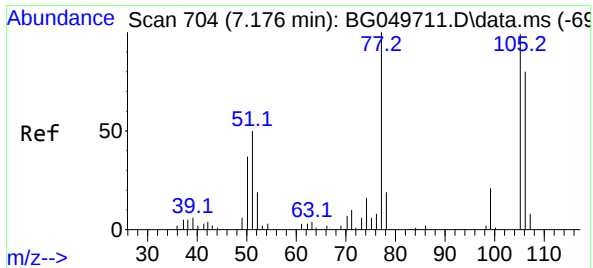

#6
Benzaldehyde
Concen: 1.602 ng/ul
RT: 7.173 min Scan# 704
Delta R.T. -0.000 min
Lab File: BG049717.D
Acq: 7 Aug 2021 23:39

Instrument :
BNA_G
ClientSampleId :
JCE01

Tgt Ion: 77 Resp: 2538

Ion	Ratio	Lower	Upper
77	100		
105	87.5	83.3	124.9
106	102.8	81.0	121.4

