

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080521\
 Data File : BG049729.D
 Acq On : 8 Aug 2021 8:36
 Operator : CG/JU
 Sample : M3208-10
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C00F0

Manual Integrations
 APPROVED

mohammad
 8/9/2021 12:11:49 PM

Quant Time: Aug 09 04:32:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 04 16:17:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.043	152	41072	20.000	ng/ul	0.00
20) Naphthalene-d8	10.863	136	166377	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.699	164	108052	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.448	188	217041	20.000	ng/ul	0.00
79) Chrysene-d12	21.730	240	186815	20.000	ng/ul	0.00
88) Perylene-d12	25.014	264	196707	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.431	96	2610	2.971	ng/uL	0.00
4) Pyridine-d5	3.872	84	18729	7.105	ng/ul	0.02
7) Phenol-d5	7.203	99	64370	17.269	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.361	67	37081	17.319	ng/ul	0.00
11) 2-Chlorophenol-d4	7.573	132	48129	18.040	ng/ul	0.00
15) 4-Methylphenol-d8	8.754	113	45690	16.076	ng/ul	0.00
21) Nitrobenzene-d5	9.218	128	25315	19.316	ng/ul	0.00
24) 2-Nitrophenol-d4	9.940	143	31387	20.970	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	52300	18.532	ng/ul	0.00
31) 4-Chloroaniline-d4	11.004	131	20553	5.320	ng/ul	0.00
46) Dimethylphthalate-d6	14.093	166	166495	19.635	ng/ul	0.00
49) Acenaphthylene-d8	14.387	160	196049	19.434	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	22924	16.721	ng/ul	0.01
60) Fluorene-d10	15.691	176	142867	19.601	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.809	200	21383	14.638	ng/ul	0.00
73) Anthracene-d10	17.548	188	197440	19.272	ng/ul	0.00
81) Pyrene-d10	19.833	212	216753	21.058	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.785	264	194953	18.088	ng/ul	0.00
Target Compounds					Qvalue	
30) Naphthalene	10.915	128	9033	1.040	ng/ul#	87
36) 2-Methylnaphthalene	12.525	142	8106	1.218	ng/ul	93
72) Phenanthrene	17.489	178	29110	2.534	ng/ul	94
80) Fluoranthene	19.498	202	50447	3.971	ng/ul	99
82) Pyrene	19.862	202	39393	3.109	ng/ul#	98
85) Benzo(a)anthracene	21.713	228	26232m	2.139	ng/ul	
87) Chrysene	21.777	228	32874	2.870	ng/ul#	94
90) Benzo(b)fluoranthene	23.974	252	38500	2.995	ng/ul#	97
93) Benzo(a)pyrene	24.855	252	18634	1.646	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.756	276	16044m	1.080	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080521\
Data File : BG049729.D
Acq On : 8 Aug 2021 8:36
Operator : CG/JU
Sample : M3208-10
Misc :
ALS Vial : 62 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C00F0

Manual Integrations
APPROVED

mohammad
8/9/2021 12:11:49 PM


Quant Time: Aug 09 04:32:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG080421.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 04 16:17:29 2021
Response via : Initial Calibration

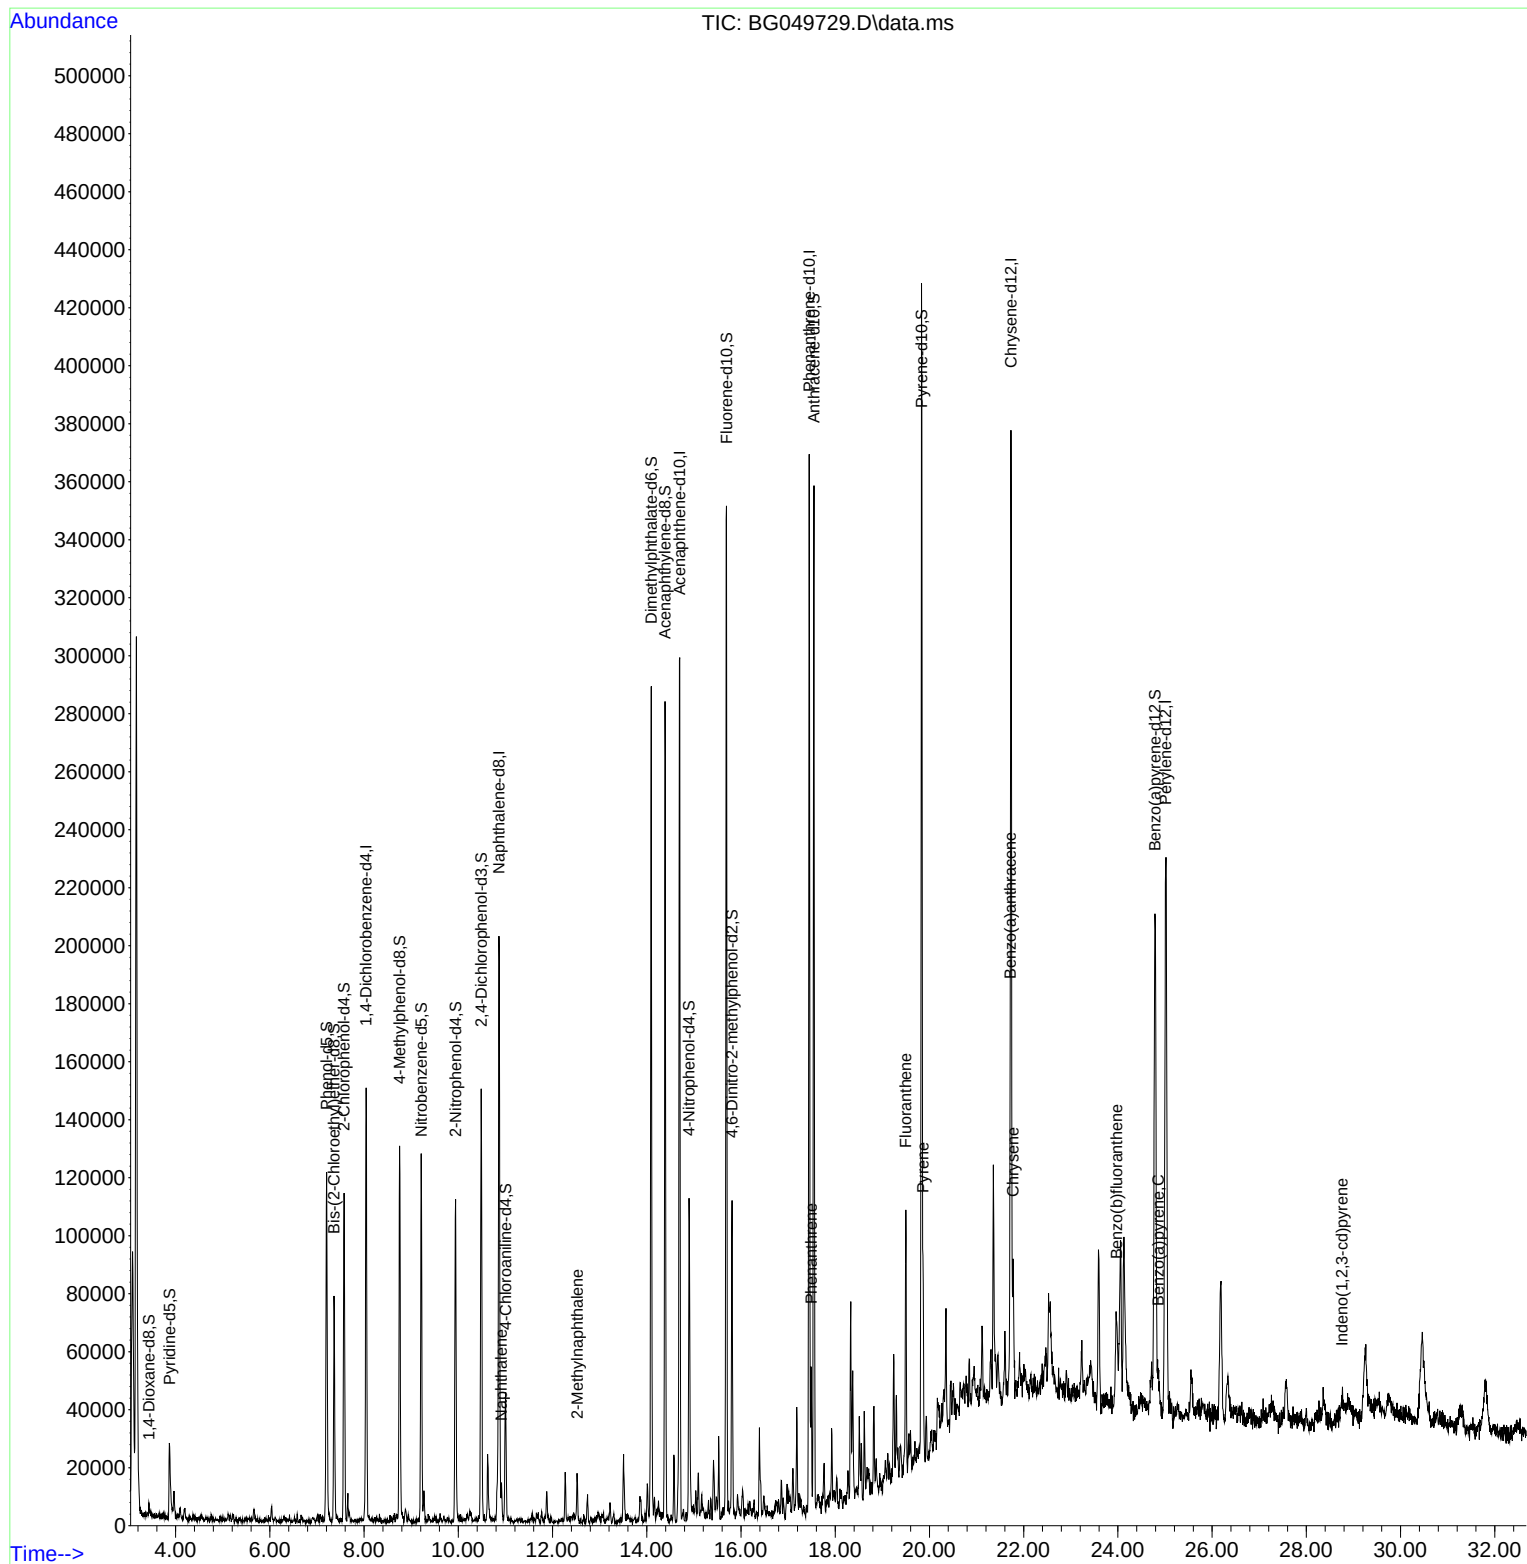



#30
Naphthalene
Concen: 1.040 ng/ul
RT: 10.915 min Scan# 1341
Delta R.T. -0.000 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36




Instrument :
BNA_G
ClientSampled :
C00F0

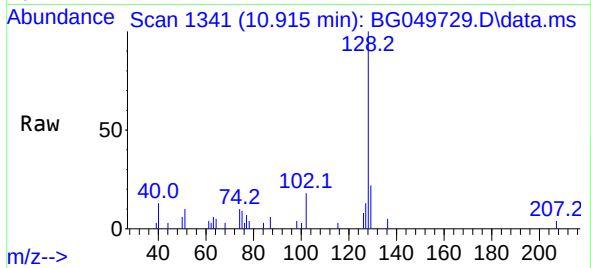


Tgt Ion:128 Resp: 9033
Ion Ratio Lower Upper
128 100
129 21.9 8.7 13.1#
127 13.3 10.6 16.0

Manual Integrations
APPROVED



mohammad
8/9/2021 12:11:49 PM

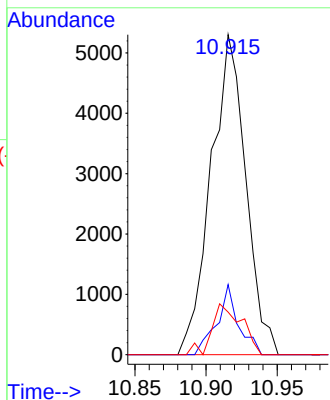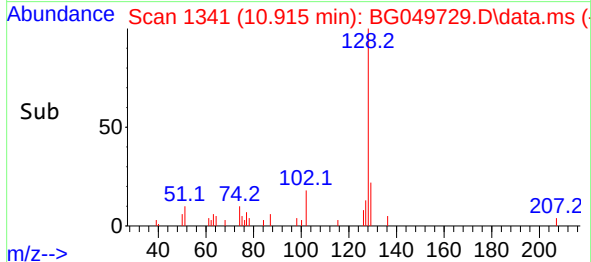


#36
2-Methylnaphthalene
Concen: 1.218 ng/ul
RT: 12.525 min Scan# 1615
Delta R.T. 0.006 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36

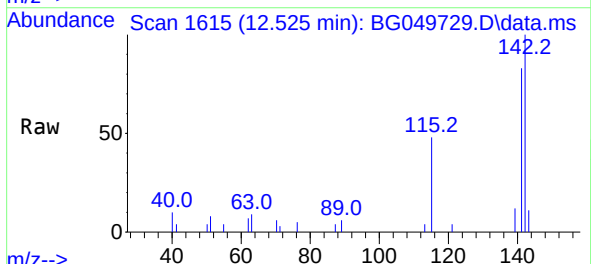


Tgt Ion:142 Resp: 8106
Ion Ratio Lower Upper
142 100
141 82.9 71.8 107.8


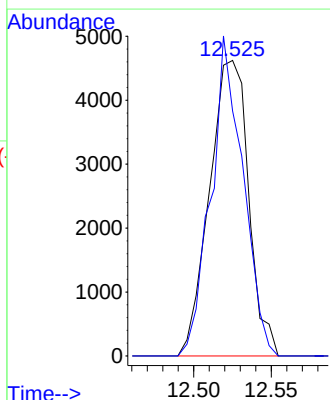
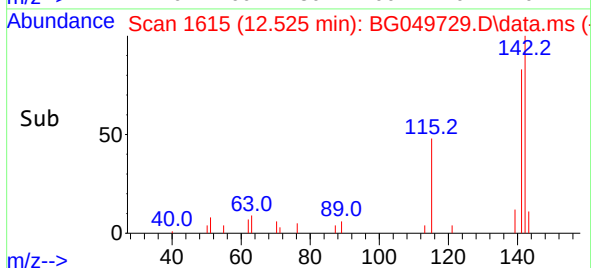





#72
Phenanthrene
Concen: 2.534 ng/ul
RT: 17.489 min Scan# 2460
Delta R.T. -0.000 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36





Tgt Ion:178 Resp: 29110
Ion Ratio Lower Upper
178 100
179 18.2 12.4 18.6
176 22.2 15.4 23.2

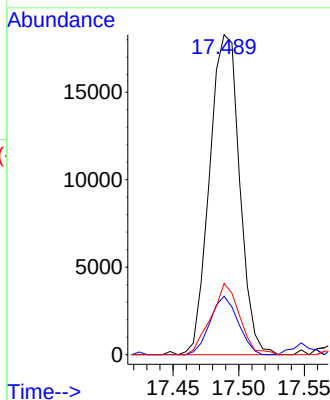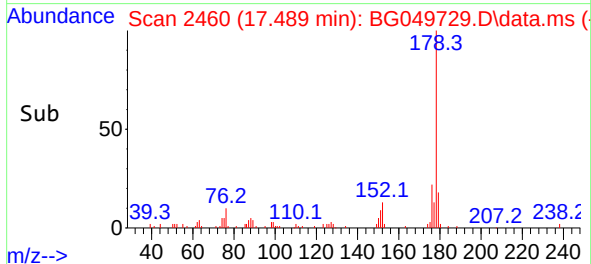

#80
Fluoranthene
Concen: 3.971 ng/ul
RT: 19.498 min Scan# 2802
Delta R.T. -0.000 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36

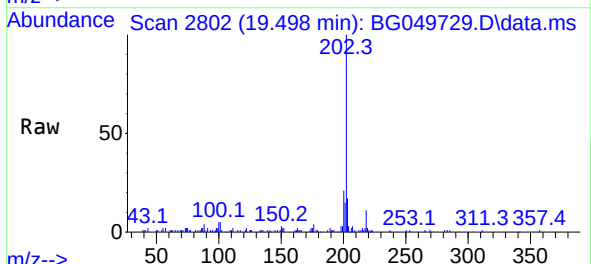


Tgt Ion:202 Resp: 50447
Ion Ratio Lower Upper
202 100
101 5.5 4.8 7.2
100 4.6 3.9 5.9

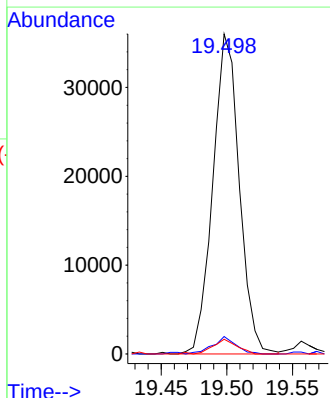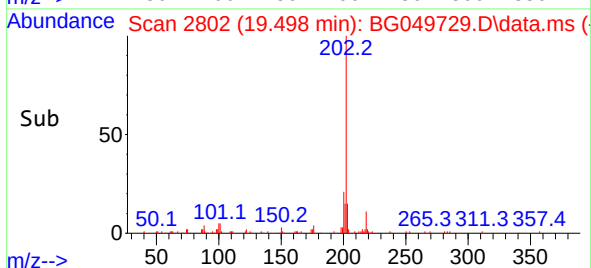


Instrument :
BNA_G
ClientSampled :
C00F0

Manual Integrations
APPROVED




mohammad
8/9/2021 12:11:49 PM




#82
Pyrene
Concen: 3.109 ng/ul
RT: 19.862 min Scan# 2864
Delta R.T. -0.000 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36

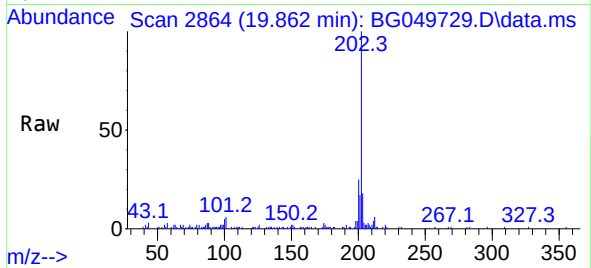



Tgt Ion:202 Resp: 39393
Ion Ratio Lower Upper
202 100
101 6.4 5.2 7.8
100 4.7 4.8 7.2#

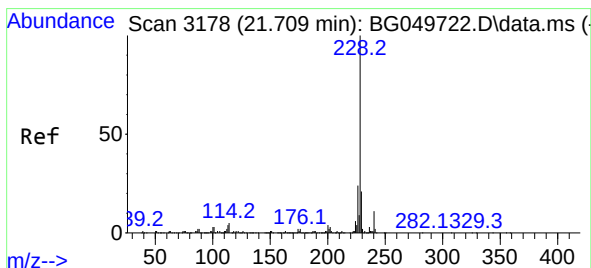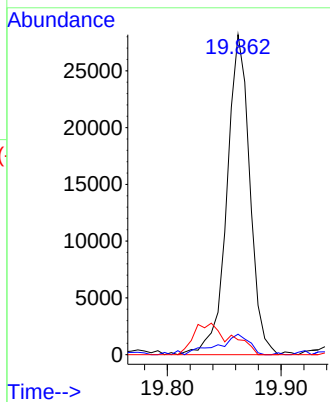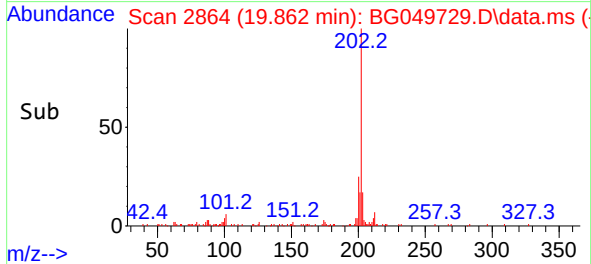

#85
Benzo(a)anthracene
Concen: 2.139 ng/ul m
RT: 21.713 min Scan# 3179
Delta R.T. 0.006 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36

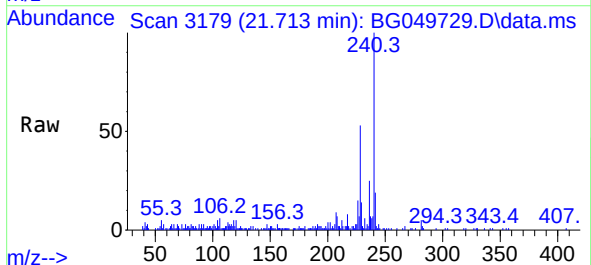


Tgt Ion:228 Resp: 26232
Ion Ratio Lower Upper
228 100
229 25.8 15.3 22.9#
226 27.4 21.0 31.6

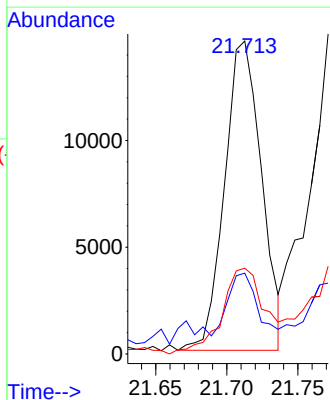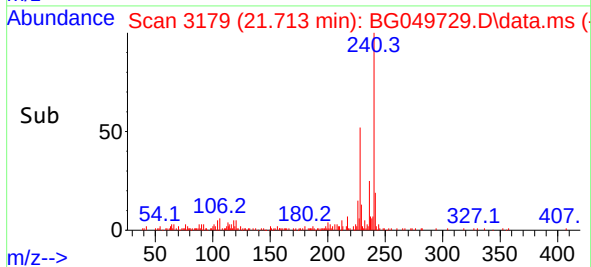

Instrument :
BNA_G
ClientSampleId :
C00F0


Manual Integrations
APPROVED

mohammad
8/9/2021 12:11:49 PM



#87
Chrysene
Concen: 2.870 ng/ul
RT: 21.777 min Scan# 3190
Delta R.T. -0.000 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36




Instrument :
BNA_G
ClientSampled :
C00F0

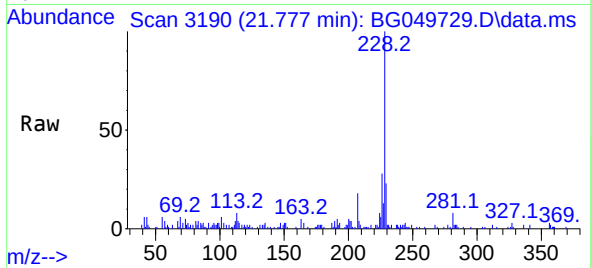


Tgt Ion:228 Resp: 32874
Ion Ratio Lower Upper
228 100
226 28.2 24.7 37.1
229 23.3 15.4 23.2#

Manual Integrations
APPROVED



mohammad
8/9/2021 12:11:49 PM

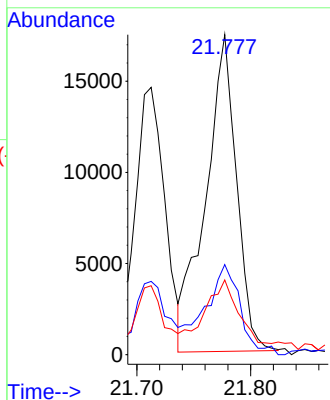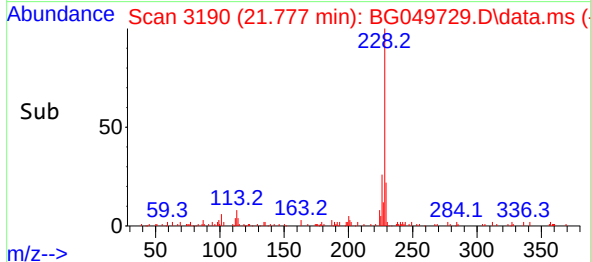


#90
Benzo(b)fluoranthene
Concen: 2.995 ng/ul
RT: 23.974 min Scan# 3564
Delta R.T. 0.017 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36

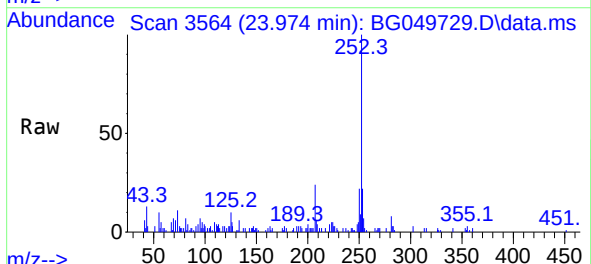


Tgt Ion:252 Resp: 38500
Ion Ratio Lower Upper
252 100
253 22.0 17.4 26.2
125 9.5 3.7 5.5#


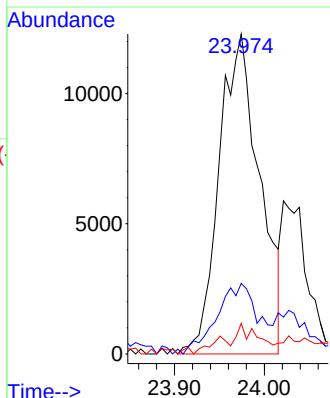
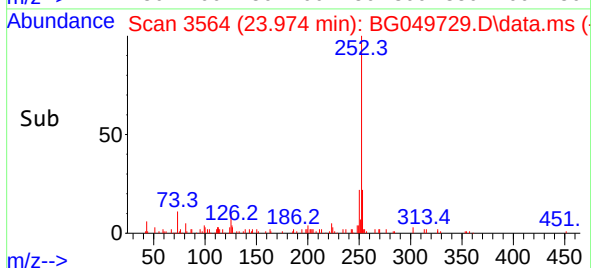


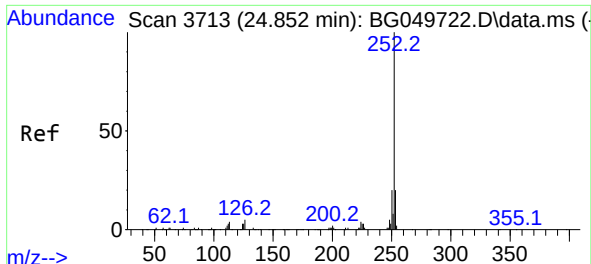


#93
Benzo(a)pyrene
Concen: 1.646 ng/ul
RT: 24.855 min Scan# 3714
Delta R.T. 0.006 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36





Tgt Ion:252 Resp: 18634
Ion Ratio Lower Upper
252 100
253 21.3 17.7 26.5
125 5.8 4.6 7.0

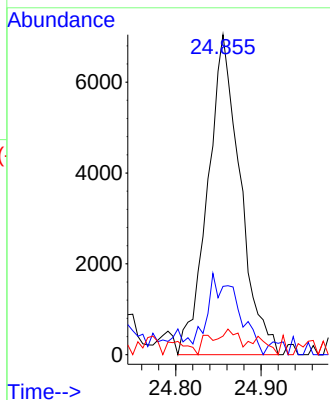

#94
Indeno(1,2,3-cd)pyrene
Concen: 1.080 ng/ul m
RT: 28.756 min Scan# 4378
Delta R.T. 0.012 min
Lab File: BG049729.D
Acq: 8 Aug 2021 8:36

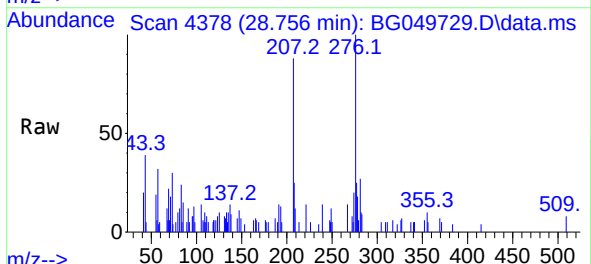

Tgt Ion:276 Resp: 16044
Ion Ratio Lower Upper
276 100
138 8.9 6.6 10.0
277 24.9 19.4 29.2

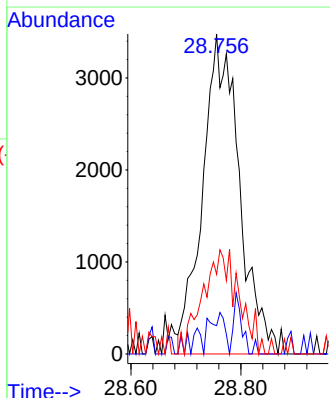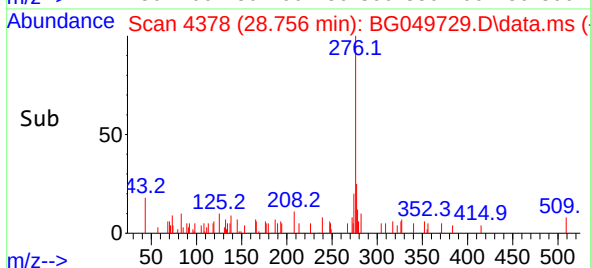

Instrument :
BNA_G
ClientSampleId :
C00F0

Manual Integrations
APPROVED

mohammad
8/9/2021 12:11:49 PM