
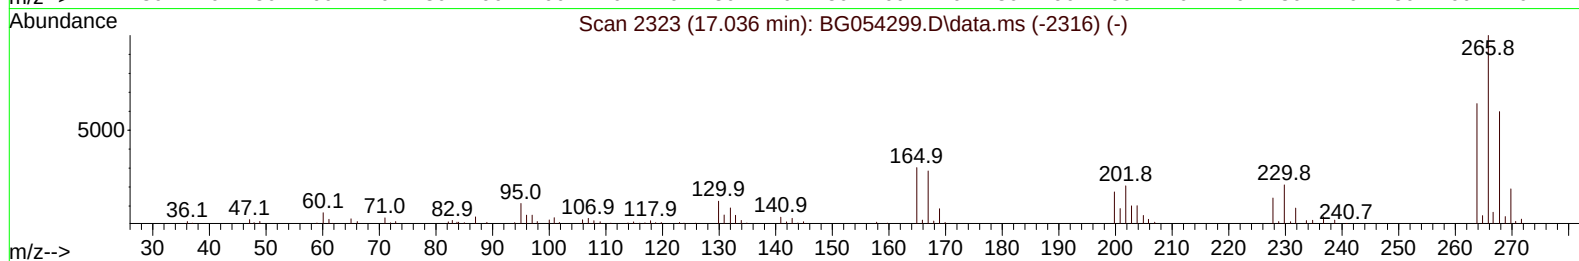
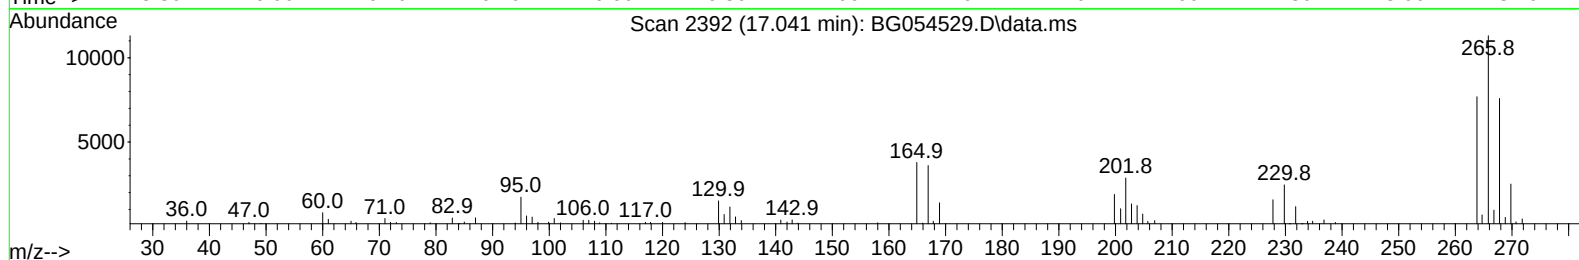


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080522\
Data File : BG054529.D
Acq On : 5 Aug 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 05:09:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

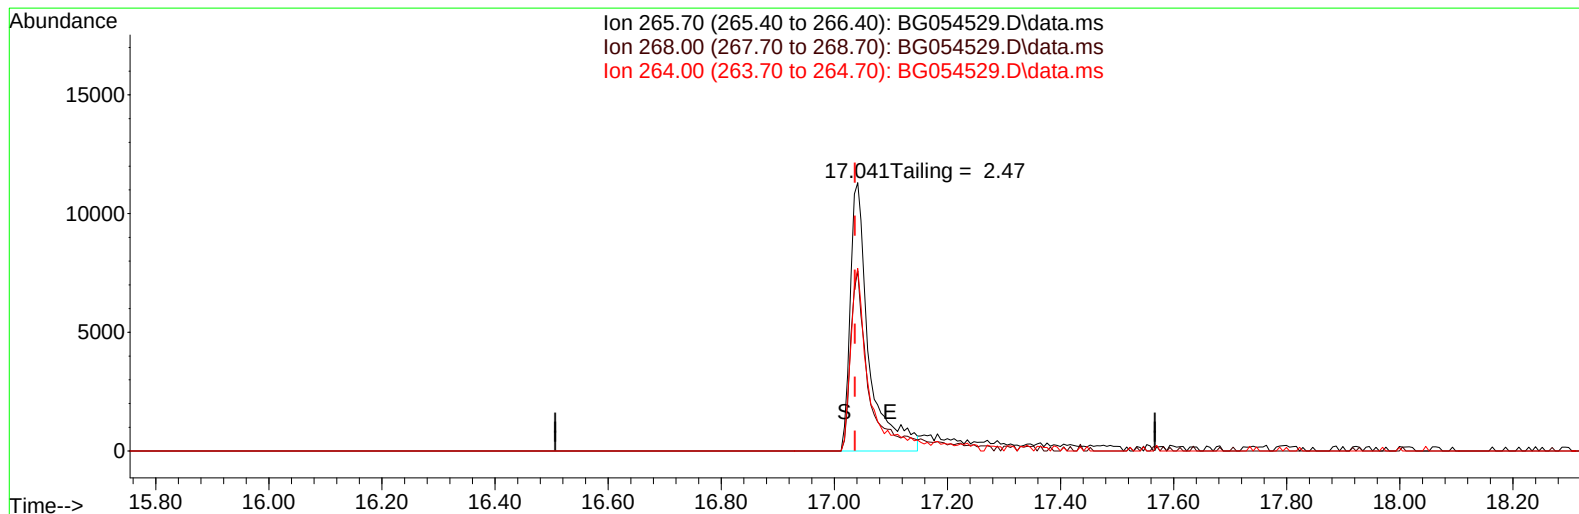

TIC: BG054529.D\data.ms

(70) Pentachlorophenol (C)




17.041min (+ 0.005) 49626.29 ng

response 24310

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.12
264.00	66.20	73.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080522\
 Data File : BG054529.D
 Acq On : 5 Aug 2022 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 05:09:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 28 04:30:50 2022
 Response via : Initial Calibration

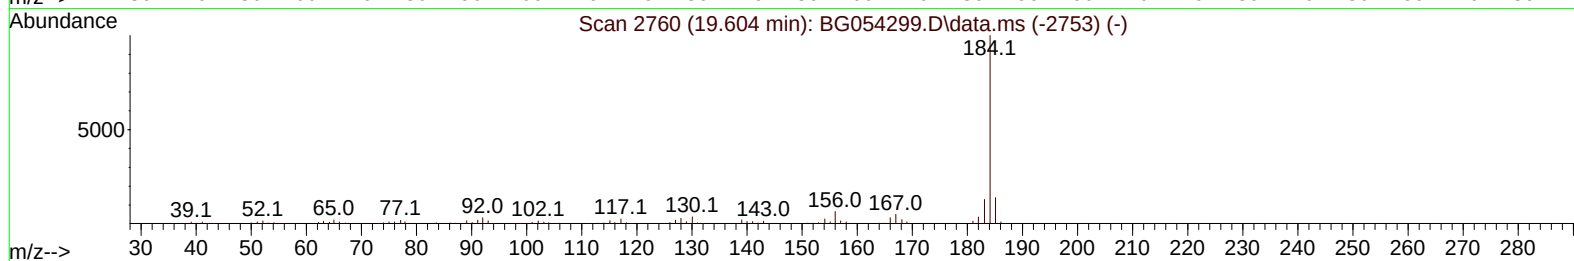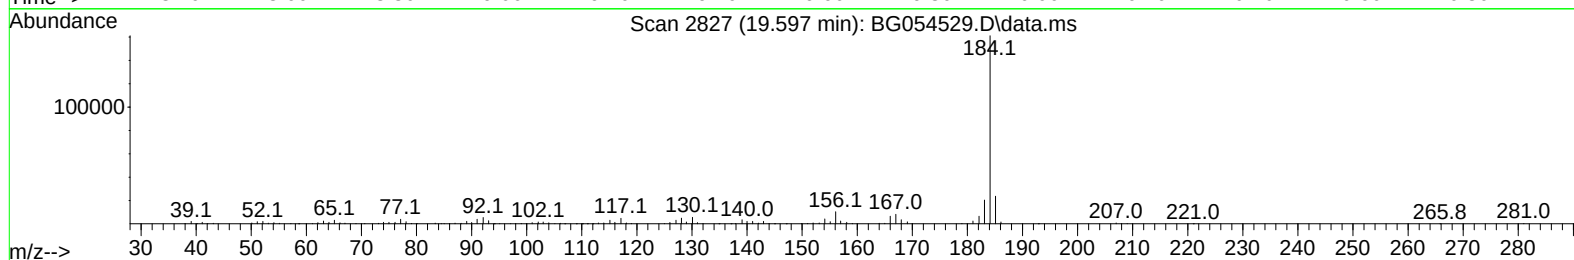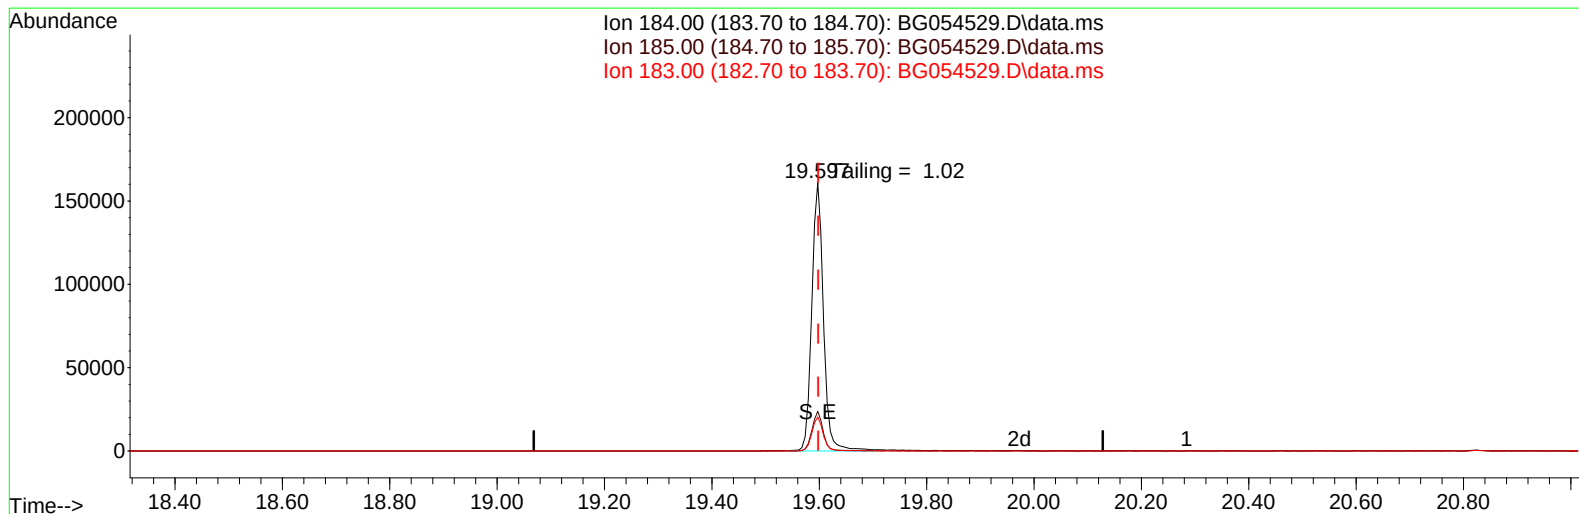

TIC: BG054529.D\data.ms

(77) Benzidine

19.597min (-0.001) 206798.00 ng m

response 250933

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.73
183.00	11.10	12.71
0.00	0.00	0.00