


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080522\
 Data File : BG054529.D
 Acq On : 5 Aug 2022 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 08 14:48:51 2022

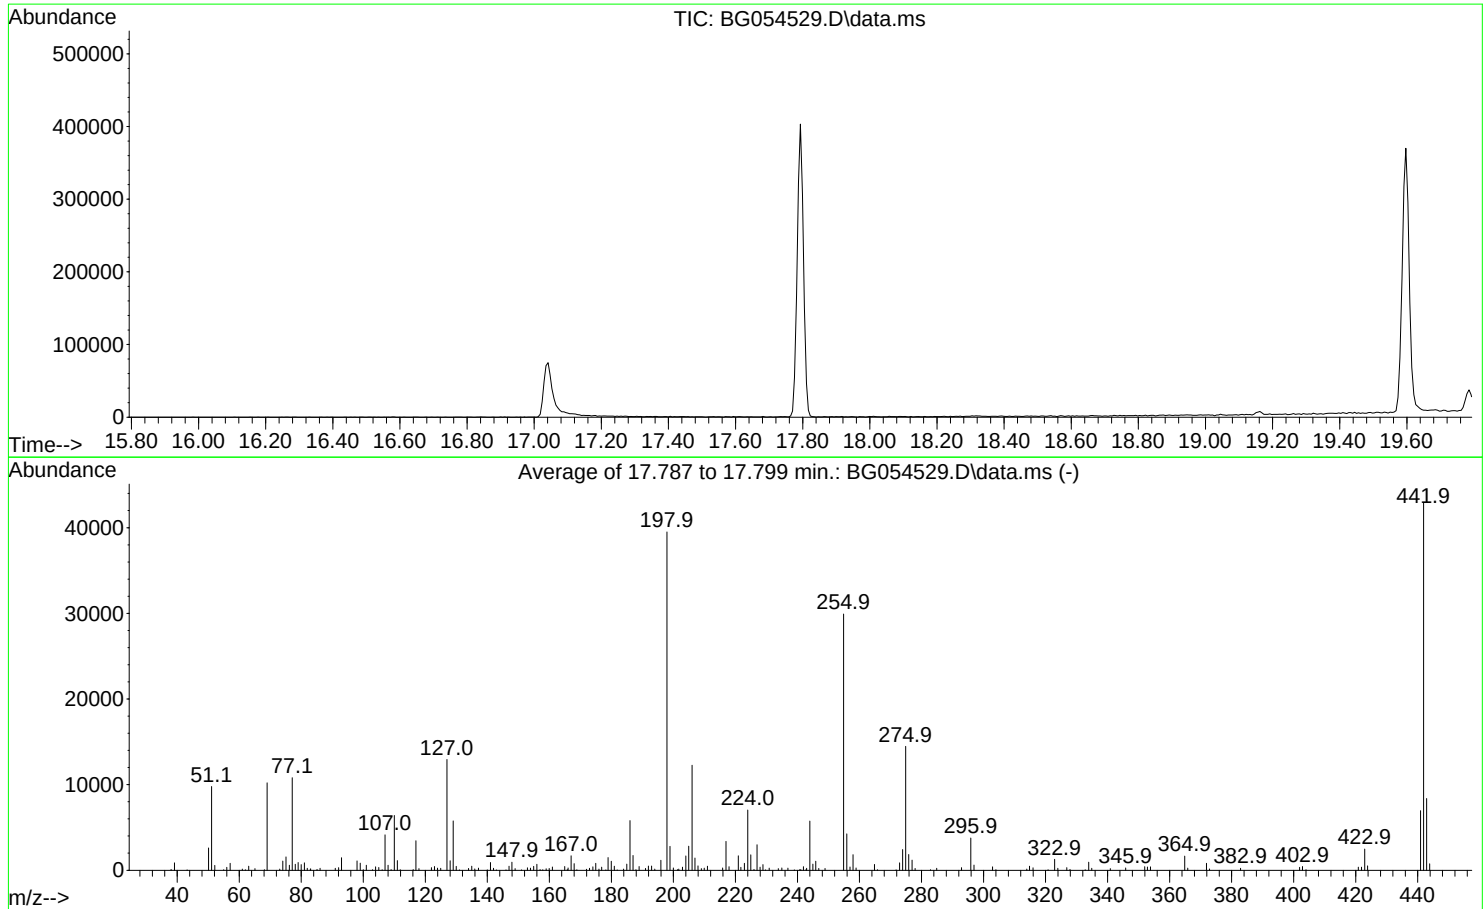




AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	9781	PASS
68	69	0.00	2	0.7	68	PASS
69	198	0.00	100	25.8	10206	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.7	12938	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39515	PASS
199	198	5	9	7.1	2801	PASS
275	198	10	60	36.6	14469	PASS
365	198	1	100	4.2	1663	PASS
441	198	0.01	100	17.6	6953	PASS
442	442	50	100	100.0	42952	PASS
443	442	15	24	19.5	8383	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080522\
Data File : BG054529.D
Acq On : 5 Aug 2022 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 08 05:09:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

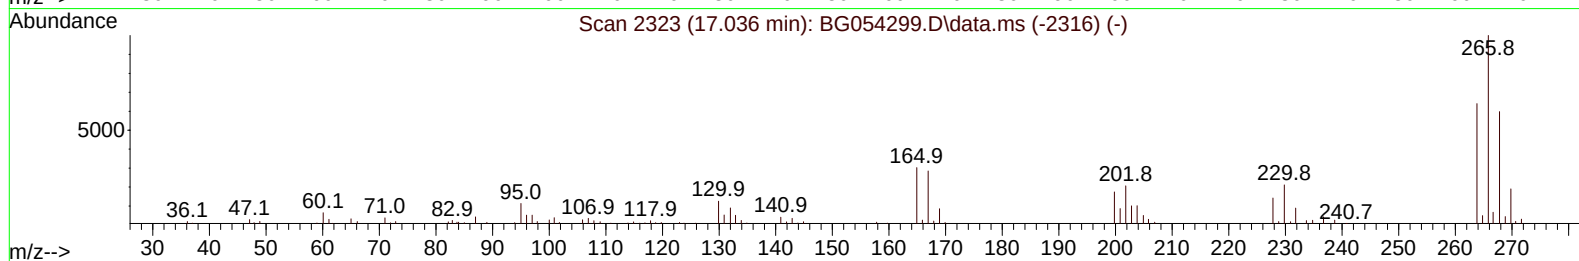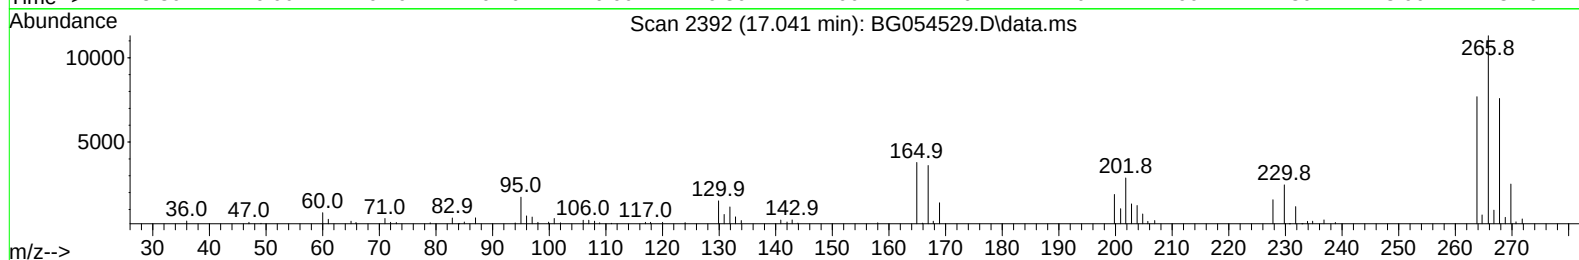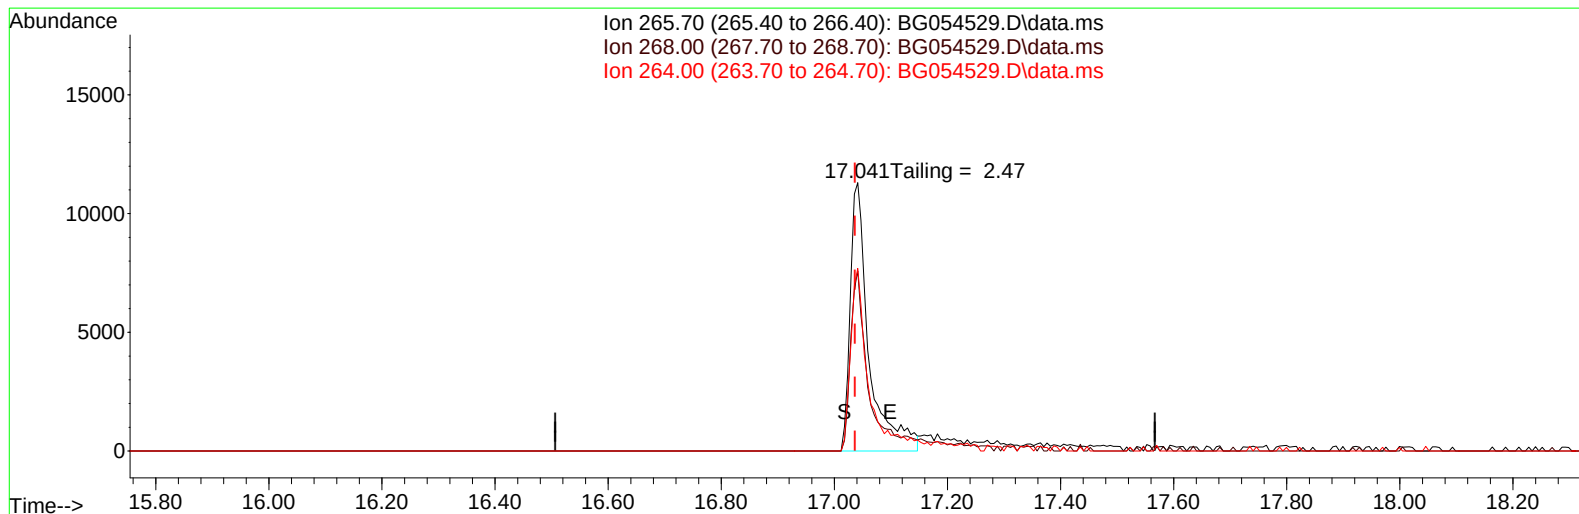

TIC: BG054529.D\data.ms

(70) Pentachlorophenol (C)

17.041min (+ 0.005) 49626.29 ng




response 24310

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.12
264.00	66.20	73.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080522\
 Data File : BG054529.D
 Acq On : 5 Aug 2022 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 08 05:09:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 28 04:30:50 2022
 Response via : Initial Calibration

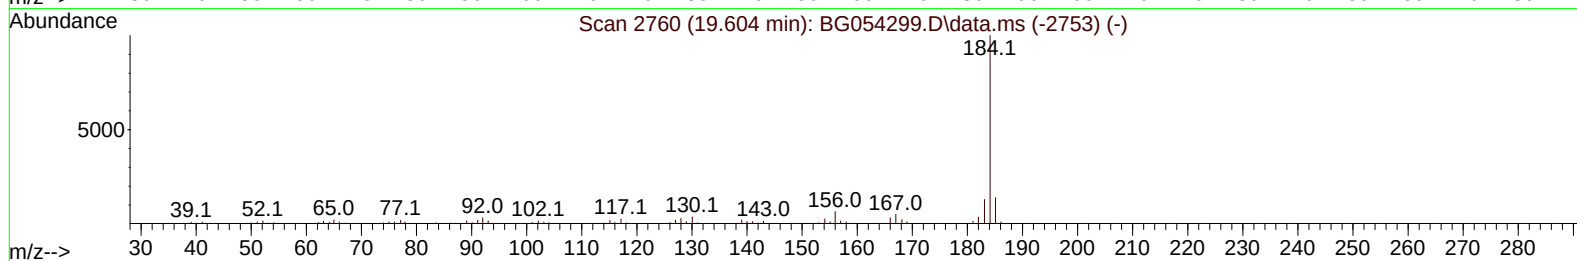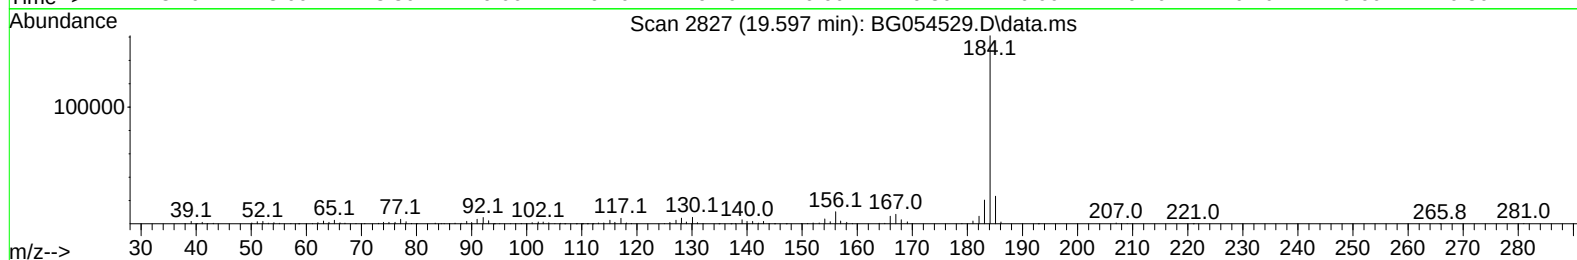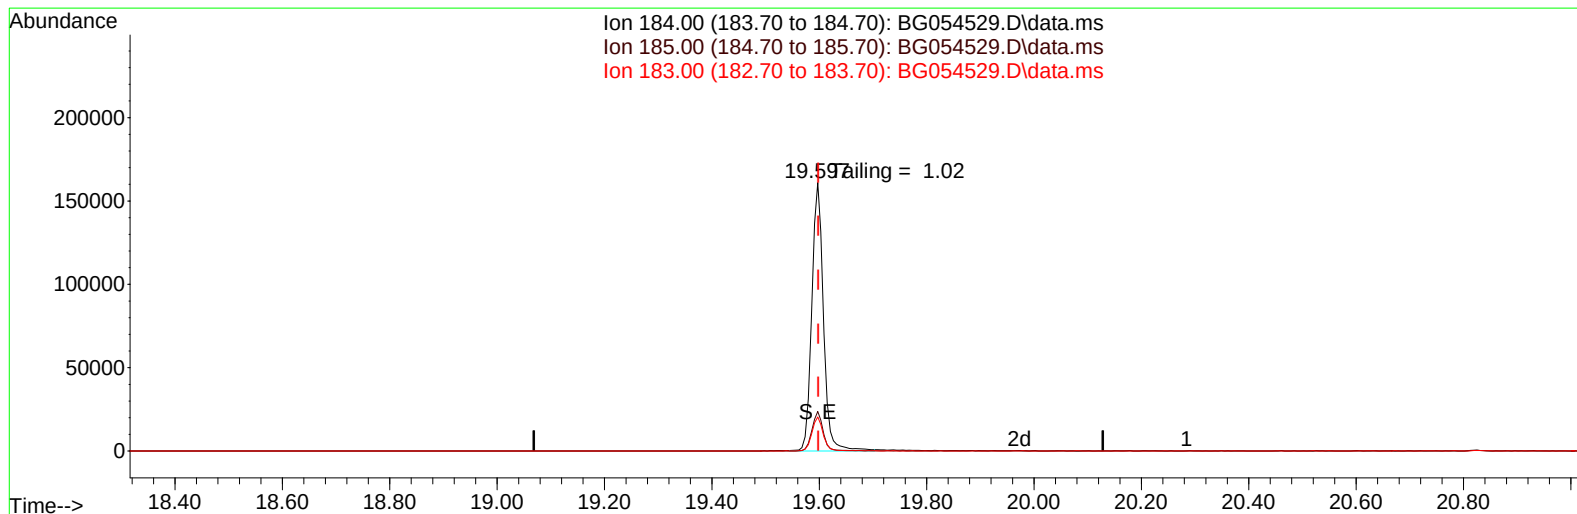

TIC: BG054529.D\data.ms

(77) Benzidine

19.597min (-0.001) 206798.00 ng m

response 250933

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.73
183.00	11.10	12.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2022	BNA_G	BG054529.D
Compound Name	Response	Retention Time
DDT	141853	20.825
DDD	5754	20.39
DDE	256	19.885
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6010	147863	4.06

Instrument :
BNA_G
ClientSampleId :
DFTPP