

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062244.D
 Acq On : 5 Aug 2024 19:21
 Operator : MA/JU
 Sample : P3361-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E20N5

Quant Time: Aug 06 02:42:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.964	152	59328	20.000	ng/ul	0.00
20) Naphthalene-d8	10.760	136	274633	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.584	164	195716	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	475305	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	465998	20.000	ng/ul	-0.01
88) Perylene-d12	24.665	264	538044	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.429	96	7299	5.305	ng/uL	0.00
4) Pyridine-d5	3.828	84	119937	27.708	ng/ul	0.00
7) Phenol-d5	7.118	99	188804	33.342	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.294	67	114304	32.791	ng/ul	0.00
11) 2-Chlorophenol-d4	7.494	132	132673	32.701	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	154890	32.839	ng/ul	0.00
21) Nitrobenzene-d5	9.115	128	65371	38.603	ng/ul	0.00
24) 2-Nitrophenol-d4	9.838	143	65519	41.129	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.372	165	155035	33.508	ng/ul	0.00
31) 4-Chloroaniline-d4	10.883	131	212208	31.622	ng/ul	0.00
46) Dimethylphthalate-d6	13.997	166	517163	34.249	ng/ul	0.00
49) Acenaphthylene-d8	14.279	160	587350	34.306	ng/ul	0.00
54) 4-Nitrophenol-d4	14.755	143	68221	32.271	ng/ul	0.00
60) Fluorene-d10	15.577	176	506040	37.335	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.683	200	41907	29.771	ng/ul	0.00
73) Anthracene-d10	17.422	188	752813	32.838	ng/ul	0.00
81) Pyrene-d10	19.707	212	944304	34.093	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.453	264	987950	34.349	ng/ul	-0.01


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.657	70	4020	1.007 ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062244.D
Acq On : 5 Aug 2024 19:21
Operator : MA/JU
Sample : P3361-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20N5

Quant Time: Aug 06 02:42:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

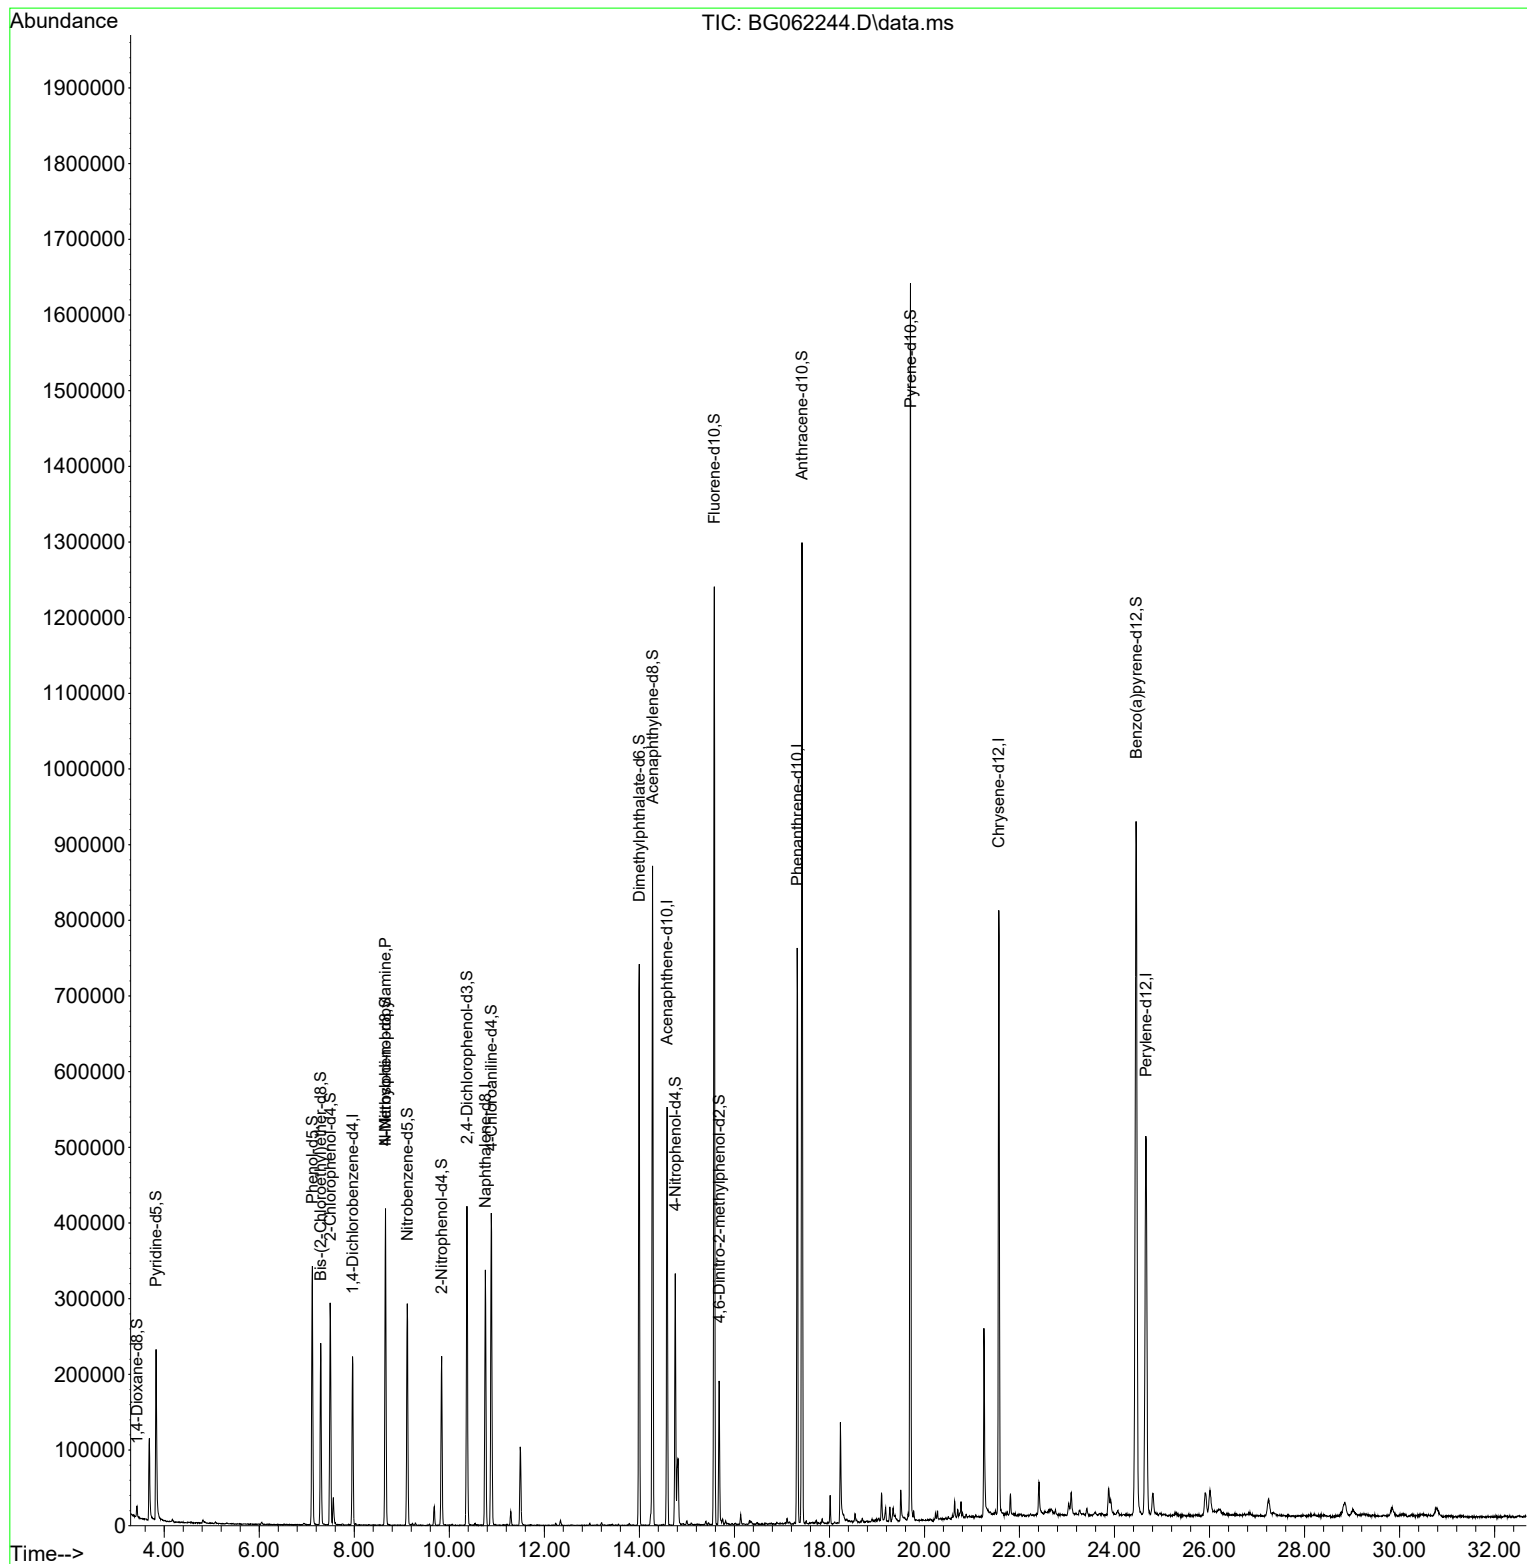

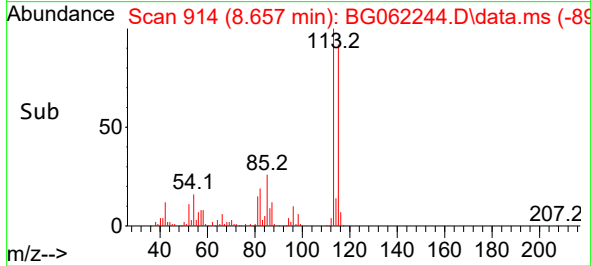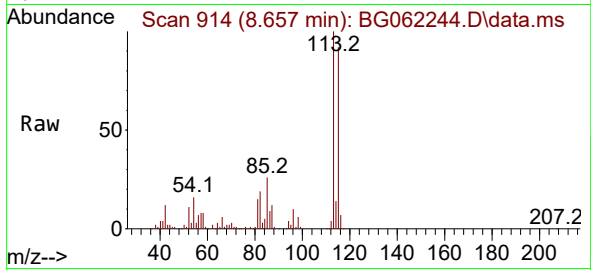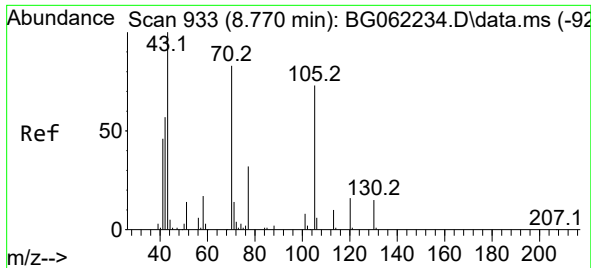

#17
N-Nitroso-di-n-propylamine
Concen: 1.007 ng/ul
RT: 8.657 min Scan# 91
Delta R.T. -0.113 min
Lab File: BG062244.D
Acq: 5 Aug 2024 19:21

Instrument :
BNA_G
ClientSampleId :
E20N5

Tgt Ion: 70	Resp: 4020
Ion Ratio	Lower Upper
70	100
42	456.1 55.4 83.0#
101	0.0 7.4 11.0#
130	0.0 13.9 20.9#

