




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062243.D
 Acq On : 5 Aug 2024 18:39
 Operator : MA/JU
 Sample : P3361-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E20N3

Manual IntegrationsAPPROVED

Quant Time: Aug 06 02:42:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/08/2024

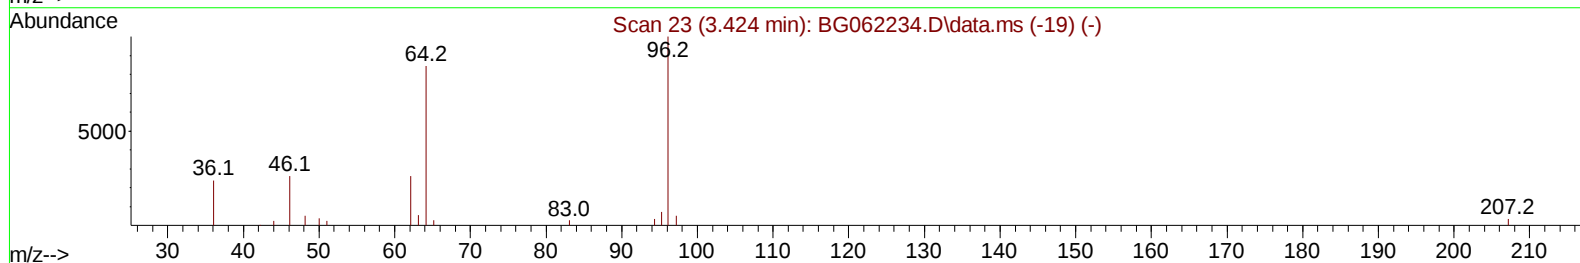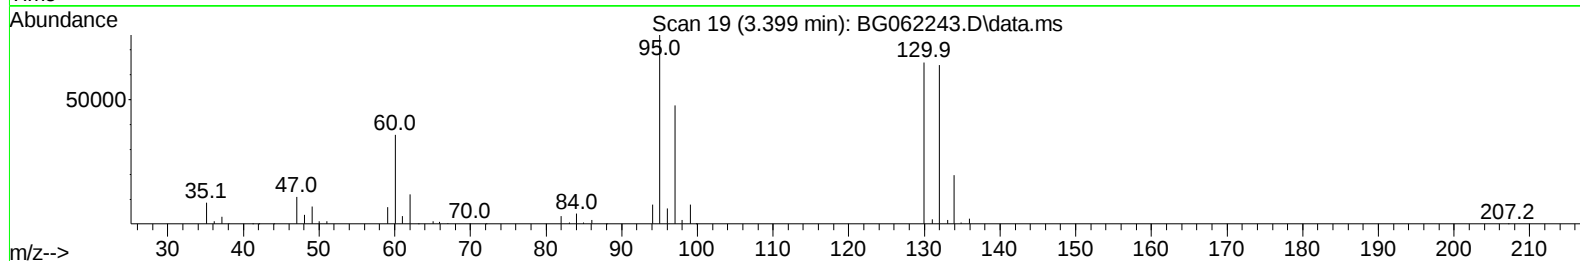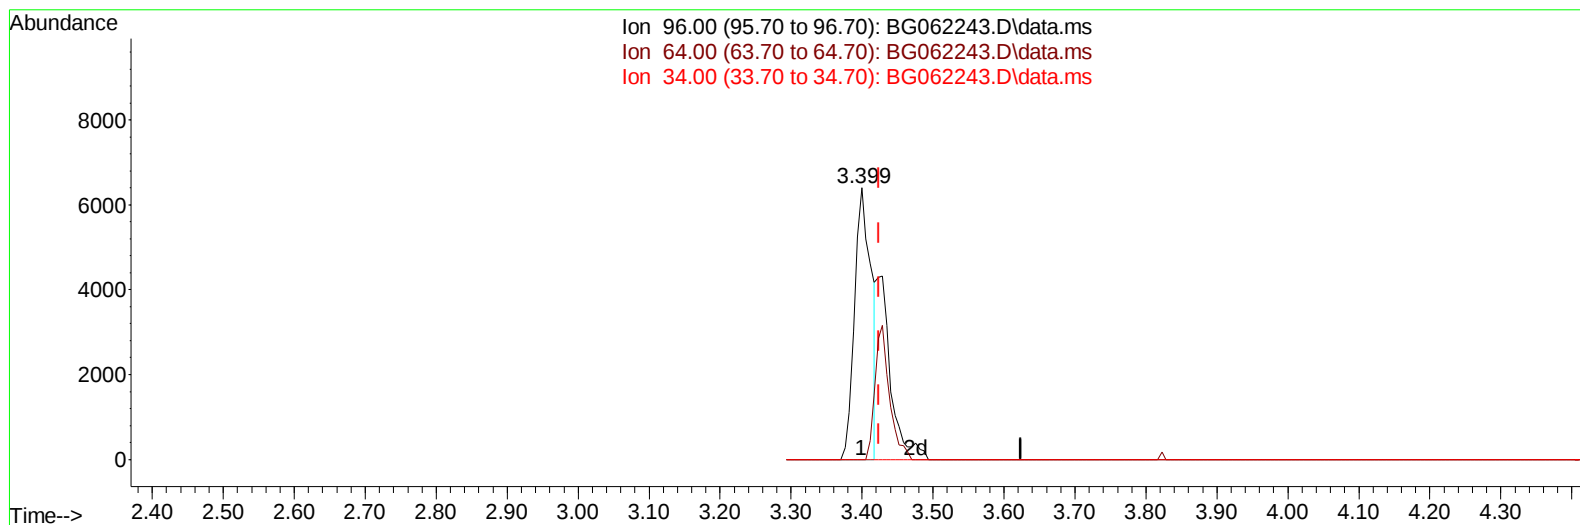

TIC: BG062243.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.399min (-0.025) 7.34 ng/uL

response 10578

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062243.D
Acq On : 5 Aug 2024 18:39
Operator : MA/JU
Sample : P3361-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20N3

Manual IntegrationsAPPROVED

Quant Time: Aug 06 02:42:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

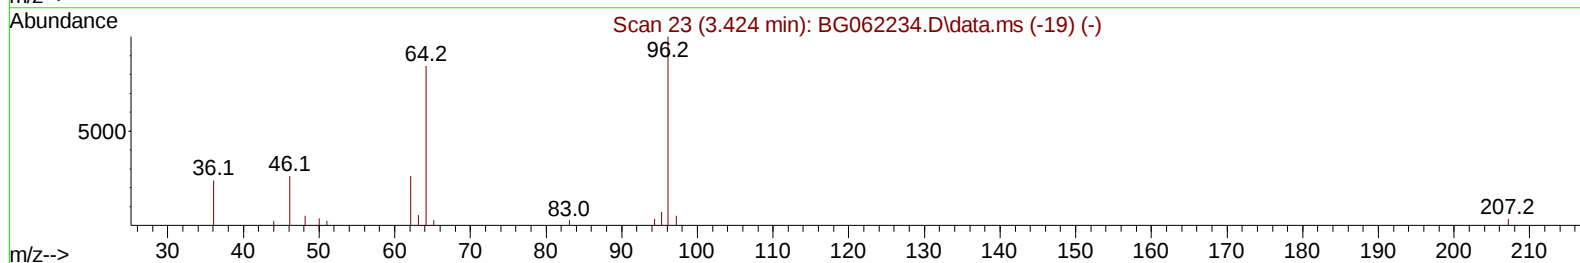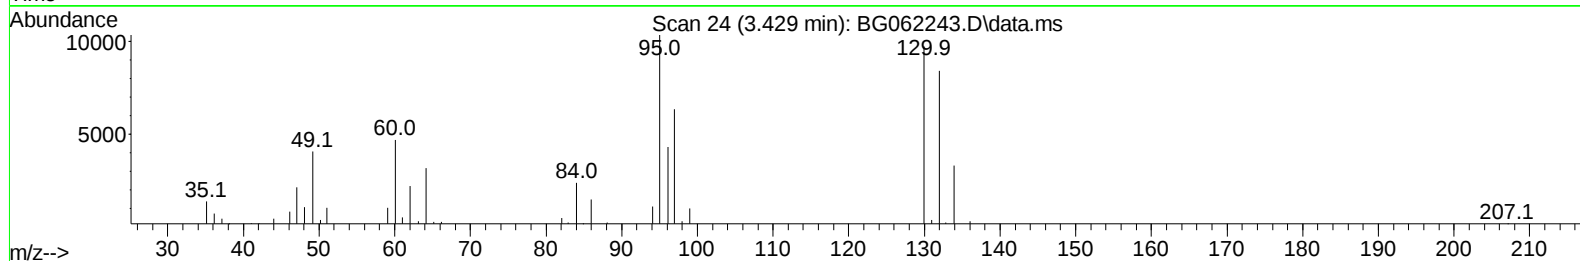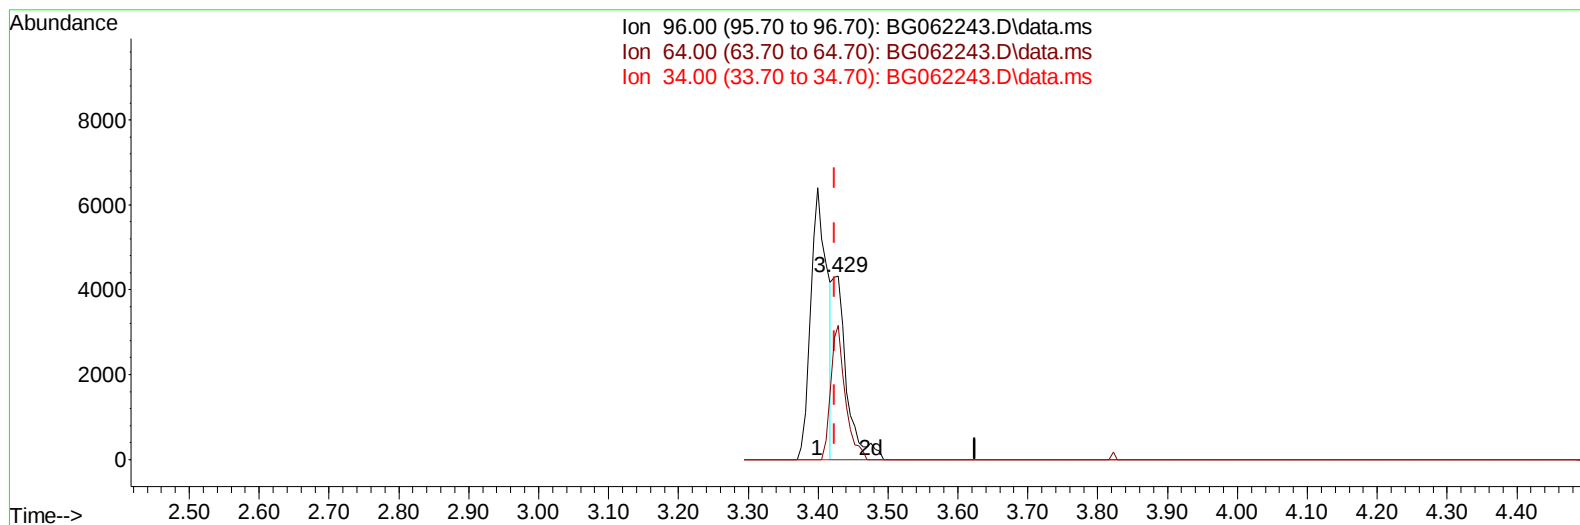

TIC: BG062243.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.429min (+ 0.005) 4.16 ng/uL m

response 6001

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	73.23
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062243.D
 Acq On : 5 Aug 2024 18:39
 Operator : MA/JU
 Sample : P3361-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E20N3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 06 03:00:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.964	152	62145	20.000	ng/ul	0.00
20) Naphthalene-d8	10.760	136	284678	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.584	164	216087	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	494694	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	482643	20.000	ng/ul	-0.01
88) Perylene-d12	24.665	264	563507	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.429	96	6001m	4.164	ng/uL	0.00
4) Pyridine-d5	3.828	84	84648	18.669	ng/ul	0.00
7) Phenol-d5	7.118	99	142992	24.107	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.294	67	87574	23.984	ng/ul	0.00
11) 2-Chlorophenol-d4	7.494	132	100099	23.554	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	122731	24.841	ng/ul	0.00
21) Nitrobenzene-d5	9.115	128	48448	27.600	ng/ul	0.00
24) 2-Nitrophenol-d4	9.838	143	48927	29.630	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.372	165	118979	24.808	ng/ul	0.00
31) 4-Chloroaniline-d4	10.883	131	175597	25.243	ng/ul	0.00
46) Dimethylphthalate-d6	13.997	166	459397	27.555	ng/ul	0.00
49) Acenaphthylene-d8	14.279	160	499393	26.419	ng/ul	0.00
54) 4-Nitrophenol-d4	14.760	143	57822	24.773	ng/ul	0.00
60) Fluorene-d10	15.577	176	437923	29.264	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.677	200	31210	21.303	ng/ul	0.00
73) Anthracene-d10	17.422	188	687480	28.813	ng/ul	0.00
81) Pyrene-d10	19.707	212	849598	29.616	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.453	264	902501	29.960	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062243.D
Acq On : 5 Aug 2024 18:39
Operator : MA/JU
Sample : P3361-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20N3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 06 03:00:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

