




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062246.D
Acq On : 5 Aug 2024 20:45
Operator : MA/JU
Sample : P3361-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20N8

Manual IntegrationsAPPROVED

Quant Time: Aug 06 02:42:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

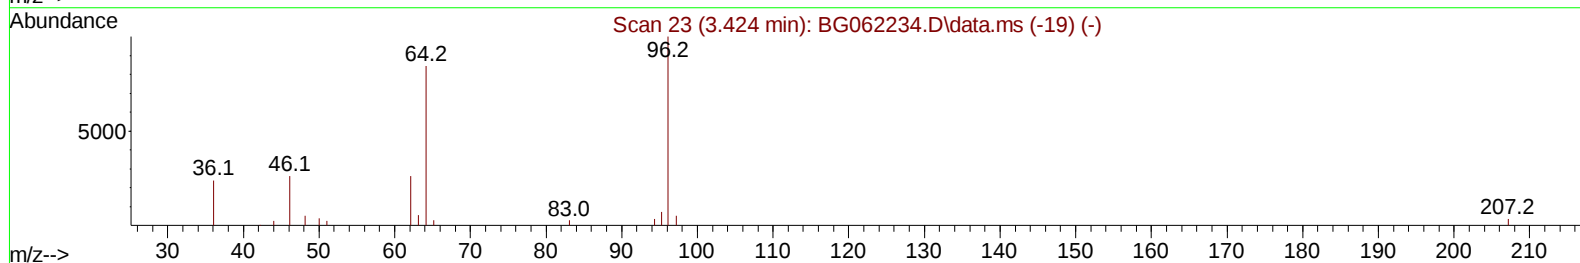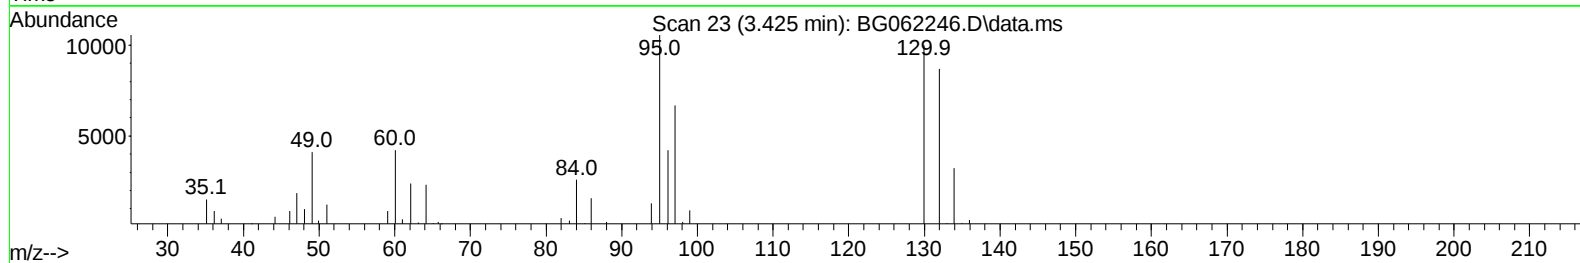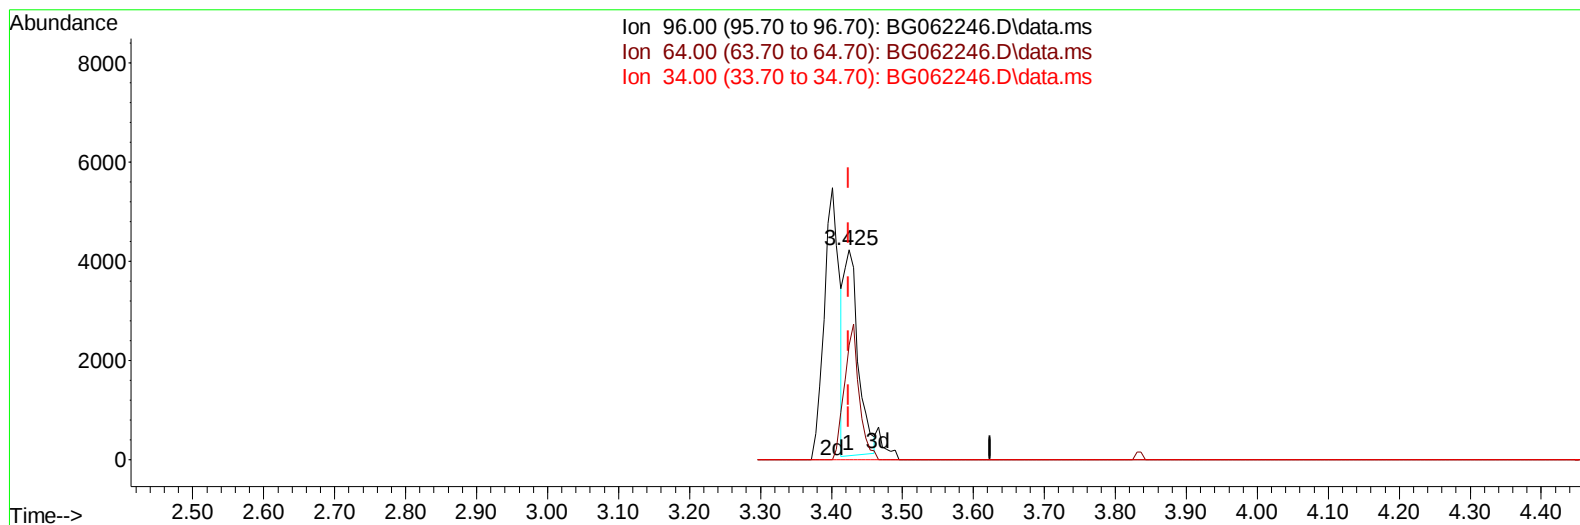

TIC: BG062246.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.425min (+ 0.001) 4.42 ng/uL

response 5760

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	54.47#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062246.D
 Acq On : 5 Aug 2024 20:45
 Operator : MA/JU
 Sample : P3361-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E20N8

Manual IntegrationsAPPROVED

Quant Time: Aug 06 02:42:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/08/2024

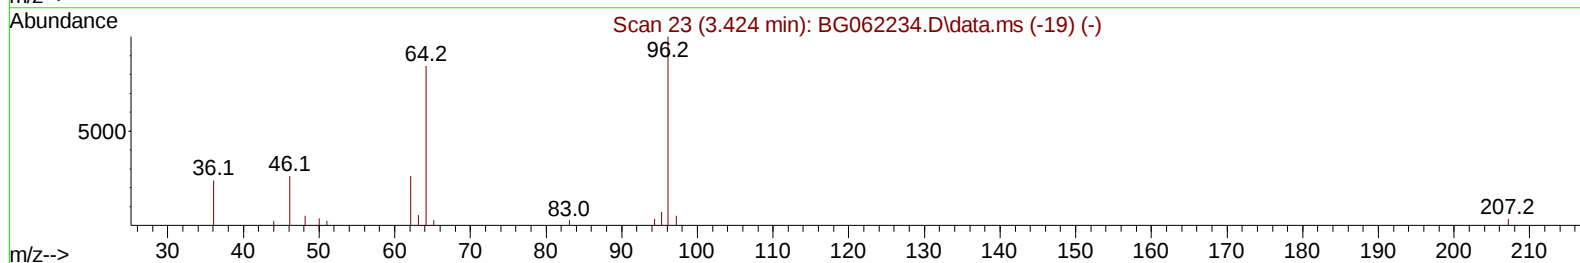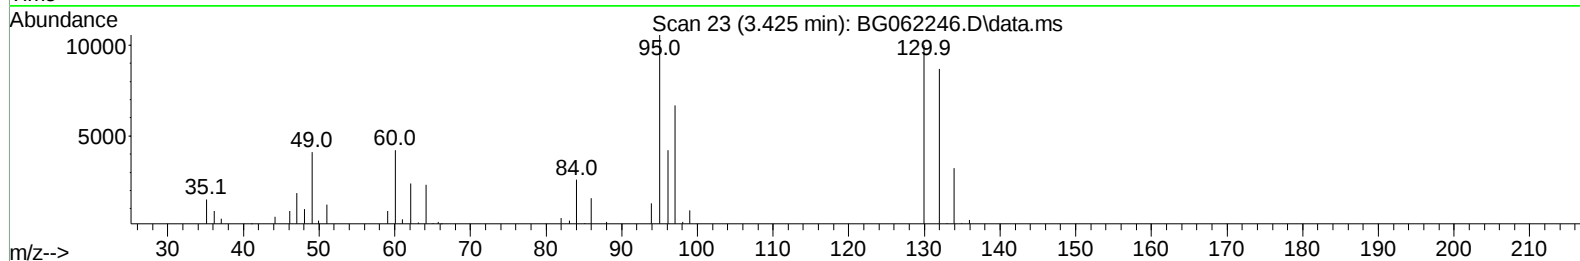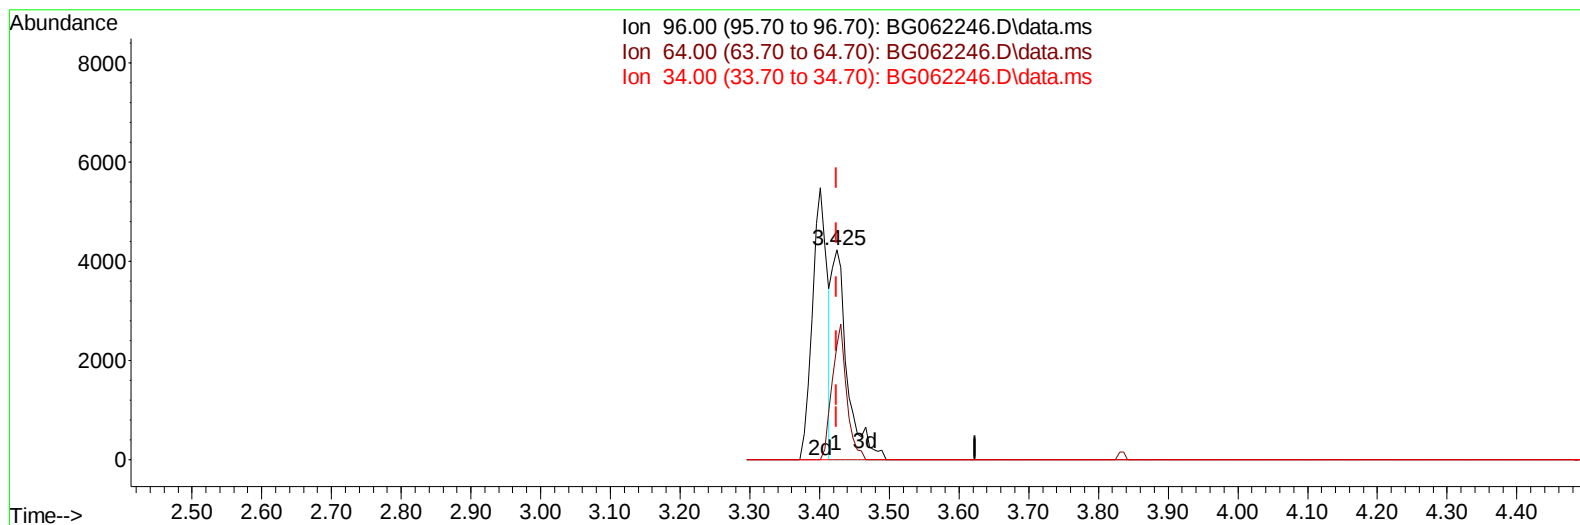

TIC: BG062246.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.425min (+ 0.001) 5.02 ng/uL m

response 6541

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	54.47#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062246.D
 Acq On : 5 Aug 2024 20:45
 Operator : MA/JU
 Sample : P3361-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E20N8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 06 03:05:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	56200	20.000	ng/ul	0.00
20) Naphthalene-d8	10.762	136	256768	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	193732	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.324	188	446818	20.000	ng/ul	0.00
79) Chrysene-d12	21.565	240	429582	20.000	ng/ul	-0.01
88) Perylene-d12	24.667	264	504766	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.425	96	6541m	5.019	ng/uL	0.00
4) Pyridine-d5	3.830	84	74915	18.270	ng/ul	0.00
7) Phenol-d5	7.114	99	116414	21.702	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.290	67	72248	21.880	ng/ul	0.00
11) 2-Chlorophenol-d4	7.496	132	81988	21.333	ng/ul	0.00
15) 4-Methylphenol-d8	8.659	113	98107	21.958	ng/ul	0.00
21) Nitrobenzene-d5	9.117	128	40409	25.522	ng/ul	0.00
24) 2-Nitrophenol-d4	9.840	143	40440	27.152	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.374	165	96346	22.272	ng/ul	0.00
31) 4-Chloroaniline-d4	10.885	131	139142	22.177	ng/ul	0.00
46) Dimethylphthalate-d6	13.993	166	341591	22.853	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160	385413	22.742	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	43261	20.673	ng/ul	0.00
60) Fluorene-d10	15.573	176	334609	24.940	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.679	200	22562	17.050	ng/ul	0.00
73) Anthracene-d10	17.423	188	506654	23.510	ng/ul	0.00
81) Pyrene-d10	19.703	212	626781	24.548	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.449	264	639269	23.691	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062246.D
Acq On : 5 Aug 2024 20:45
Operator : MA/JU
Sample : P3361-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20N8

Manual IntegrationsAPPROVED

Quant Time: Aug 06 03:05:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

