




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062252.D
Acq On : 6 Aug 2024 00:55
Operator : MA/JU
Sample : P3361-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20P4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 06 04:20:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

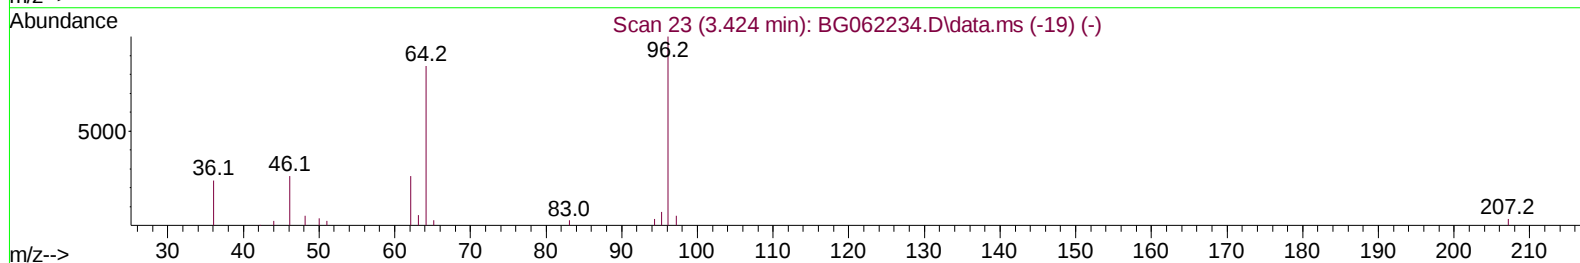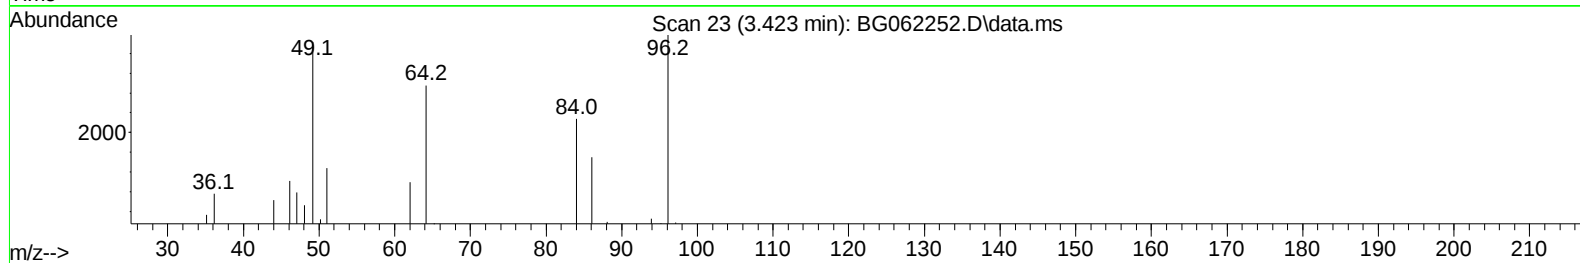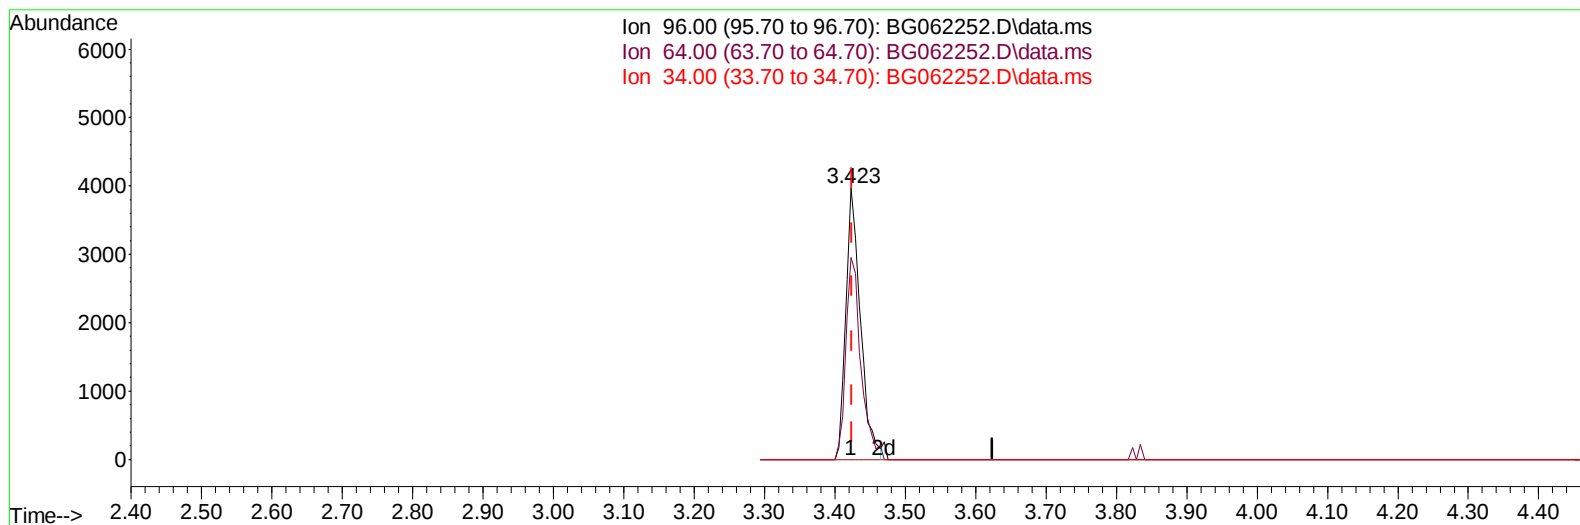

TIC: BG062252.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.423min (-0.001) 4.44 ng/uL

response 5698

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	74.41
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062252.D
 Acq On : 6 Aug 2024 00:55
 Operator : MA/JU
 Sample : P3361-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E20P4

Manual IntegrationsAPPROVED

Quant Time: Aug 06 04:20:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/08/2024

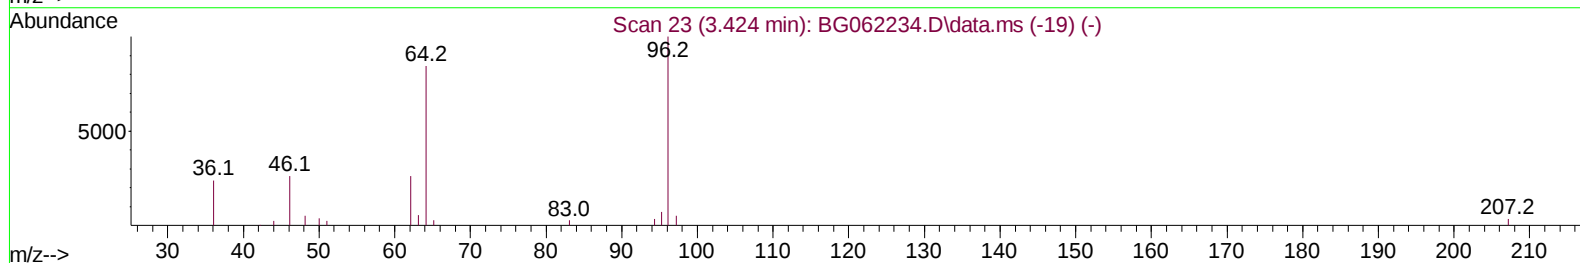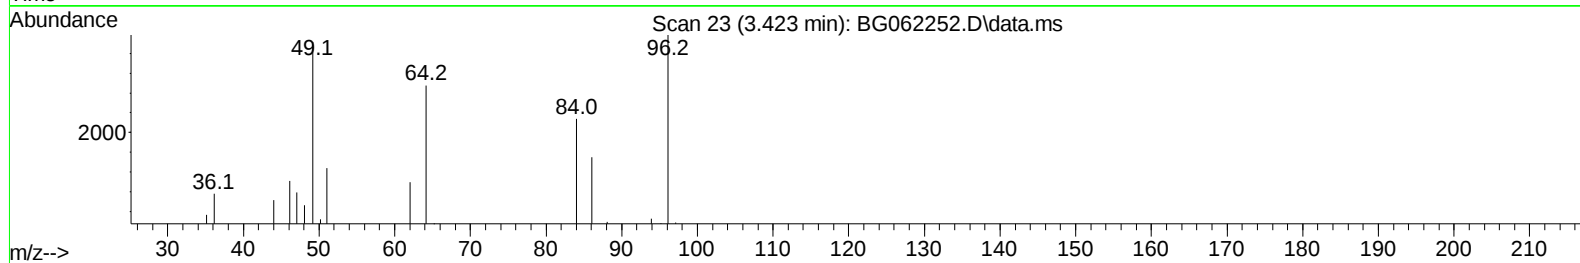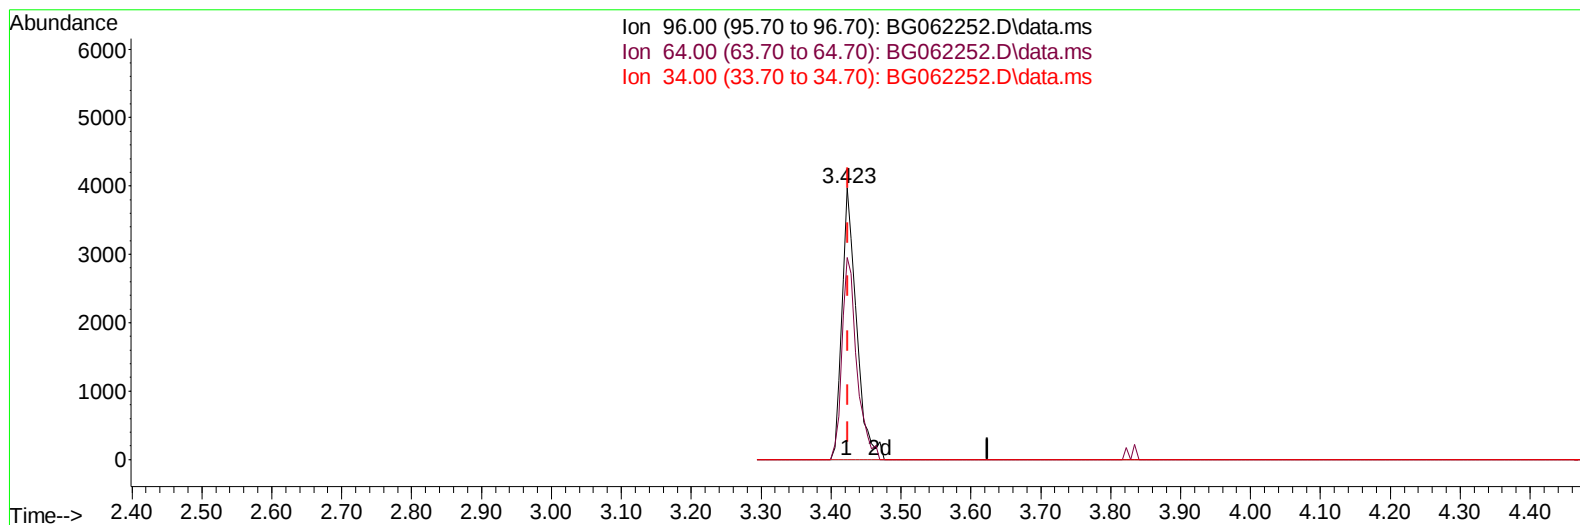

TIC: BG062252.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.423min (-0.001) 4.51 ng/uL m

response 5789

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	74.41
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062252.D
 Acq On : 6 Aug 2024 00:55
 Operator : MA/JU
 Sample : P3361-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E20P4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 06 04:25:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.964	152	55337	20.000	ng/ul	0.00
20) Naphthalene-d8	10.760	136	262774	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.584	164	203157	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	461486	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	454830	20.000	ng/ul	-0.01
88) Perylene-d12	24.659	264	526504	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.423	96	5789m	4.511	ng/uL	0.00
4) Pyridine-d5	3.828	84	91239	22.598	ng/ul	0.00
7) Phenol-d5	7.112	99	139190	26.353	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.294	67	86635	26.646	ng/ul	0.00
11) 2-Chlorophenol-d4	7.494	132	103566	27.368	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	117687	26.751	ng/ul	0.00
21) Nitrobenzene-d5	9.115	128	49019	30.253	ng/ul	0.00
24) 2-Nitrophenol-d4	9.832	143	51864	34.026	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.372	165	116770	26.376	ng/ul	0.00
31) 4-Chloroaniline-d4	10.884	131	167473	26.082	ng/ul	0.00
46) Dimethylphthalate-d6	13.991	166	420717	26.841	ng/ul	0.00
49) Acenaphthylene-d8	14.273	160	478128	26.904	ng/ul	0.00
54) 4-Nitrophenol-d4	14.755	143	56146	25.586	ng/ul	0.00
60) Fluorene-d10	15.577	176	385537	27.403	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.677	200	33042	24.176	ng/ul	0.00
73) Anthracene-d10	17.422	188	608856	27.354	ng/ul	0.00
81) Pyrene-d10	19.701	212	744386	27.535	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.448	264	786982	27.961	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062252.D
Acq On : 6 Aug 2024 00:55
Operator : MA/JU
Sample : P3361-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20P4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 06 04:25:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

