




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062259.D
Acq On : 6 Aug 2024 6:26
Operator : MA/JU
Sample : P3361-23
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20Q3

Manual IntegrationsAPPROVED

Quant Time: Aug 06 07:01:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

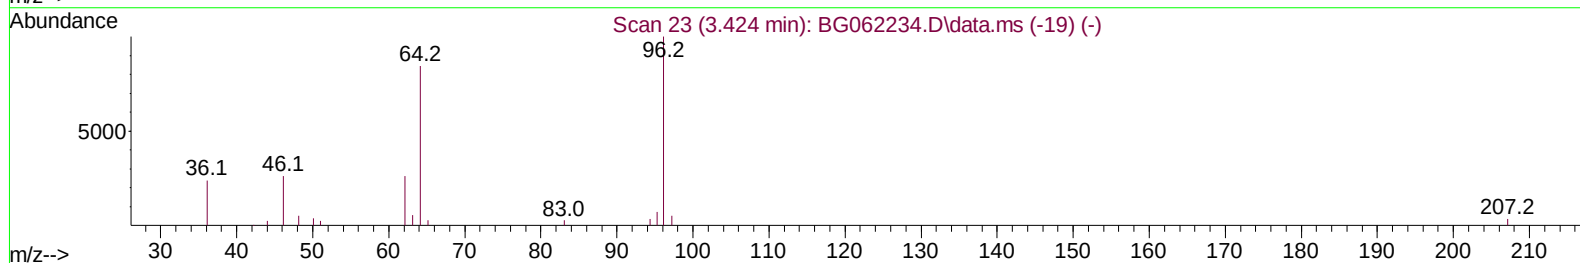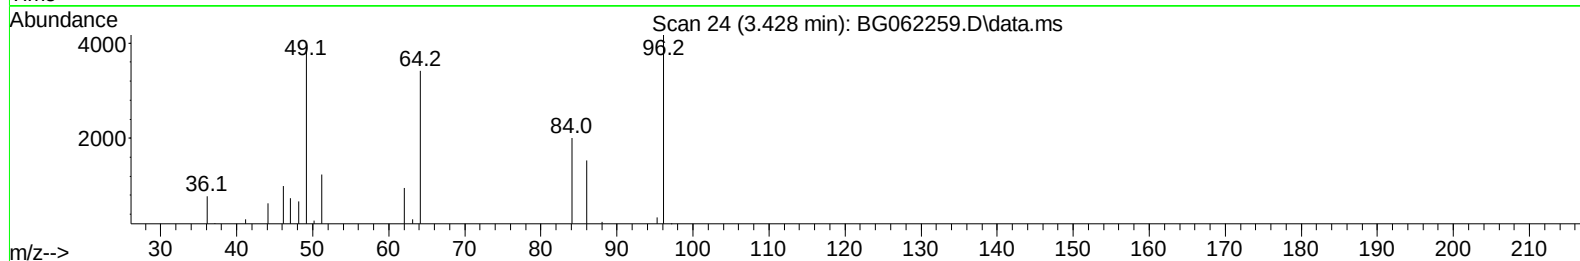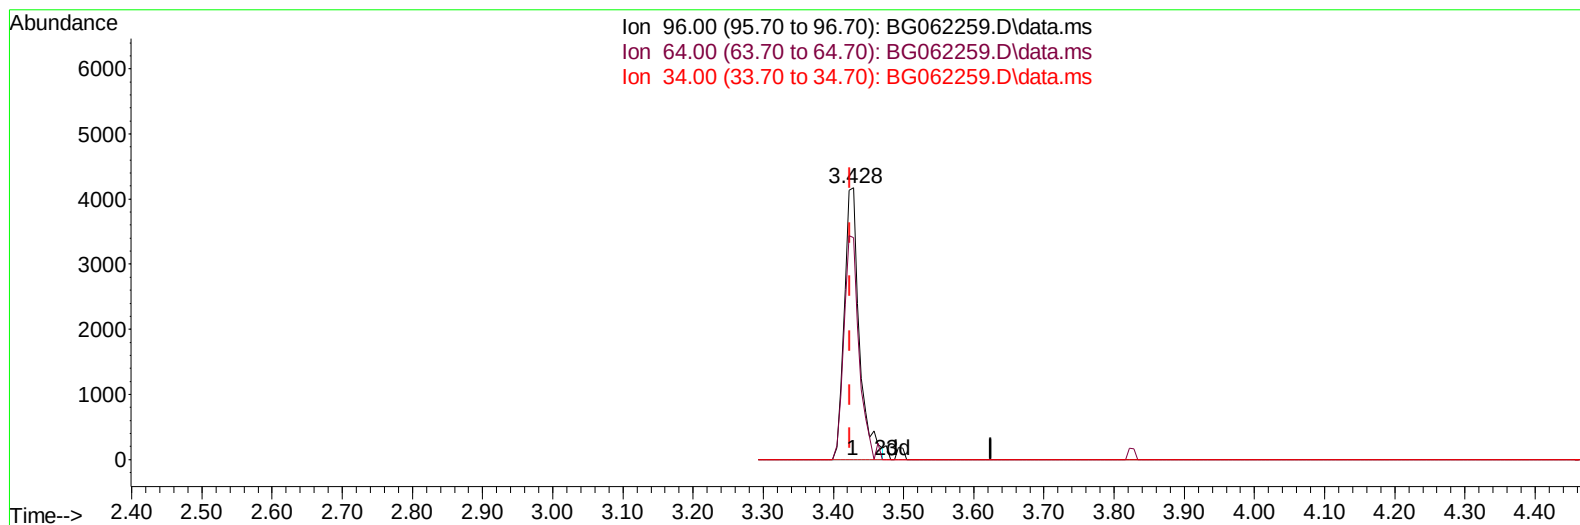

TIC: BG062259.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.428min (+ 0.004) 4.12 ng/uL

response 6250

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	81.78
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062259.D
Acq On : 6 Aug 2024 6:26
Operator : MA/JU
Sample : P3361-23
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20Q3

Manual IntegrationsAPPROVED

Quant Time: Aug 06 07:01:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

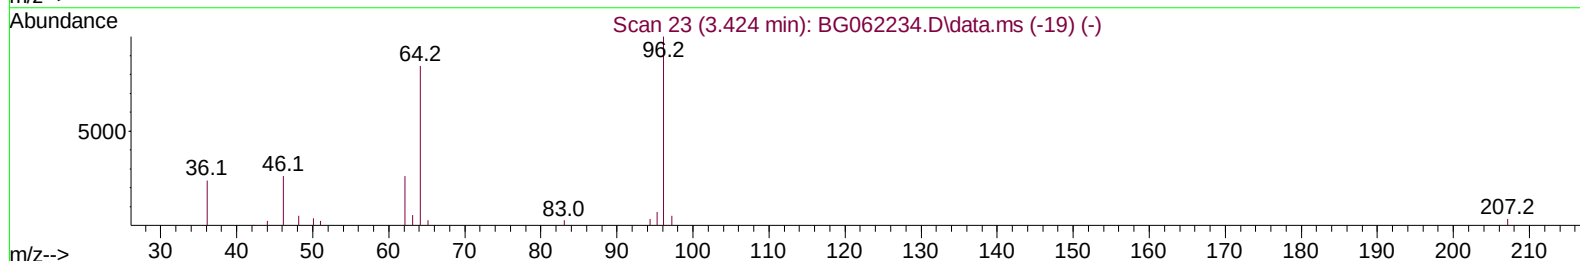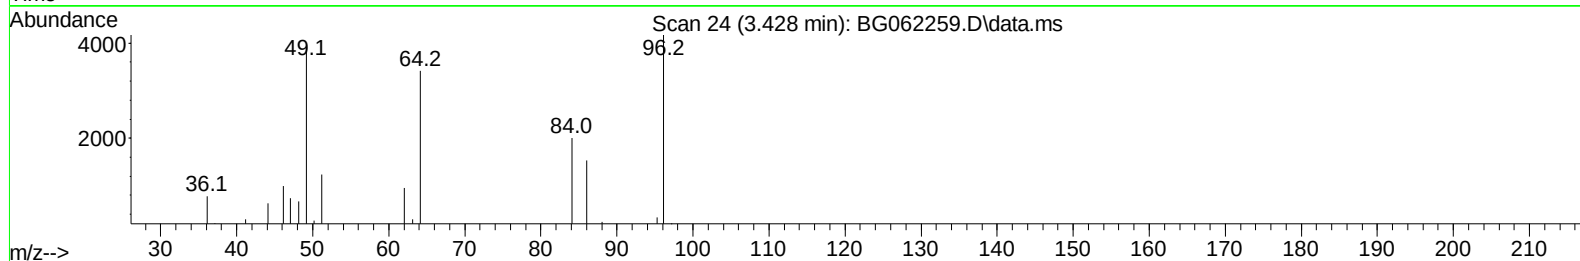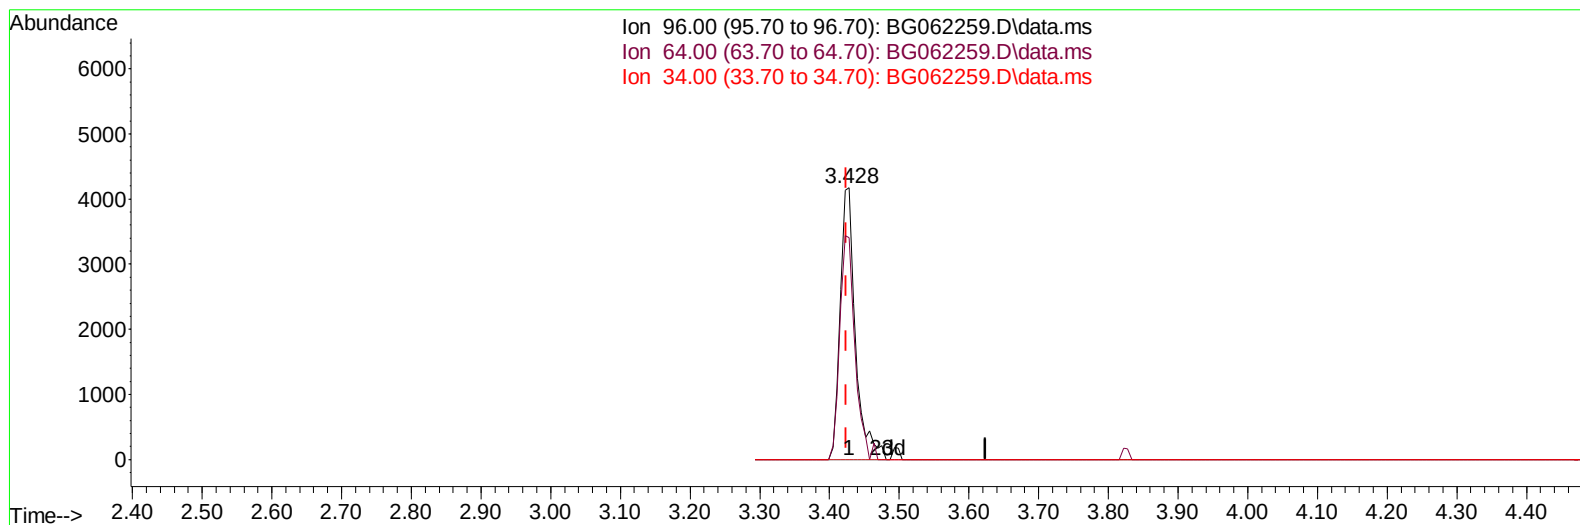

TIC: BG062259.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.428min (+ 0.004) 4.17 ng/uL m

response 6323

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	81.78
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062259.D
 Acq On : 6 Aug 2024 6:26
 Operator : MA/JU
 Sample : P3361-23
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E20Q3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 06 07:01:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	65377	20.000	ng/ul	0.00
20) Naphthalene-d8	10.760	136	309576	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.584	164	244822	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.321	188	543415	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	525628	20.000	ng/ul	-0.01
88) Perylene-d12	24.658	264	611654	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	6323m	4.170	ng/uL	0.00
4) Pyridine-d5	3.828	84	97946	20.534	ng/ul	0.00
7) Phenol-d5	7.112	99	142220	22.791	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.294	67	89561	23.316	ng/ul	0.00
11) 2-Chlorophenol-d4	7.493	132	104697	23.418	ng/ul	0.00
15) 4-Methylphenol-d8	8.656	113	119515	22.994	ng/ul	0.00
21) Nitrobenzene-d5	9.115	128	51361	26.906	ng/ul	0.00
24) 2-Nitrophenol-d4	9.831	143	51895	28.899	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.372	165	119688	22.948	ng/ul	0.00
31) 4-Chloroaniline-d4	10.883	131	174003	23.002	ng/ul	0.00
46) Dimethylphthalate-d6	13.990	166	433348	22.942	ng/ul	0.00
49) Acenaphthylene-d8	14.272	160	494597	23.094	ng/ul	0.00
54) 4-Nitrophenol-d4	14.754	143	53022	20.050	ng/ul	0.00
60) Fluorene-d10	15.577	176	394960	23.295	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.676	200	30870	19.182	ng/ul	0.00
73) Anthracene-d10	17.421	188	609139	23.241	ng/ul	0.00
81) Pyrene-d10	19.700	212	734789	23.519	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.447	264	772331	23.620	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062259.D
Acq On : 6 Aug 2024 6:26
Operator : MA/JU
Sample : P3361-23
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20Q3

Manual IntegrationsAPPROVED

Quant Time: Aug 06 07:01:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

