




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062272.D
Acq On : 6 Aug 2024 16:07
Operator : MA/JU
Sample : P3328-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1ZT4

Manual IntegrationsAPPROVED

Quant Time: Aug 06 16:40:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

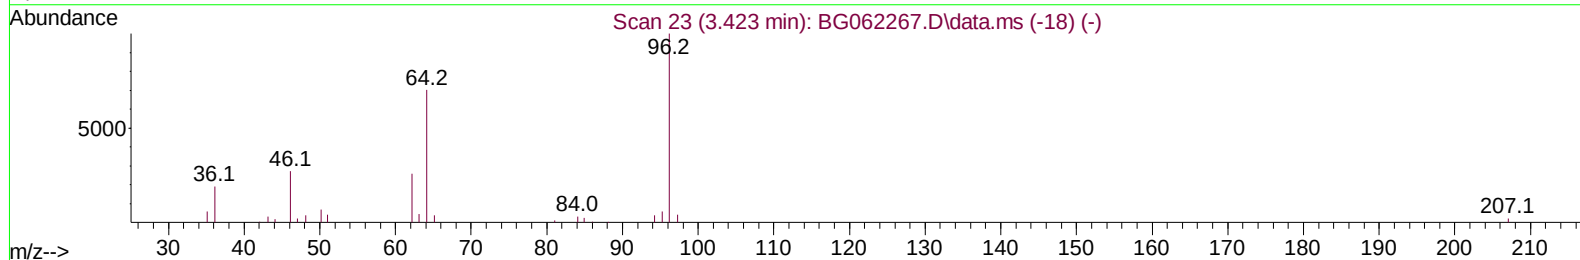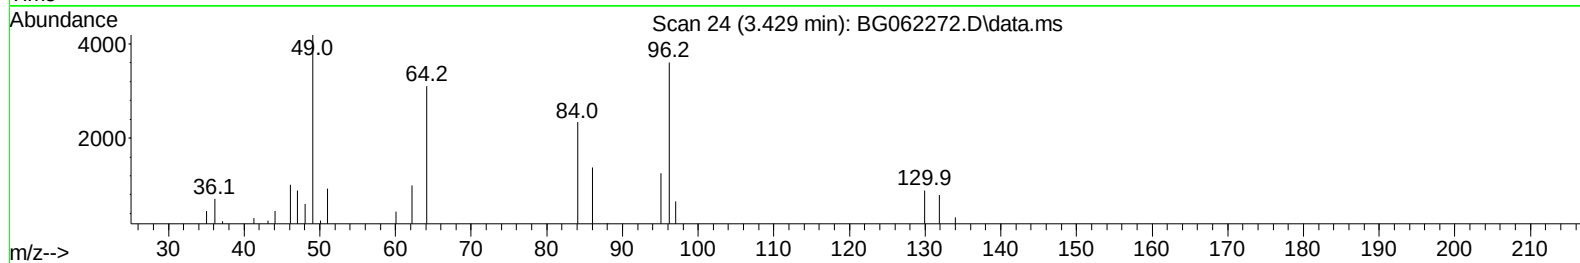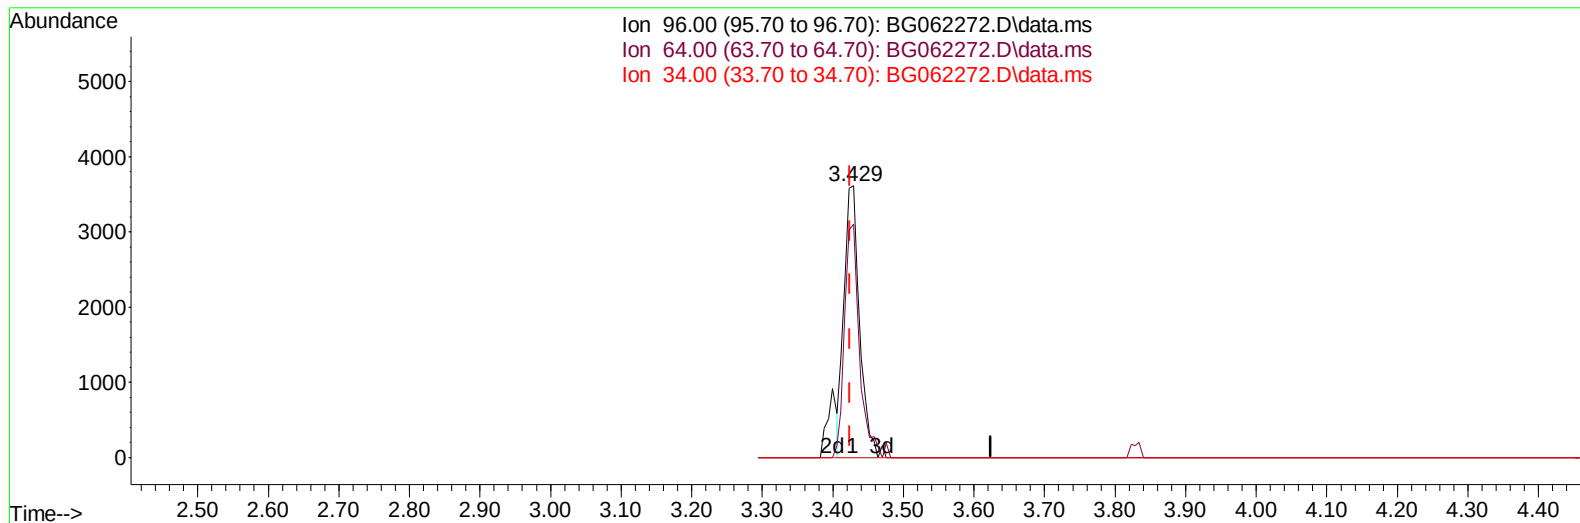

TIC: BG062272.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.429min (+ 0.005) 3.88 ng/uL

response 5593

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	86.01
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062272.D
Acq On : 6 Aug 2024 16:07
Operator : MA/JU
Sample : P3328-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1ZT4

Manual IntegrationsAPPROVED

Quant Time: Aug 06 16:40:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

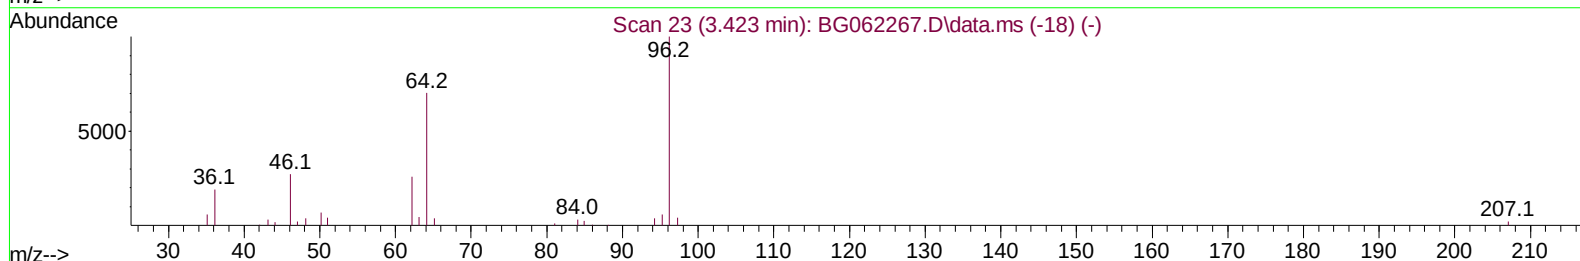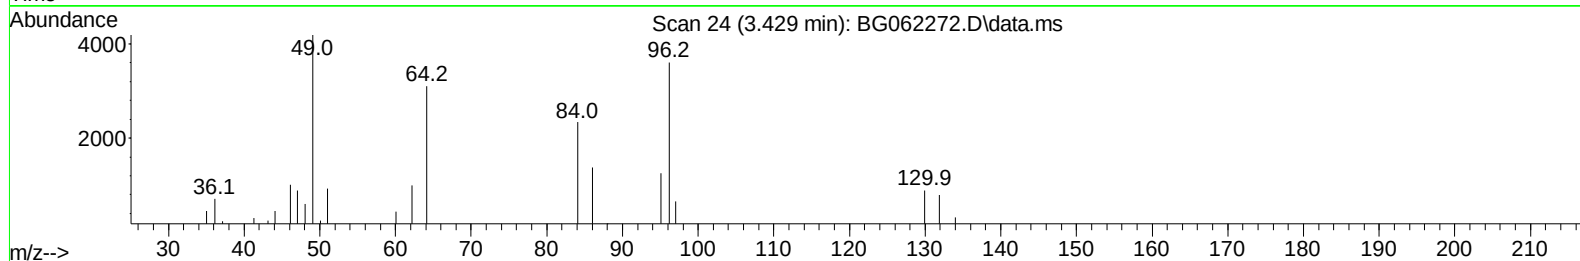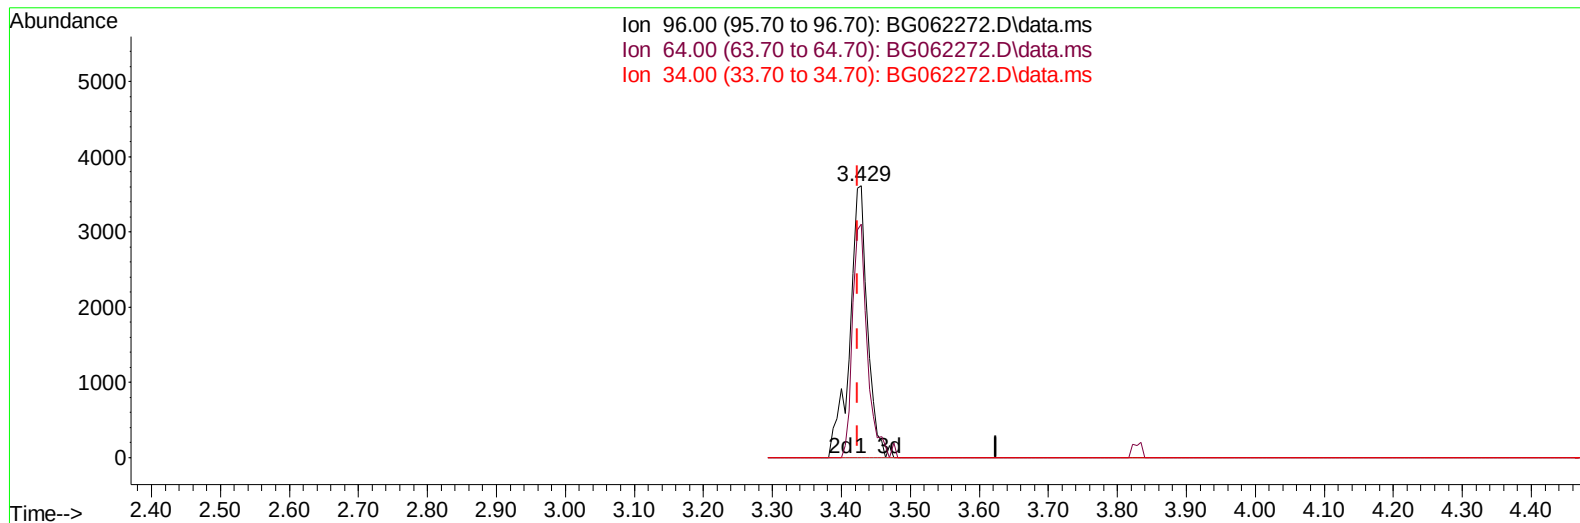

TIC: BG062272.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.429min (+ 0.005) 4.51 ng/uL m

response 6497

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	86.01
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062272.D
 Acq On : 6 Aug 2024 16:07
 Operator : MA/JU
 Sample : P3328-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1ZT4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 06 16:41:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.964	152	62098	20.000	ng/ul	0.00
20) Naphthalene-d8	10.760	136	290952	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.584	164	226618	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	490462	20.000	ng/ul	0.00
79) Chrysene-d12	21.563	240	482425	20.000	ng/ul	-0.01
88) Perylene-d12	24.659	264	562066	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.429	96	6497m	4.511	ng/uL	0.00
4) Pyridine-d5	3.828	84	77490	17.103	ng/ul	0.00
7) Phenol-d5	7.118	99	137228	23.153	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.294	67	81150	22.242	ng/ul	0.00
11) 2-Chlorophenol-d4	7.494	132	96768	22.787	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	114823	23.258	ng/ul	0.00
21) Nitrobenzene-d5	9.115	128	48095	26.808	ng/ul	0.00
24) 2-Nitrophenol-d4	9.838	143	53274	31.566	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.372	165	120002	24.481	ng/ul	0.00
31) 4-Chloroaniline-d4	10.884	131	167979	23.627	ng/ul	0.00
46) Dimethylphthalate-d6	13.991	166	419366	23.985	ng/ul	0.00
49) Acenaphthylene-d8	14.273	160	485397	24.485	ng/ul	0.00
54) 4-Nitrophenol-d4	14.755	143	53148	21.712	ng/ul	0.00
60) Fluorene-d10	15.571	176	375504	23.927	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.677	200	30501	20.999	ng/ul	0.00
73) Anthracene-d10	17.422	188	585614	24.755	ng/ul	0.00
81) Pyrene-d10	19.701	212	725694	25.308	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.453	264	753445	25.076	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062272.D
Acq On : 6 Aug 2024 16:07
Operator : MA/JU
Sample : P3328-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1ZT4

Manual IntegrationsAPPROVED

Quant Time: Aug 06 16:41:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
Supervised By :mohammad ahmed 08/08/2024

