




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062284.D
Acq On : 7 Aug 2024 1:08
Operator : MA/JU
Sample : P3336-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
F7E11

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/07/2024
Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 07 01:52:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 07 01:46:39 2024
Response via : Initial Calibration

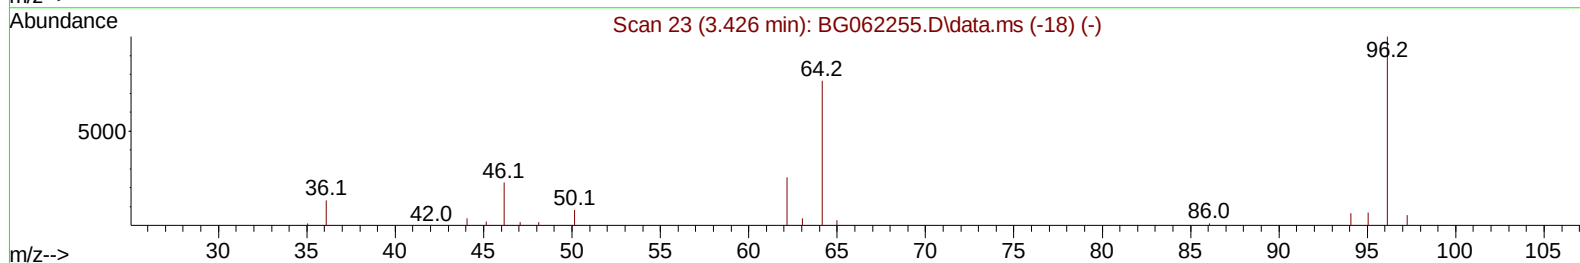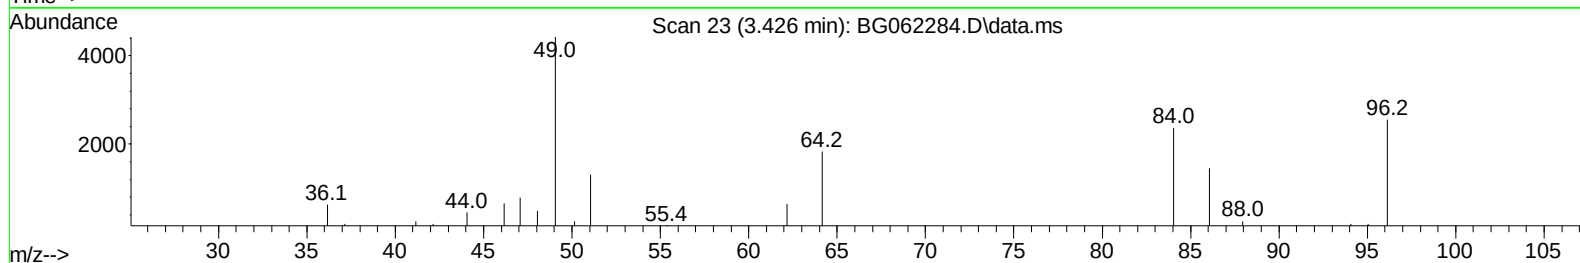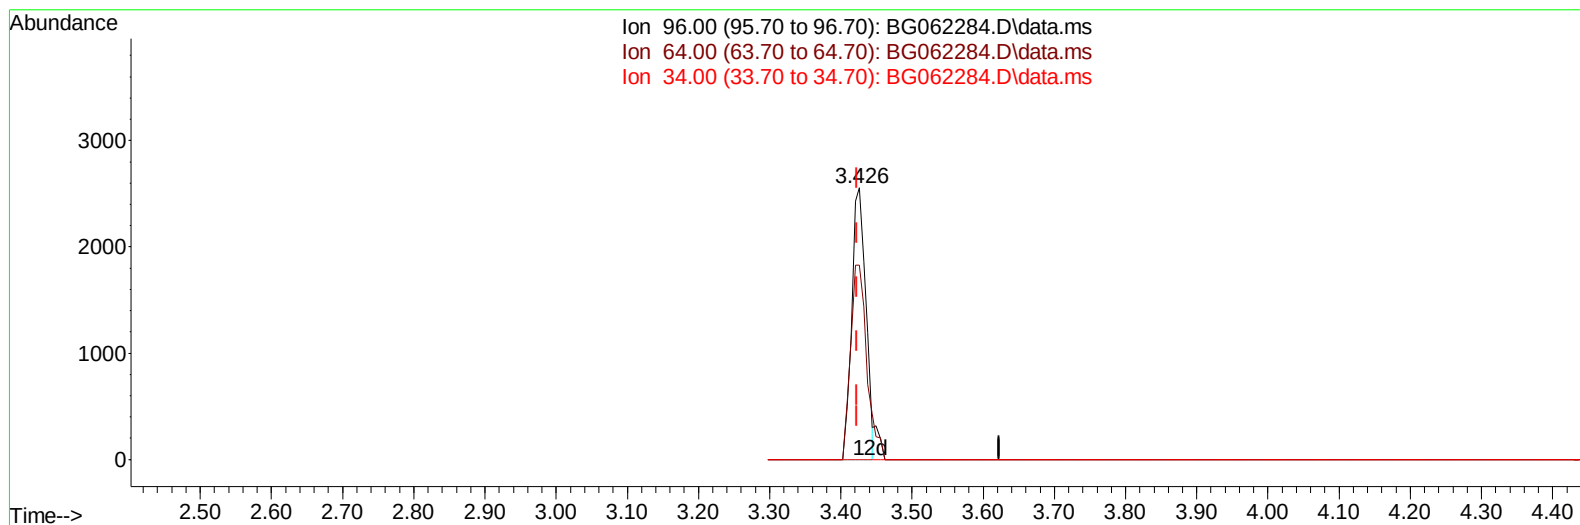

TIC: BG062284.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.426min (+ 0.003) 2.90 ng/uL

response 3514

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	71.50
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062284.D
Acq On : 7 Aug 2024 1:08
Operator : MA/JU
Sample : P3336-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
F7E11

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/07/2024
Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 07 01:52:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 07 01:46:39 2024
Response via : Initial Calibration

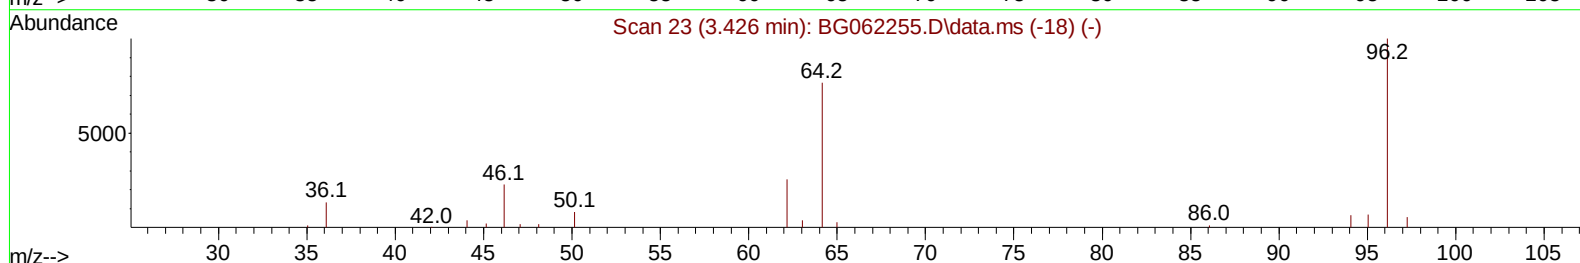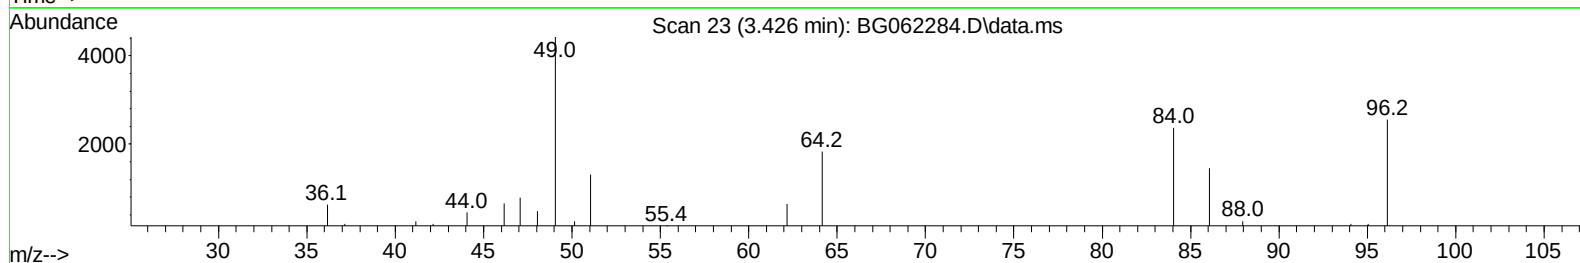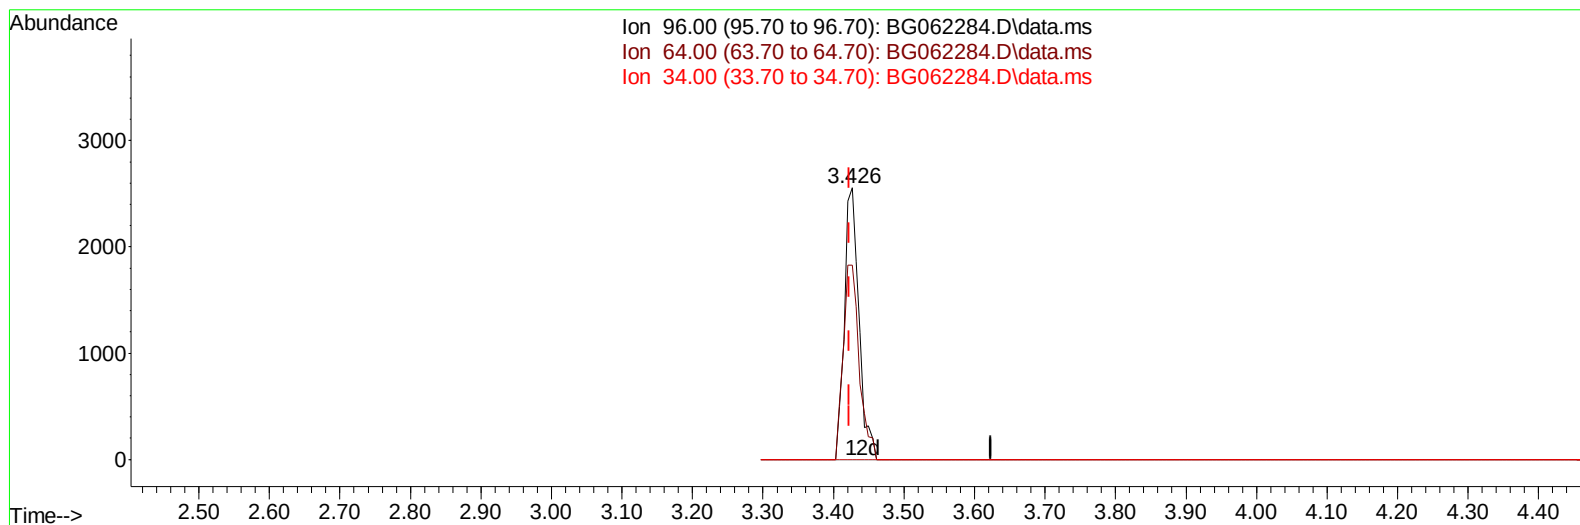

TIC: BG062284.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.426min (+ 0.003) 3.04 ng/uL m

response 3695

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	71.50
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062284.D
 Acq On : 7 Aug 2024 1:08
 Operator : MA/JU
 Sample : P3336-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F7E11

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/07/2024
 Supervised By :mohammad ahmed 08/08/2024

Quant Time: Aug 07 01:56:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 07 01:46:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.961	152	52329	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	247822	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.582	164	191667	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.319	188	416985	20.000	ng/ul	0.00
79) Chrysene-d12	21.560	240	417574	20.000	ng/ul	0.00
88) Perylene-d12	24.650	264	490316	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.426	96	3695m	3.045	ng/uL	0.00
4) Pyridine-d5	3.832	84	42411	11.108	ng/ul	0.00
7) Phenol-d5	7.115	99	96741	19.369	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.292	67	58300	18.962	ng/ul	0.00
11) 2-Chlorophenol-d4	7.491	132	69608	19.452	ng/ul	0.00
15) 4-Methylphenol-d8	8.654	113	84322	20.268	ng/ul	0.00
21) Nitrobenzene-d5	9.113	128	35321	23.114	ng/ul	0.00
24) 2-Nitrophenol-d4	9.835	143	39030	27.151	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.370	165	87246	20.896	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	120583	19.913	ng/ul	0.00
46) Dimethylphthalate-d6	13.988	166	339514	22.959	ng/ul	0.00
49) Acenaphthylene-d8	14.270	160	375744	22.410	ng/ul	0.00
54) 4-Nitrophenol-d4	14.752	143	45912	22.177	ng/ul	0.00
60) Fluorene-d10	15.569	176	305749	23.035	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200	27923	22.611	ng/ul	0.00
73) Anthracene-d10	17.419	188	483051	24.018	ng/ul	0.00
81) Pyrene-d10	19.698	212	614040	24.740	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.439	264	651323	24.849	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062284.D
Acq On : 7 Aug 2024 1:08
Operator : MA/JU
Sample : P3336-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
F7E11

Manual IntegrationsAPPROVED

Quant Time: Aug 07 01:56:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 07 01:46:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/07/2024
Supervised By :mohammad ahmed 08/08/2024

