

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062264.D
 Acq On : 6 Aug 2024 9:52
 Operator : MA/JU
 Sample : P3361-15
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E20P5

Quant Time: Aug 06 10:47:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 02:21:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.966	152	81053	20.000	ng/u1	0.00
20) Naphthalene-d8	10.762	136	383064	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.586	164	291088	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.324	188	614575	20.000	ng/u1	0.00
79) Chrysene-d12	21.565	240	580640	20.000	ng/u1	-0.01
88) Perylene-d12	24.667	264	677342	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.425	96	4913	2.614	ng/uL	0.00
4) Pyridine-d5	3.830	84	88728	15.004	ng/u1	0.00
7) Phenol-d5	7.114	99	154859	20.017	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.296	67	90672	19.040	ng/u1	0.00
11) 2-Chlorophenol-d4	7.496	132	110216	19.885	ng/u1	0.00
15) 4-Methylphenol-d8	8.659	113	135490	21.026	ng/u1	0.00
21) Nitrobenzene-d5	9.117	128	56171	23.781	ng/u1	0.00
24) 2-Nitrophenol-d4	9.840	143	59711	26.873	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.374	165	139934	21.683	ng/u1	0.00
31) 4-Chloroaniline-d4	10.885	131	183746	19.630	ng/u1	0.00
46) Dimethylphthalate-d6	13.993	166	470465	20.948	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	536633	21.074	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	64293	20.448	ng/u1	0.00
60) Fluorene-d10	15.573	176	426143	21.139	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.685	200	35747	19.640	ng/u1	0.00
73) Anthracene-d10	17.424	188	638431	21.538	ng/u1	0.00
81) Pyrene-d10	19.703	212	782767	22.681	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.455	264	809140	22.346	ng/u1	-0.01
Target Compounds						
47) Dimethylphthalate	14.040	163	26057	1.157	ng/u1#	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062264.D
Acq On : 6 Aug 2024 9:52
Operator : MA/JU
Sample : P3361-15
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E20P5

Quant Time: Aug 06 10:47:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 02:21:27 2024
Response via : Initial Calibration

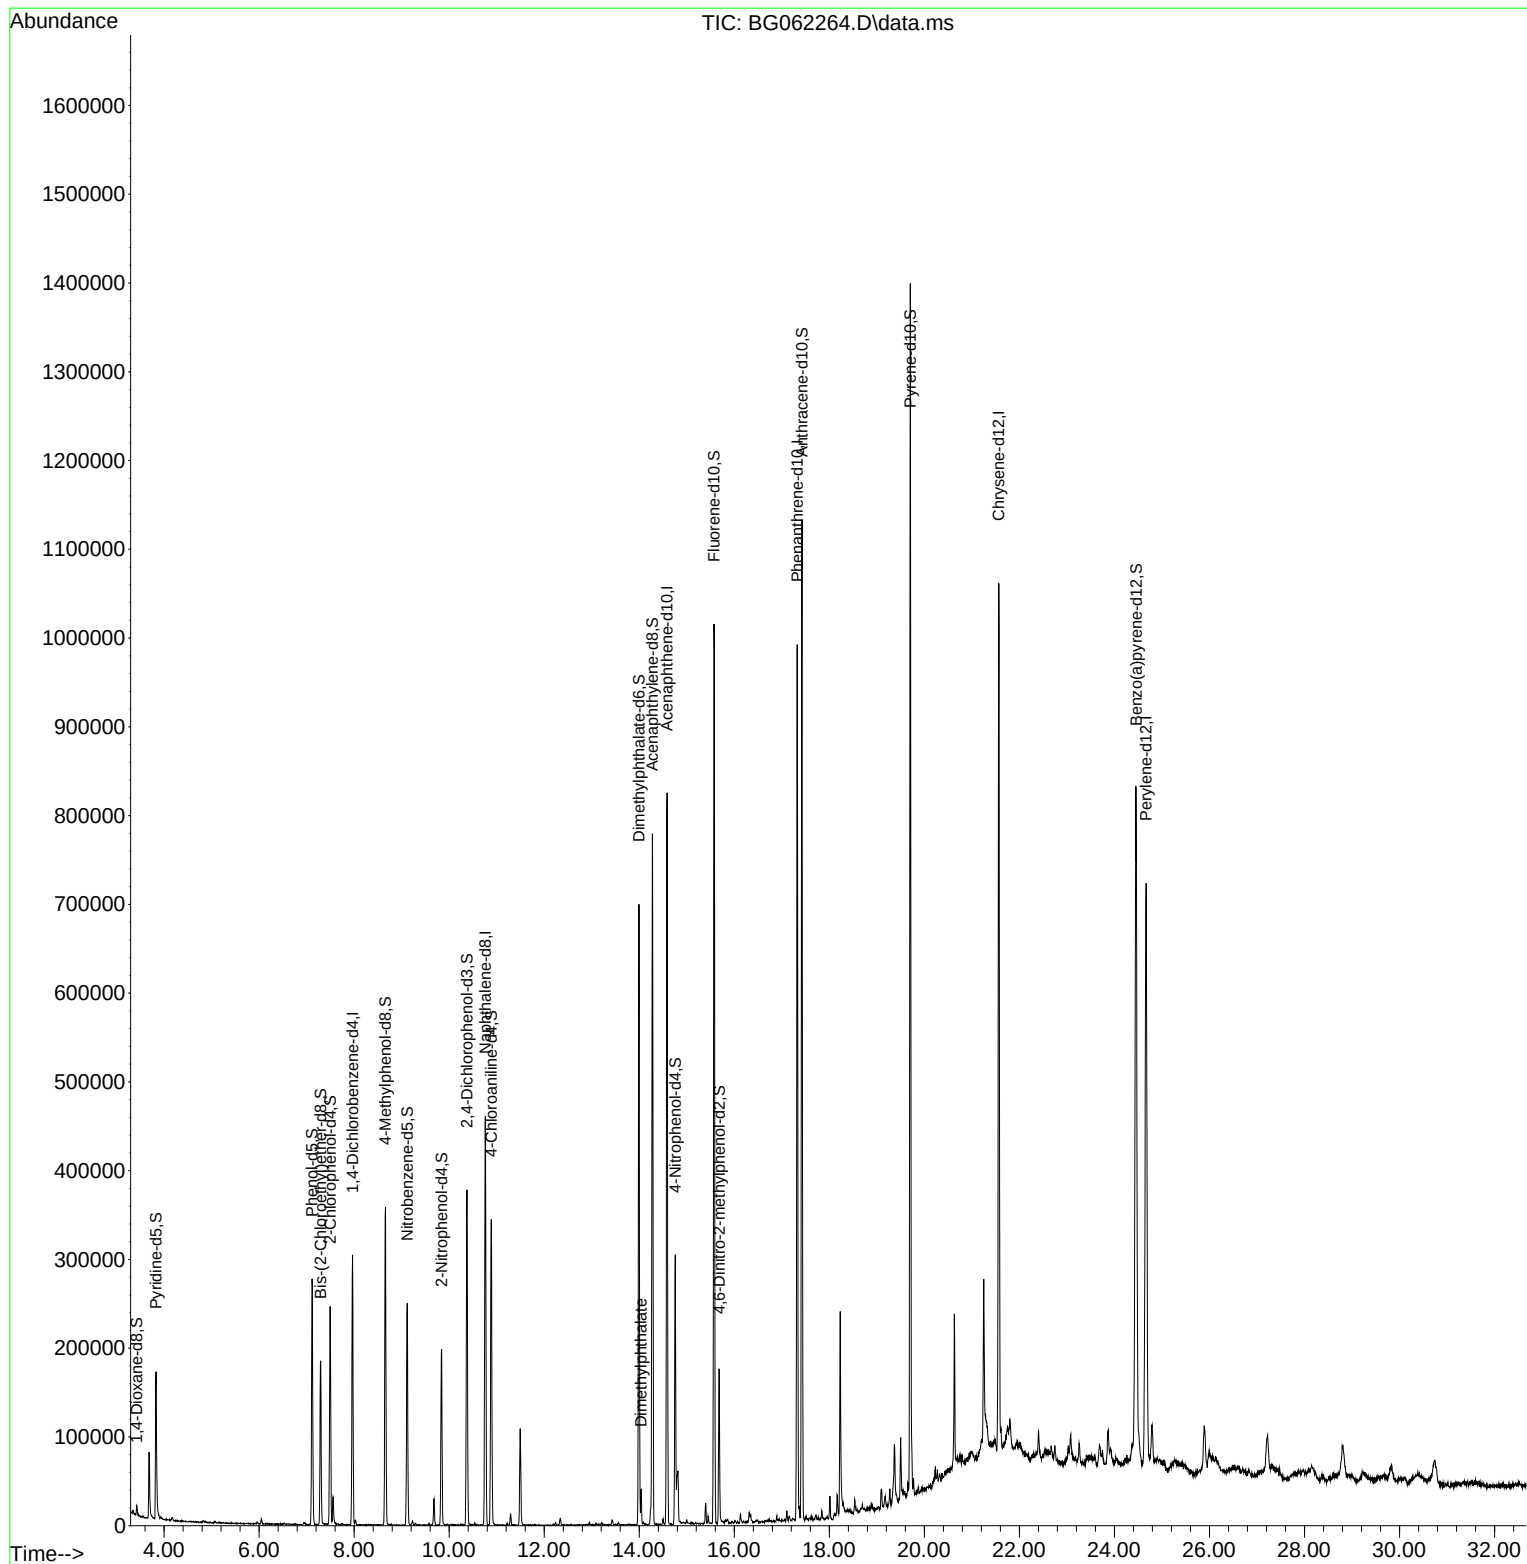

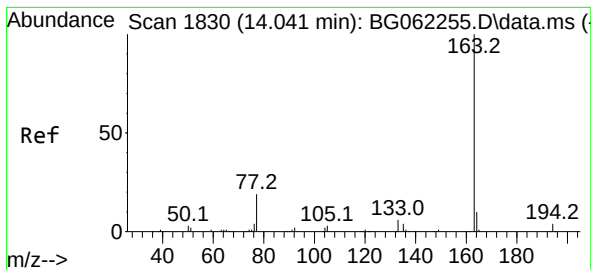

#47

Dimethylphthalate

Concen: 1.157 ng/ul

RT: 14.040 min Scan# 11

Delta R.T. -0.005 min

Lab File: BG062264.D


Acq: 6 Aug 2024 9:52

Instrument :

BNA_G

ClientSampleId :

E20P5

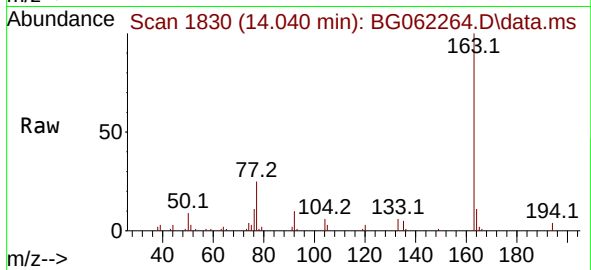

Tgt Ion:163 Resp: 26057

Ion Ratio Lower Upper

163 100

194 4.1 2.7 4.1#

164 11.1 8.1 12.1

