

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
 Data File : BG062256.D
 Acq On : 6 Aug 2024 4:21
 Operator : MA/JU
 Sample : PB162406BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK406

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	19	23	34	rVB	29217	45741	0.96%	0.093%
2	3.828	87	92	109	rBV	425174	715176	14.94%	1.460%
3	4.174	147	151	159	rVB4	6945	11079	0.23%	0.023%
4	4.386	183	187	192	rBV2	7240	9948	0.21%	0.020%
5	4.791	252	256	260	rVB5	2956	5078	0.11%	0.010%
6	7.117	644	652	662	rBV	639964	1072000	22.39%	2.189%
7	7.293	674	682	692	rBV	474713	776628	16.22%	1.586%
8	7.493	708	716	726	rBV	574639	963877	20.14%	1.968%
9	7.963	789	796	805	rBV	525132	883006	18.45%	1.803%
10	8.656	907	914	923	rBV	761684	1305102	27.26%	2.664%
11	9.115	983	992	1001	rBV	580524	1040758	21.74%	2.125%
12	9.837	1107	1115	1126	rBV	498337	850256	17.76%	1.736%
13	10.060	1149	1153	1159	rBV4	2699	4833	0.10%	0.010%
14	10.372	1195	1206	1218	rBV	808681	1406633	29.39%	2.872%
15	10.759	1264	1272	1285	rVB	862088	1511323	31.57%	3.086%
16	10.889	1285	1294	1304	rBV	830553	1510983	31.57%	3.085%
17	11.535	1401	1404	1410	rBV4	2919	6247	0.13%	0.013%
18	12.340	1533	1541	1548	rVB2	13842	23920	0.50%	0.049%
19	13.996	1815	1823	1829	rBV	1584834	2236879	46.73%	4.567%
20	14.278	1863	1871	1881	rBV2	1748718	2773550	57.94%	5.662%
21	14.584	1915	1923	1931	rVB	1547798	2422796	50.61%	4.946%
22	14.760	1945	1953	1967	rBV	742382	1186190	24.78%	2.422%
23	15.576	2084	2092	2103	rBV	2285723	3481331	72.73%	7.107%
24	15.682	2103	2110	2124	rBV	533982	786799	16.44%	1.606%
25	15.811	2129	2132	2138	rVB2	9549	13954	0.29%	0.028%
26	16.358	2221	2225	2229	rBV2	8166	9533	0.20%	0.019%
27	16.869	2309	2312	2316	rVB2	4231	5371	0.11%	0.011%
28	17.110	2348	2353	2359	rVB2	4256	6426	0.13%	0.013%
29	17.204	2365	2369	2376	rBV3	3102	5504	0.11%	0.011%
30	17.327	2382	2390	2397	rBV	1832960	2894133	60.46%	5.909%
31	17.421	2399	2406	2419	rVB2	2259902	3446881	72.01%	7.037%
32	17.615	2433	2439	2444	rVB5	2999	5108	0.11%	0.010%
33	17.668	2444	2448	2451	rBV4	2870	4846	0.10%	0.010%
34	18.537	2592	2596	2602	rBV3	18927	34546	0.72%	0.071%
35	18.690	2618	2622	2628	rVB3	13515	16783	0.35%	0.034%
36	19.101	2686	2692	2701	rVB	107285	161205	3.37%	0.329%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062256.D
Acq On : 6 Aug 2024 4:21
Operator : MA/JU
Sample : PB162406BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK406

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Title : SVOA CALIBRATION

37	19.271	2716	2721	2726	rBV2	34401	50874	1.06%	0.104%
38	19.336	2726	2732	2737	rBV	34898	53787	1.12%	0.110%
39	19.418	2743	2746	2751	rVB5	3928	5052	0.11%	0.010%
40	19.653	2782	2786	2788	rBV	12703	14602	0.31%	0.030%
41	19.706	2788	2795	2805	rVB	2992813	4363438	91.15%	8.908%
42	20.699	2960	2964	2968	rVB3	13821	15414	0.32%	0.031%
43	20.899	2994	2998	3001	rBV4	3848	5090	0.11%	0.010%
44	21.568	3104	3112	3125	rBV2	1981561	3169307	66.21%	6.470%
45	21.809	3149	3153	3160	rVB4	8043	13756	0.29%	0.028%
46	22.402	3250	3254	3260	rBV5	14877	20562	0.43%	0.042%
47	23.084	3364	3370	3377	rVB2	35984	63601	1.33%	0.130%
48	23.865	3497	3503	3512	rVV	56891	122311	2.56%	0.250%
49	24.464	3591	3605	3623	rBV2	1728826	4786874	100.00%	9.773%
50	24.670	3627	3640	3654	rVV	1294731	3539240	73.94%	7.226%
51	24.793	3654	3661	3671	rVB2	83213	209780	4.38%	0.428%
52	25.898	3839	3849	3860	rBV2	78543	234448	4.90%	0.479%
53	26.097	3879	3883	3884	rBV3	5126	6674	0.14%	0.014%
54	27.219	4064	4074	4087	rBV3	72319	256578	5.36%	0.524%
55	28.817	4335	4346	4363	rVB4	50877	222159	4.64%	0.454%
56	30.756	4661	4676	4693	rVB6	38624	193196	4.04%	0.394%




Sum of corrected areas: 48981166

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062256.D
Acq On : 6 Aug 2024 4:21
Operator : MA/JU
Sample : PB162406BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK406

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

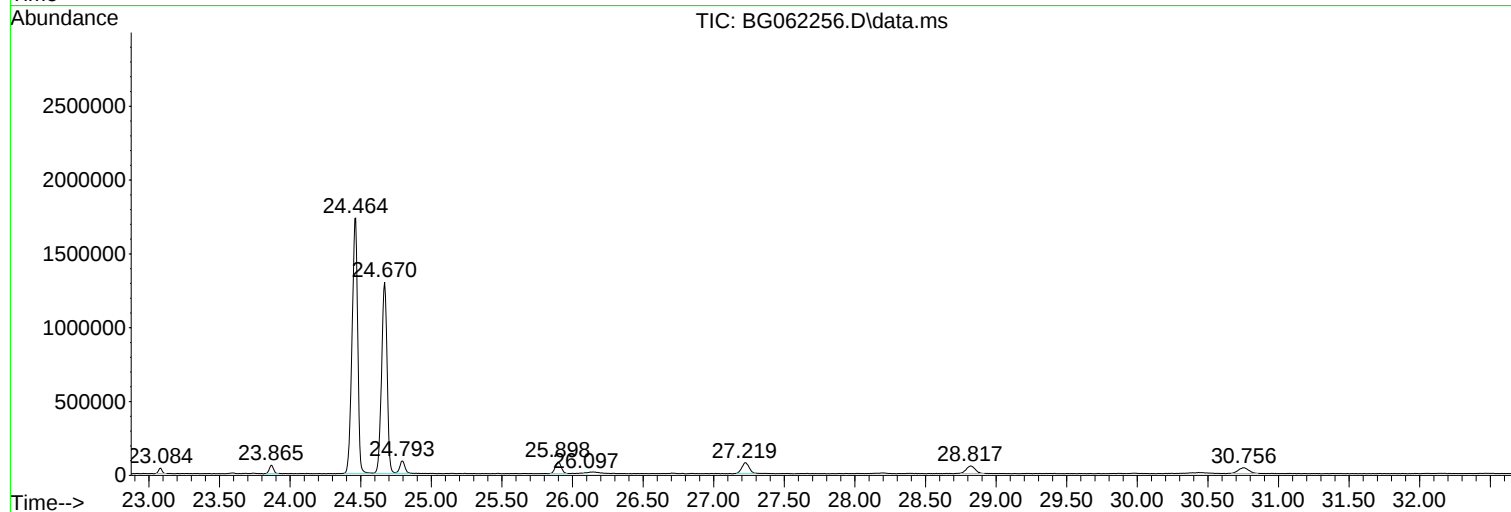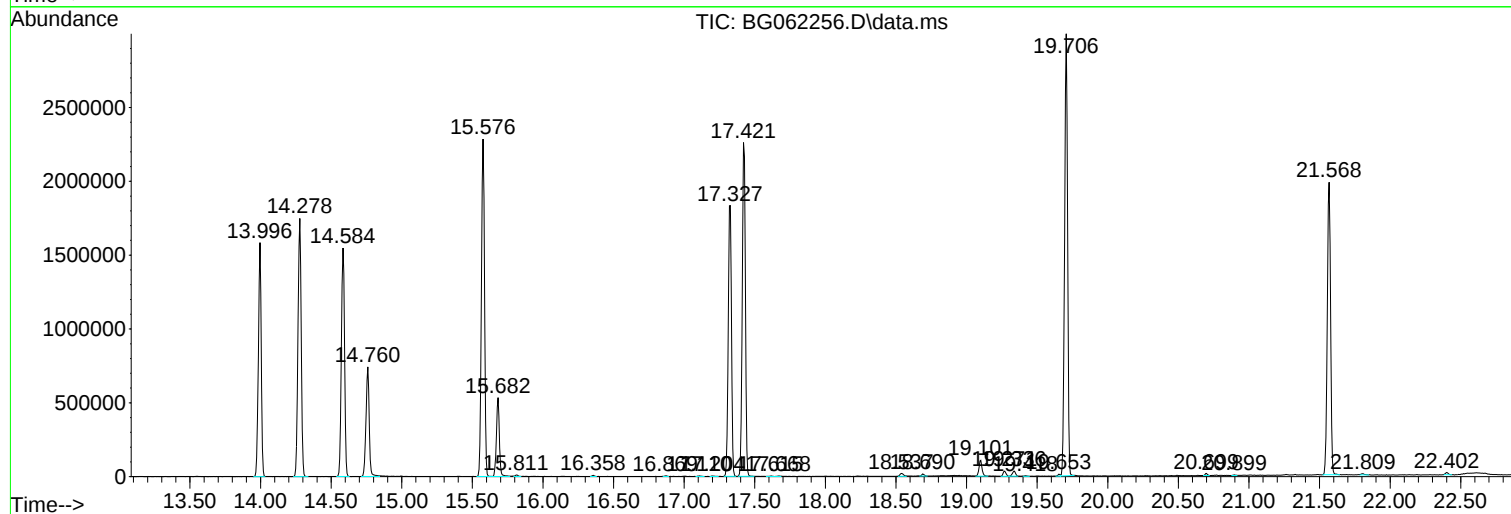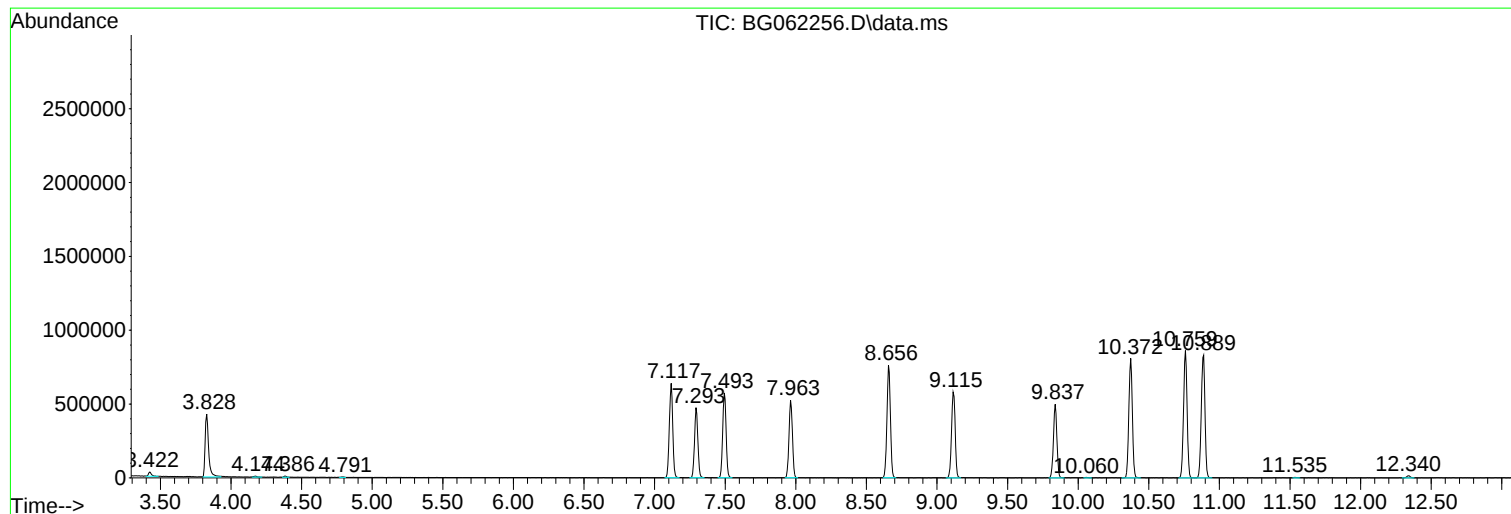

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062256.D
Acq On : 6 Aug 2024 4:21
Operator : MA/JU
Sample : PB162406BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK406

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080524\
Data File : BG062256.D
Acq On : 6 Aug 2024 4:21
Operator : MA/JU
Sample : PB162406BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK406

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc