
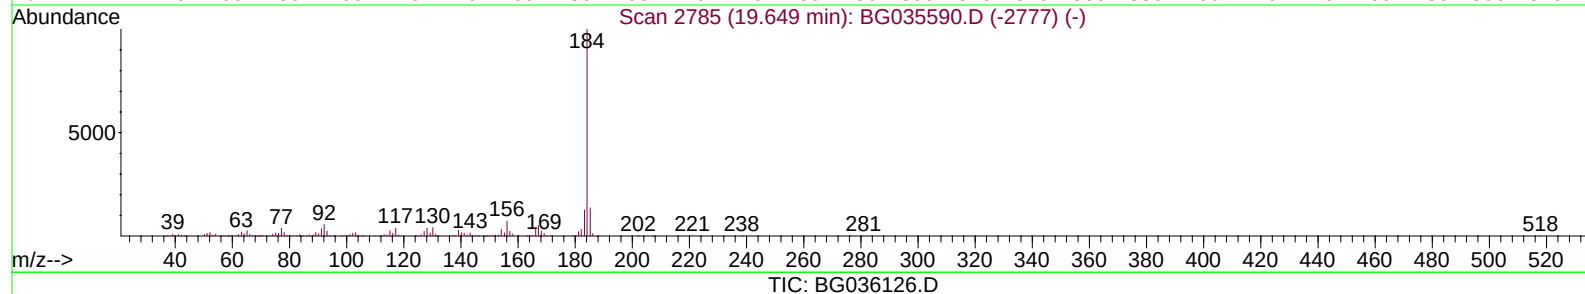
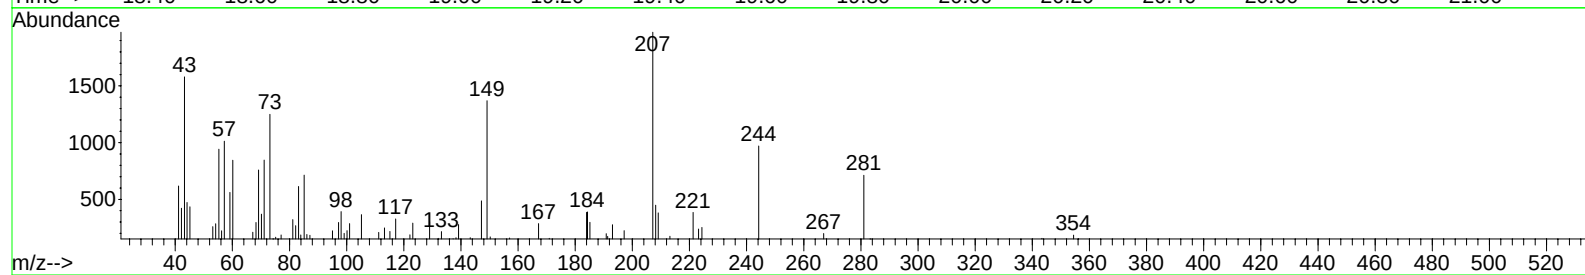


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080618\
Data File : BG036126.D
Acq On : 6 Aug 2018 14:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 19:19:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

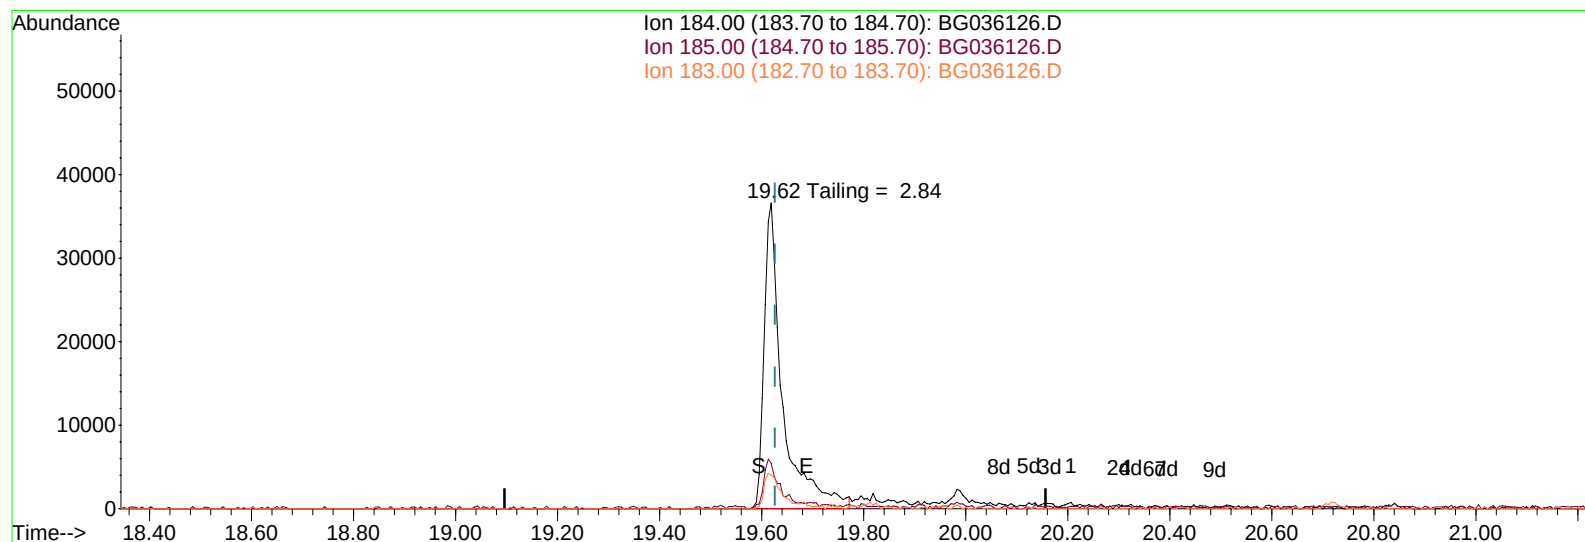

(76) Benzidine




20.206min (+0.580) 79.10ng

response 601

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	38.50#
183.00	13.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080618\
Data File : BG036126.D
Acq On : 6 Aug 2018 14:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 19:19:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

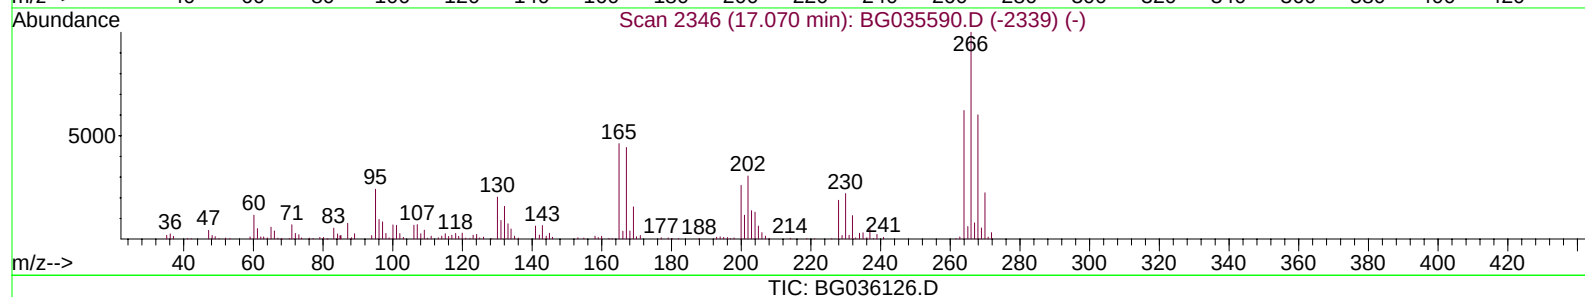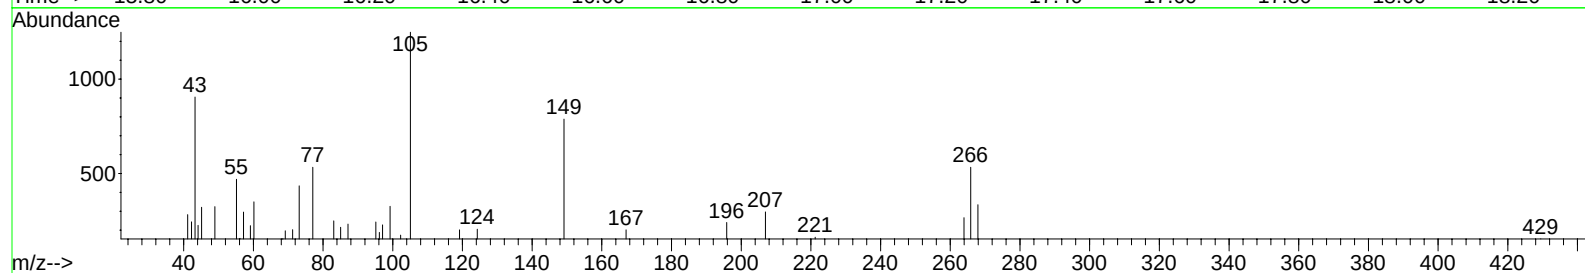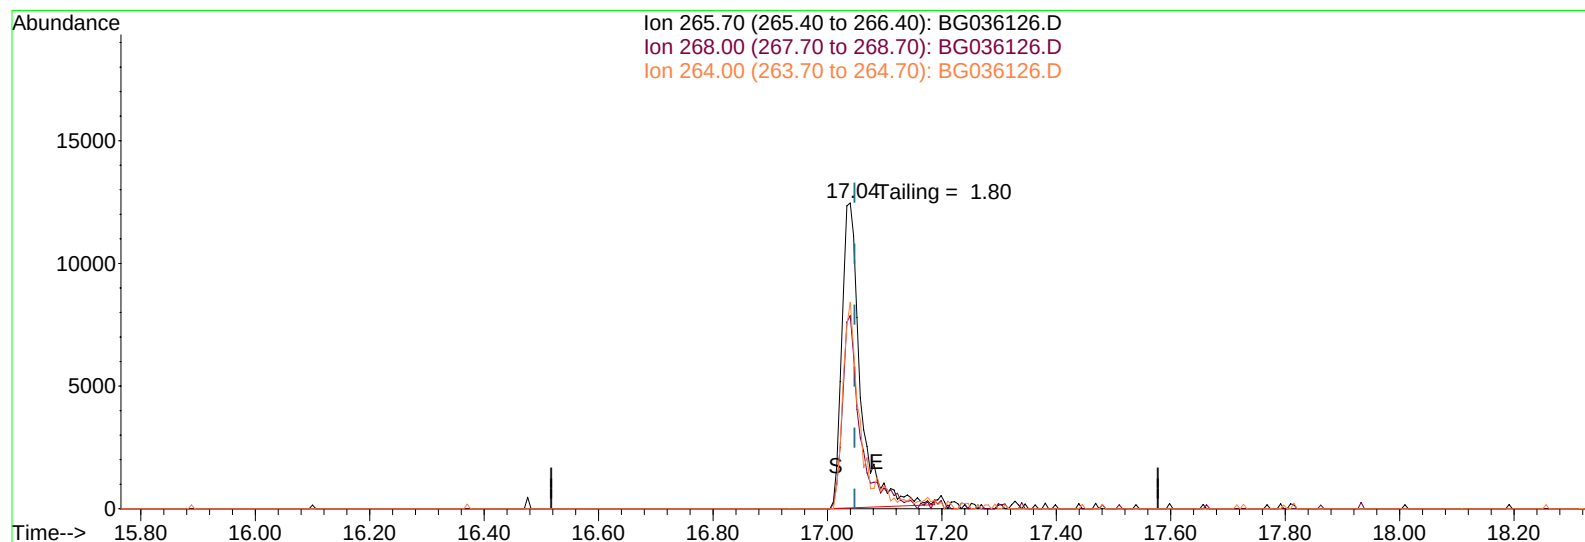

TIC: BG036126.D

(69) Pentachlorophenol (C)

17.198min (+0.151) 1248.39ng

response 536

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.66
264.00	62.00	49.91
0.00	0.00	0.00