
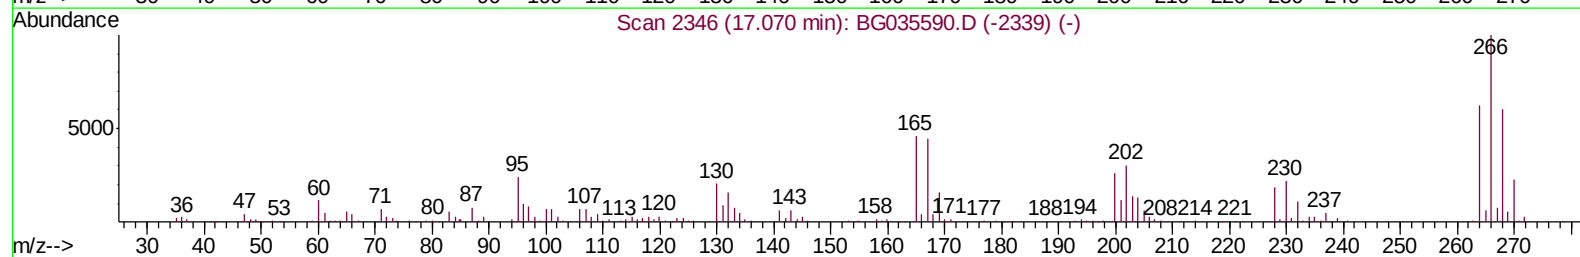
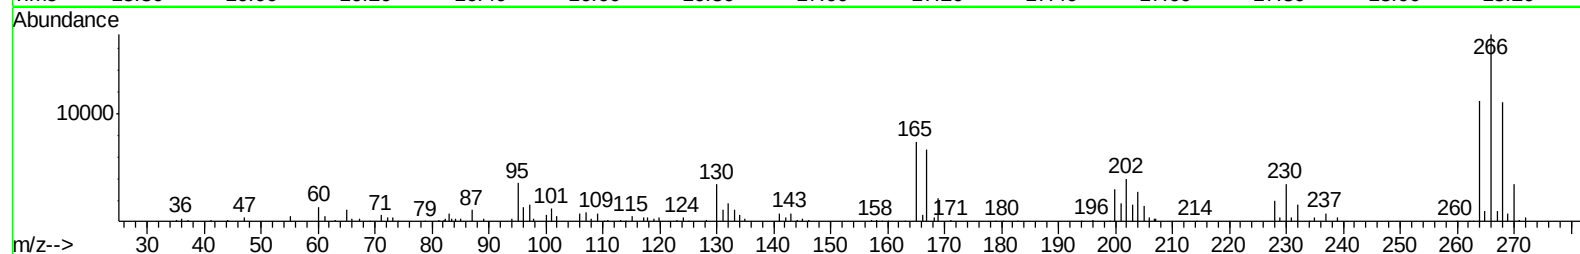


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG080618\
Data File : BG036145.D
Acq On : 7 Aug 2018 3:17
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 06:52:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

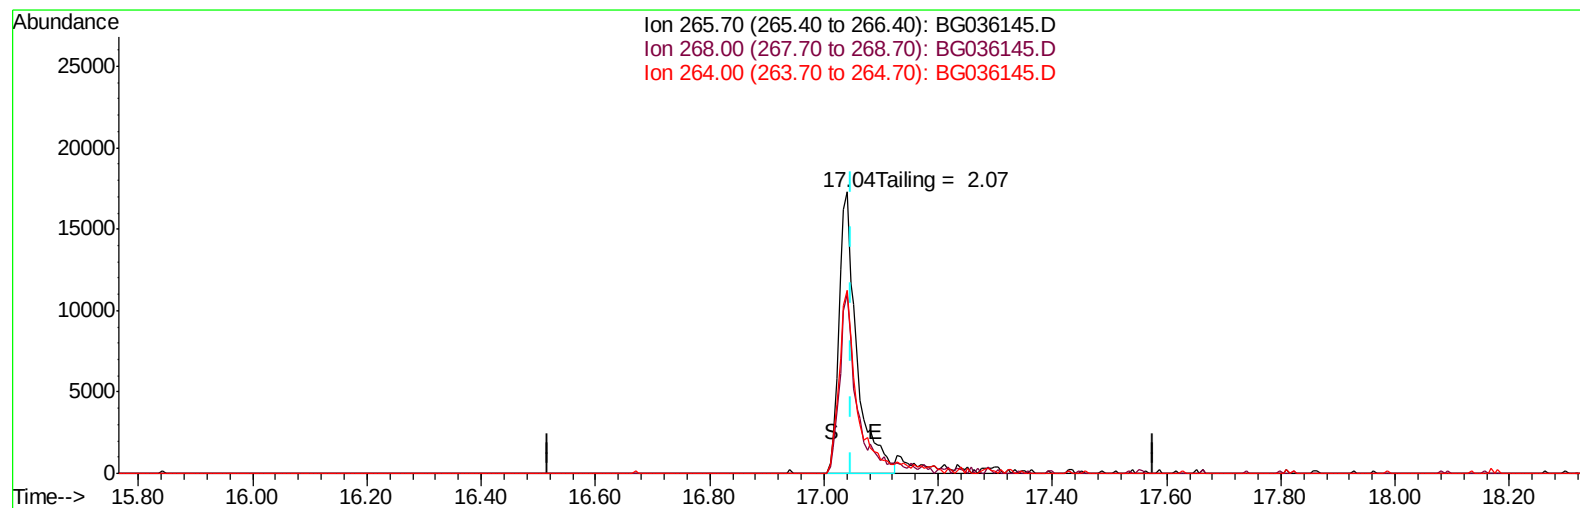

TIC: BG036145.D

(69) Pentachlorophenol (C)




17.040min (-0.007) 65757.91ng

response 36847

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.86
264.00	62.00	64.89
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG080618\
Data File : BG036145.D
Acq On : 7 Aug 2018 3:17
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 06:52:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

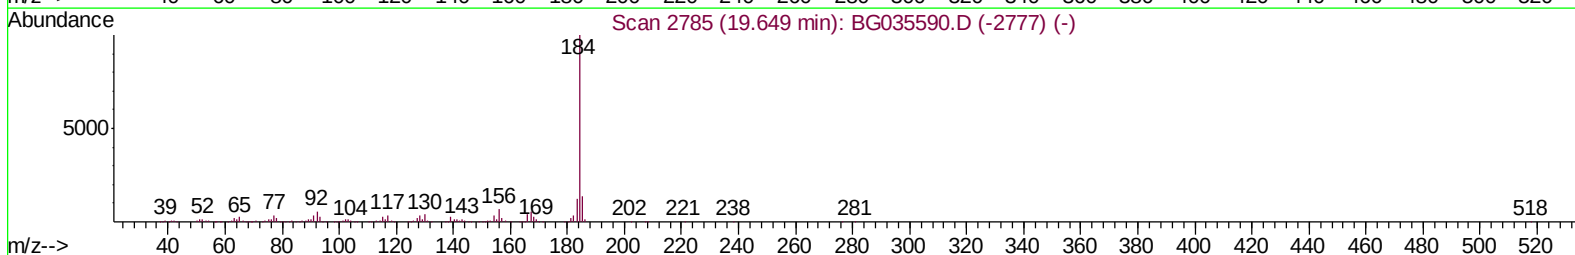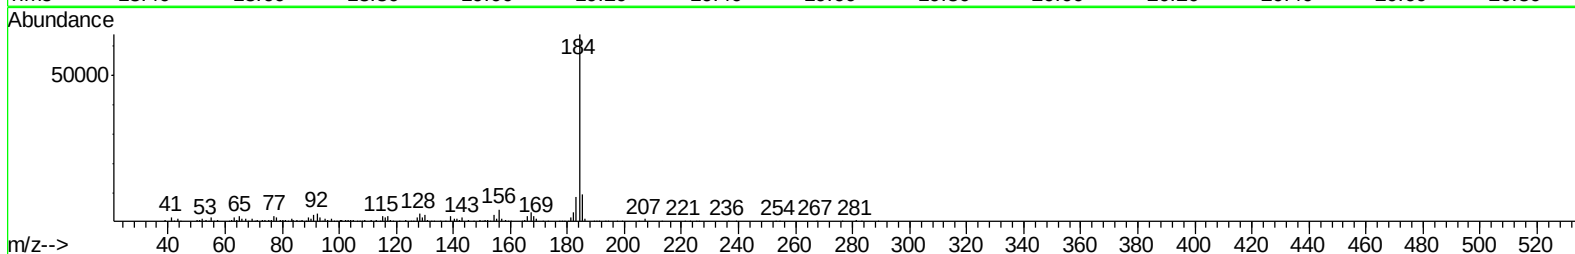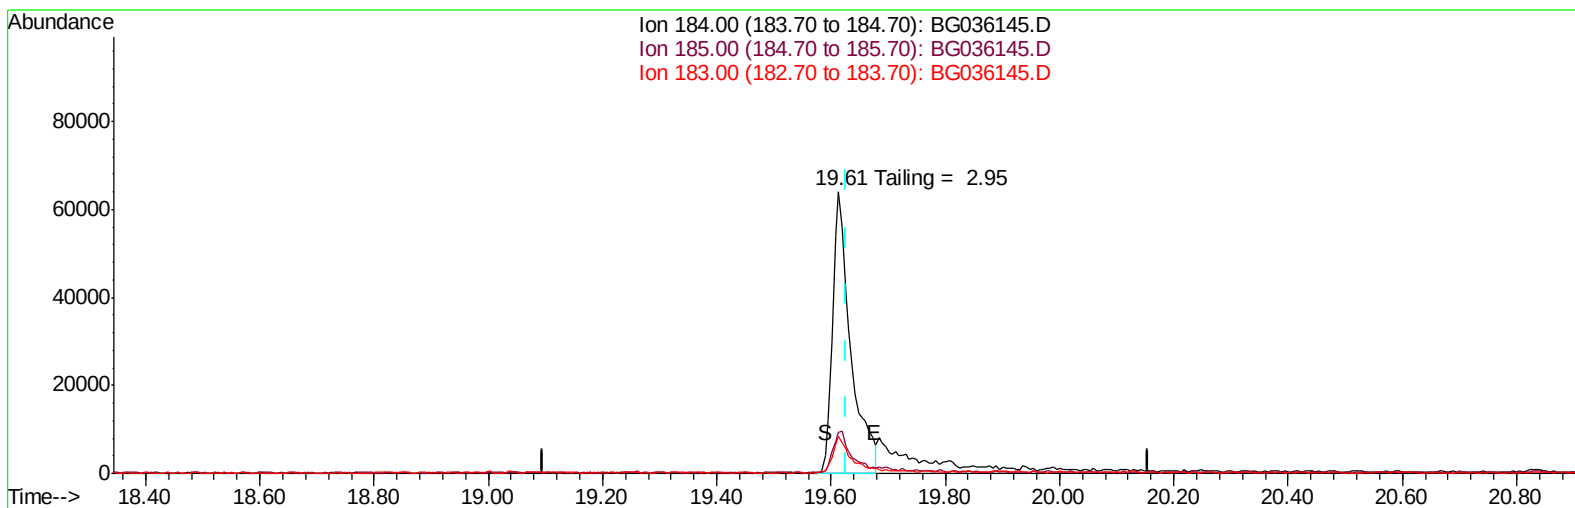

TIC: BG036145.D

(76) Benzidine

19.613min (-0.013) 77454.17ng

response 140504

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.78
183.00	13.30	13.02
0.00	0.00	0.00