

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080618\
 Data File : BG036139.D
 Acq On : 6 Aug 2018 22:42
 Operator : JU/SJ
 Sample : J4316-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 T40-CLAY-1

Quant Time: Aug 07 01:29:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 31 12:30:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	27250	20.00	ng	-0.02
21) Naphthalene-d8	10.82	136	93250	20.00	ng	-0.02
38) Acenaphthene-d10	14.63	164	63608	20.00	ng	-0.02
63) Phenanthrene-d10	17.38	188	201206	20.00	ng	-0.02
75) Chrysene-d12	21.64	240	221152	20.00	ng	-0.02
86) Perylene-d12	24.83	264	201291	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	219904	133.98	ng	-0.01
7) Phenol-d6	7.18	99	278345	113.66	ng	-0.02
23) Nitrobenzene-d5	9.17	82	232280	104.06	ng	-0.02
41) 2,4,6-Tribromophenol	16.13	330	175214	208.99	ng	-0.02
44) 2-Fluorobiphenyl	13.25	172	515734	108.63	ng	-0.02
78) Terphenyl-d14	19.99	244	1209518	120.56	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080618\
Data File : BG036139.D
Acq On : 6 Aug 2018 22:42
Operator : JU/SJ
Sample : J4316-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
T40-CLAY-1

Quant Time: Aug 07 01:29:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

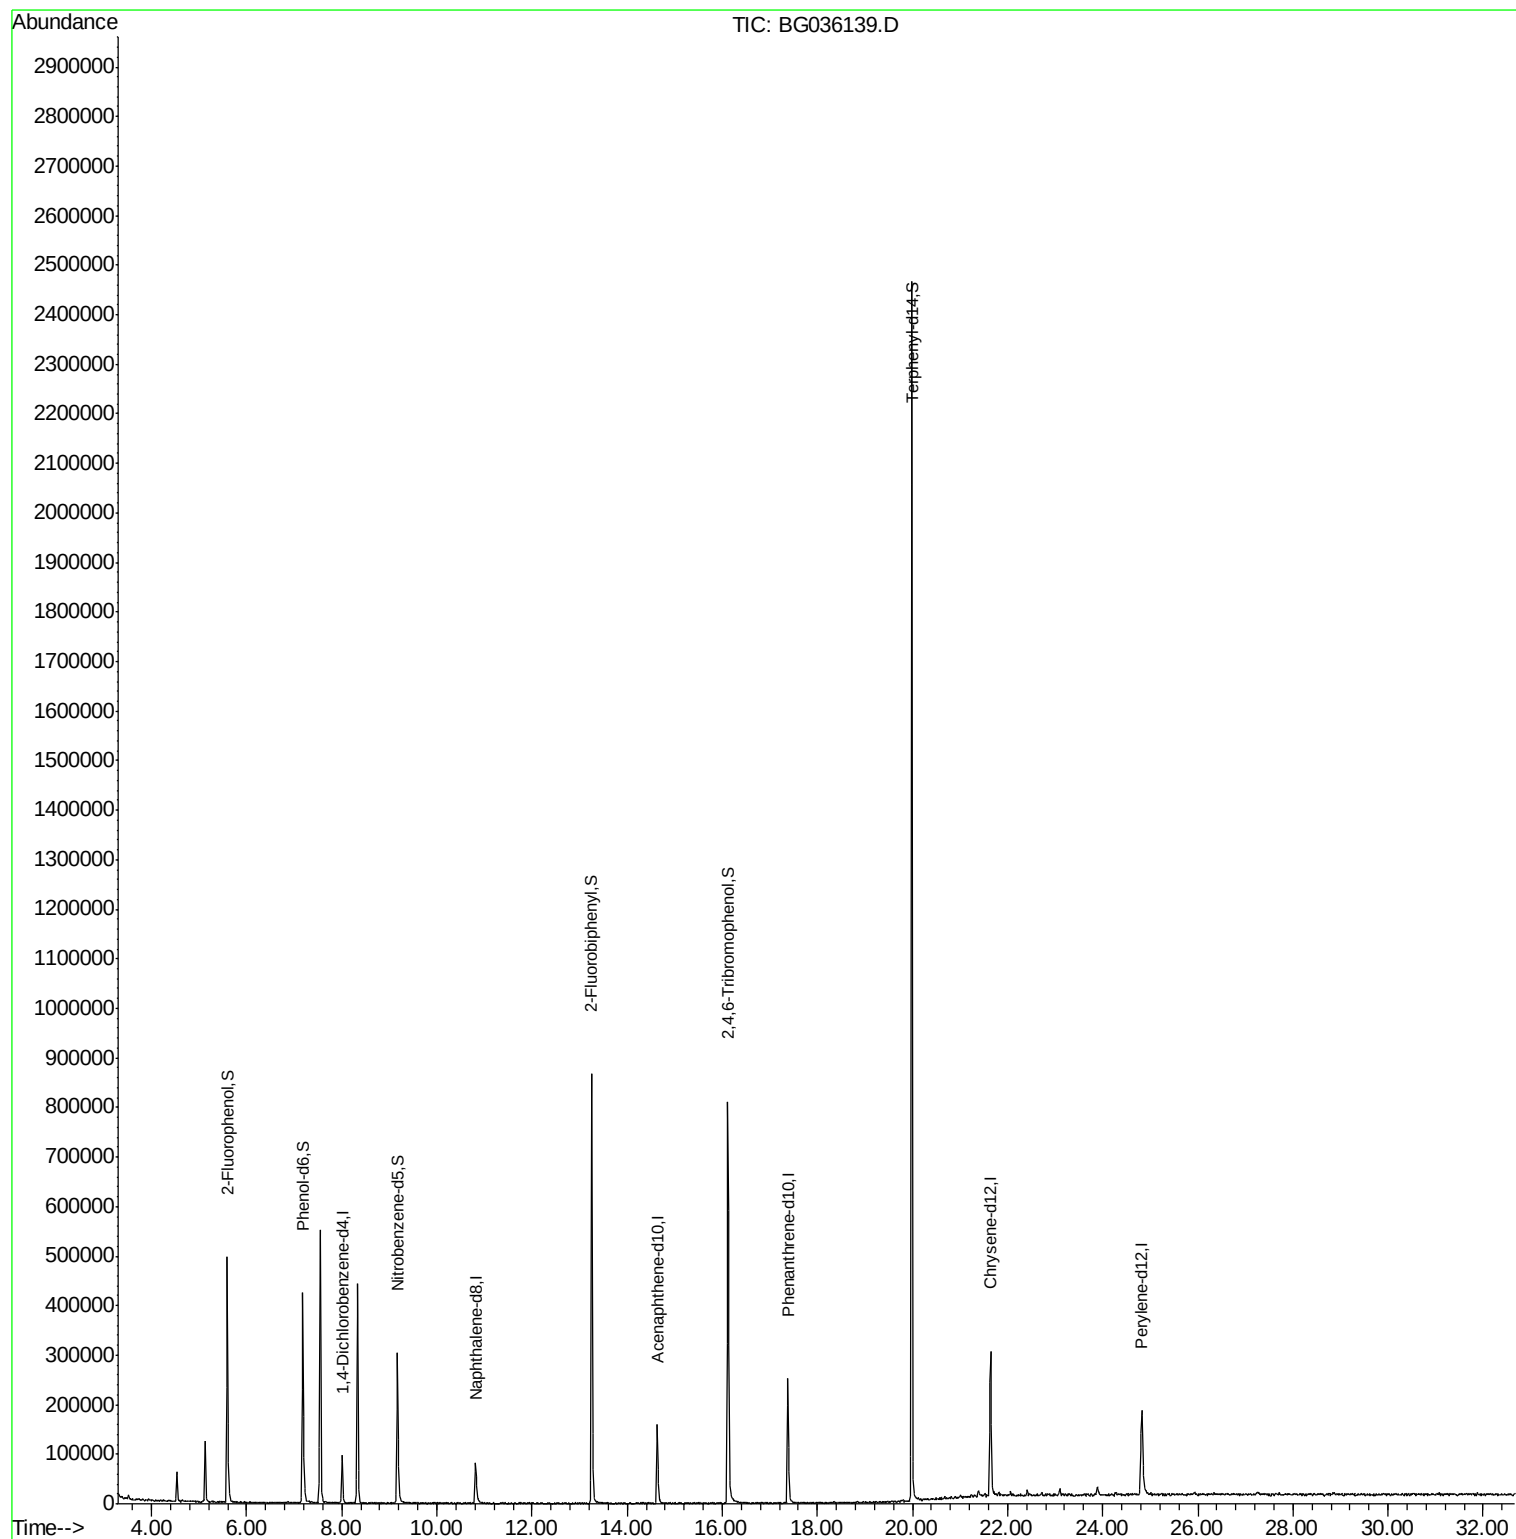

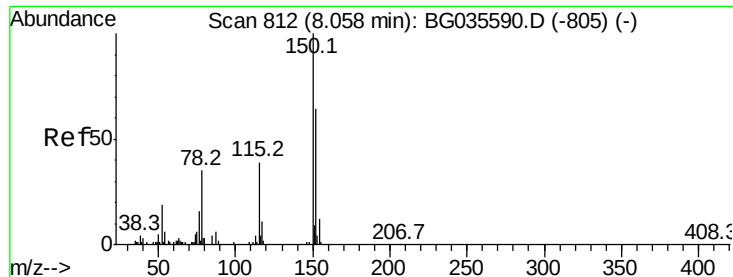


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 803
Delta R.T. -0.02 min
Lab File: BG036139.D
Acq: 6 Aug 2018 22:42

Instrument :
BNA_G
ClientSampleId :
T40-CLAY-1

Tot Ion:152 Resp: 27250
Ion Ratio Lower Upper
152 100
150 154.7 126.6 189.8
115 63.1 53.0 79.4

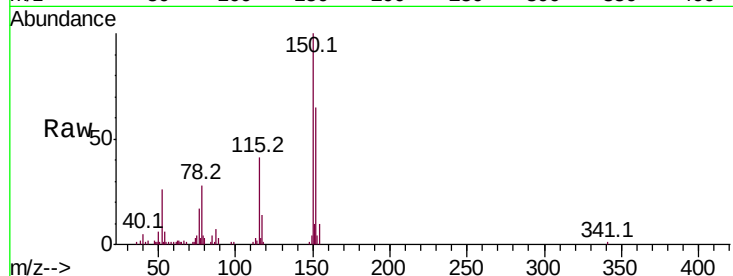


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

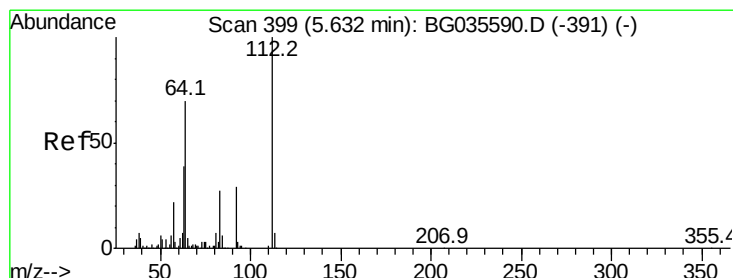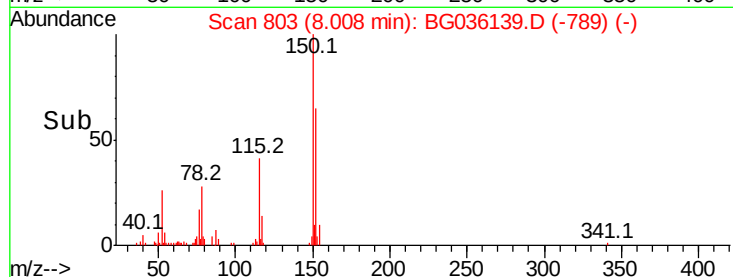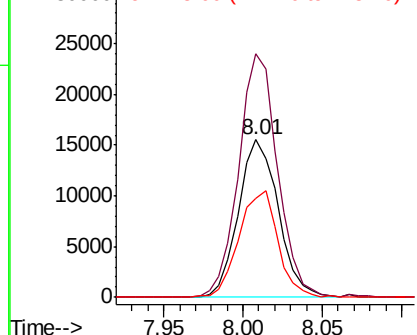



#5


2-Fluorophenol
Concen: 133.979 ng
RT: 5.59 min Scan# 392
Delta R.T. -0.01 min
Lab File: BG036139.D
Acq: 6 Aug 2018 22:42

Tgt Ion:112 Resp: 219904
Ion Ratio Lower Upper
112 100
64 61.0 56.3 84.5
63 35.5 30.1 45.1

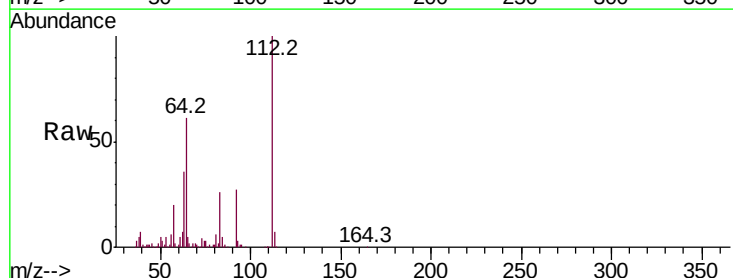

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

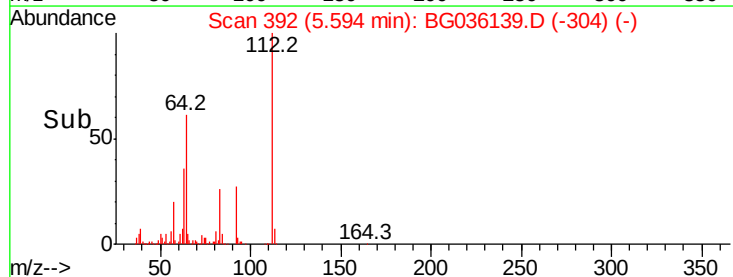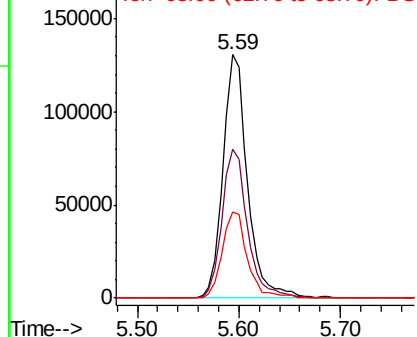

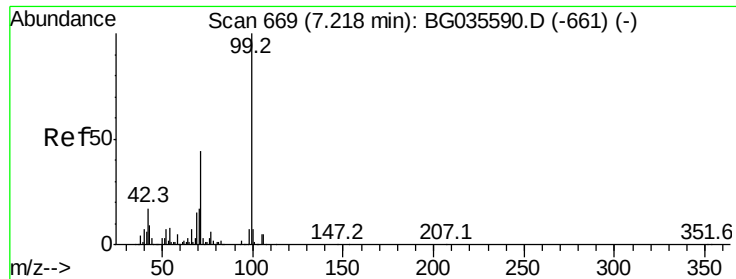

#7

Phenol-d6

Concen: 113.664 ng

RT: 7.18 min Scan# 662

Delta R.T. -0.02 min

Lab File: BG036139.D

Acq: 6 Aug 2018 22:42

Instrument :

BNA_G

ClientSampleId :

T40-CLAY-1


Tot Ion: 99 Resp: 278345

Ion Ratio Lower Upper

99 100

42 15.3 14.1 21.1




71 45.3 26.1 39.1#

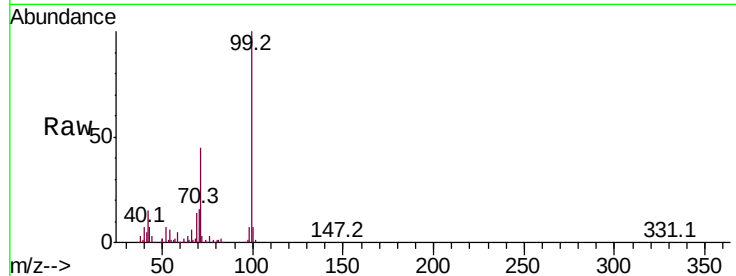

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

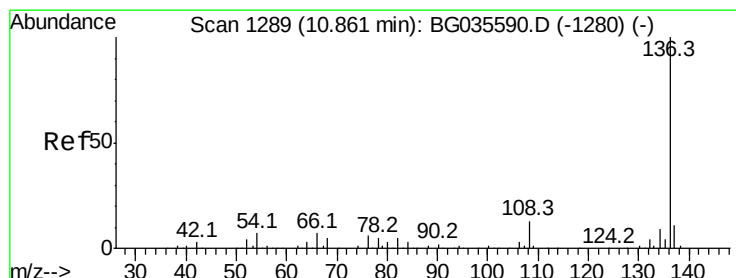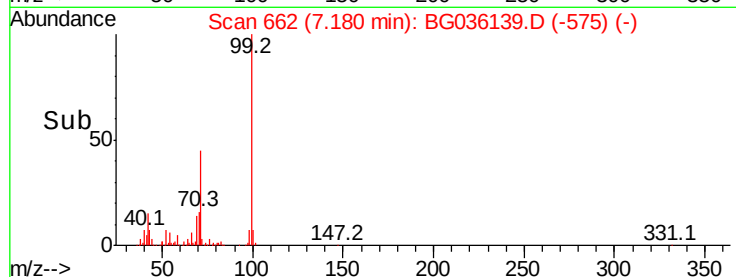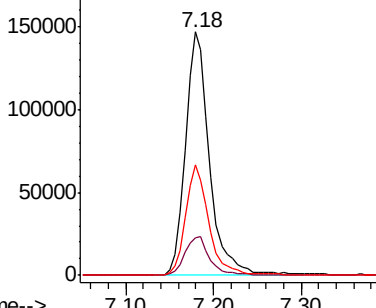

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.82 min Scan# 1281

Delta R.T. -0.02 min

Lab File: BG036139.D

Acq: 6 Aug 2018 22:42

Tgt Ion: 136 Resp: 93250


Ion Ratio Lower Upper

136 100

137 10.7 9.2 13.8

54 6.9 10.3 15.5#

68 6.3 4.5 6.7


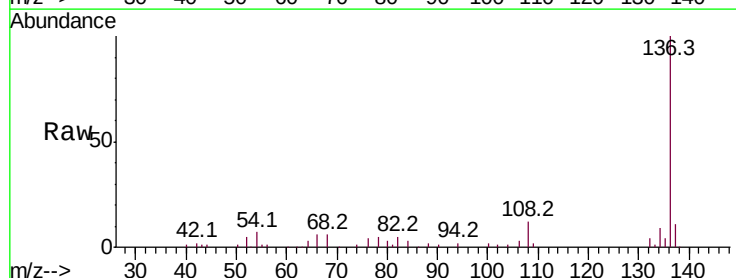



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



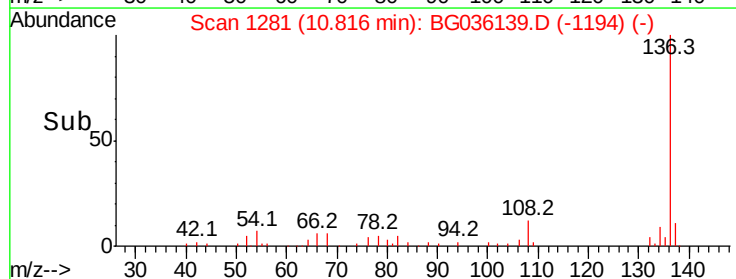
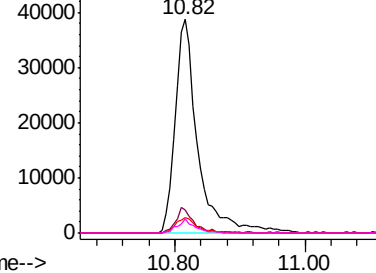


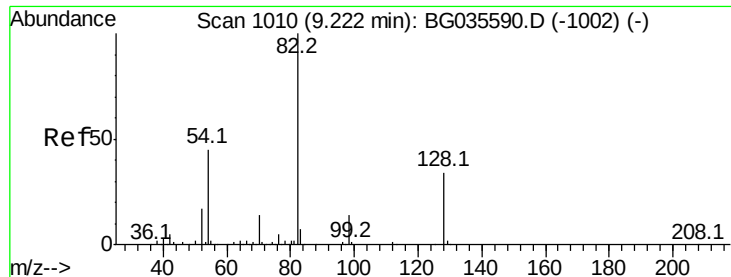

#23
 Nitrobenzene-d5
 Concen: 104.058 ng
 RT: 9.17 min Scan# 1001
 Delta R.T. -0.02 min
 Lab File: BG036139.D
 Acq: 6 Aug 2018 22:42




Instrument :
 BNA_G
 ClientSampleId :
 T40-CLAY-1


Tot Ion	82	Resp	232280
Ion Ratio	100	Lower	Upper
128	35.0	29.7	44.5
54	41.6	43.1	64.7#

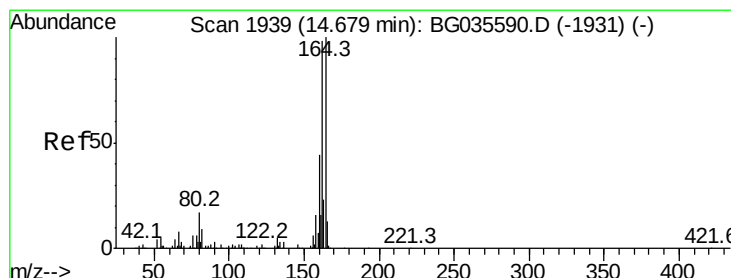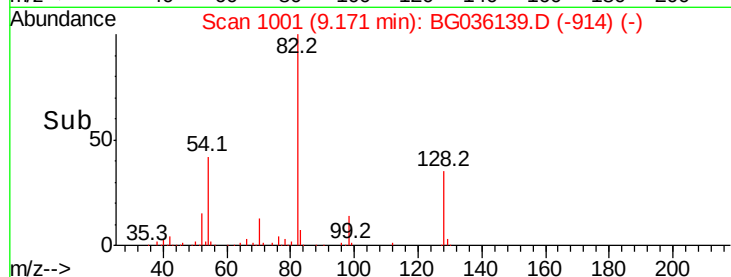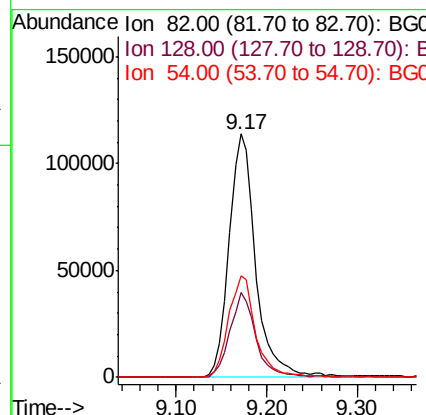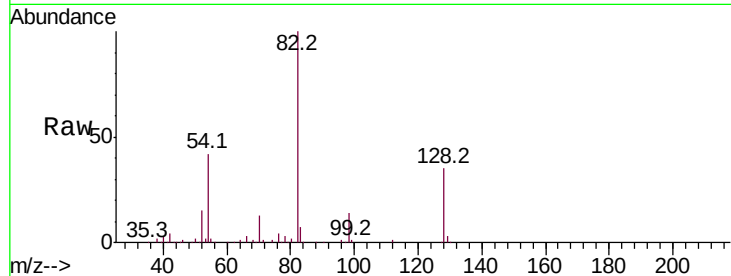

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.63 min Scan# 1931
 Delta R.T. -0.02 min
 Lab File: BG036139.D
 Acq: 6 Aug 2018 22:42

Tgt Ion	164	Resp	63608
Ion Ratio	100	Lower	Upper
162	106.8	78.8	118.2
160	47.3	35.4	53.0

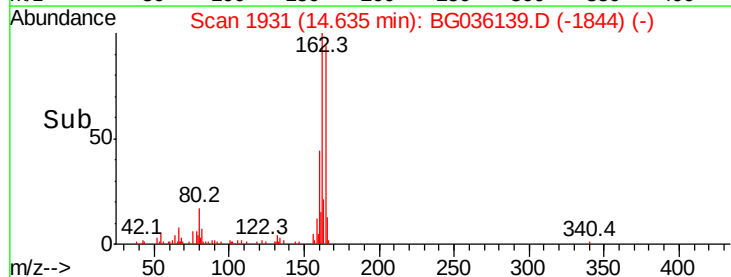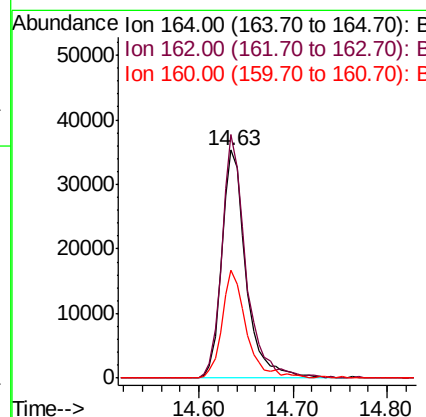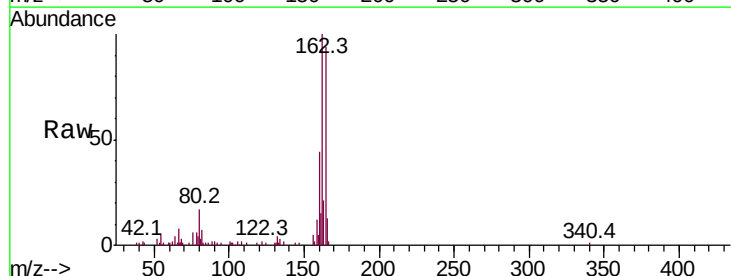


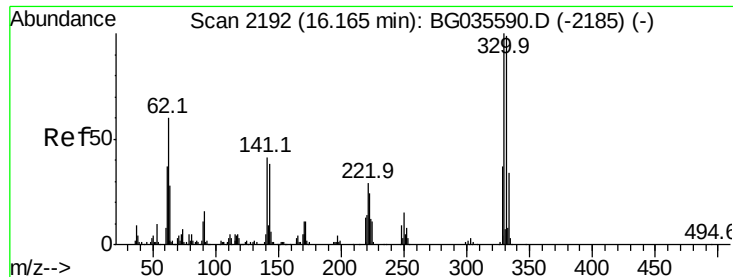




#41
 2,4,6-Tribromophenol
 Concen: 208.988 ng
 RT: 16.13 min Scan# 2185
 Delta R.T. -0.02 min
 Lab File: BG036139.D
 Acq: 6 Aug 2018 22:42

Instrument :
 BNA_G
 ClientSampleId :
 T40-CLAY-1

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.0	115.6
141	39.0	25.2	37.8#

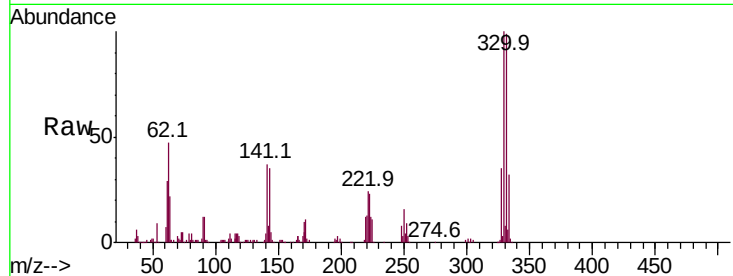


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

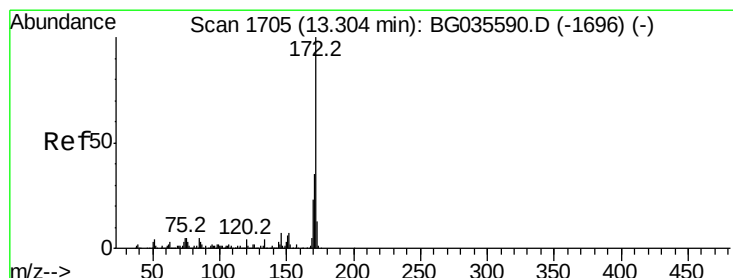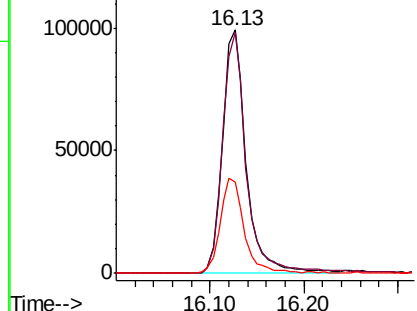
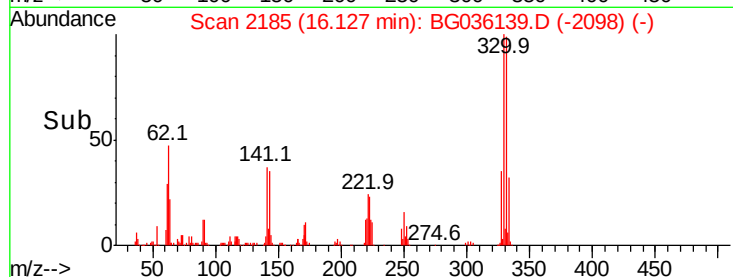



#44
 2-Fluorobiphenyl
 Concen: 108.626 ng
 RT: 13.25 min Scan# 1696
 Delta R.T. -0.02 min
 Lab File: BG036139.D
 Acq: 6 Aug 2018 22:42

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.7	30.0	45.0
170	22.2	19.5	29.3

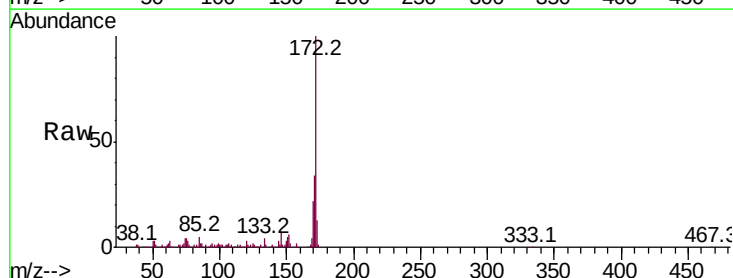

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

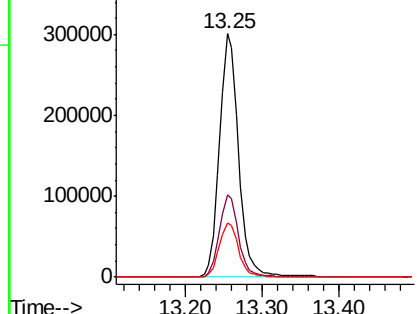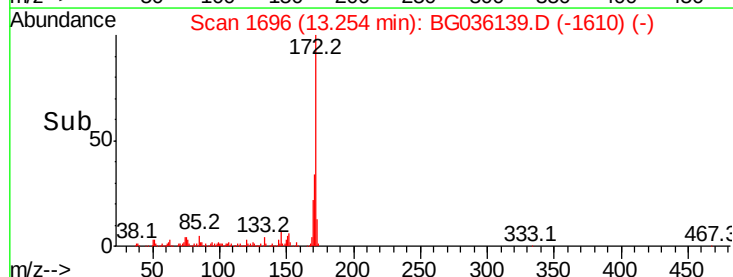

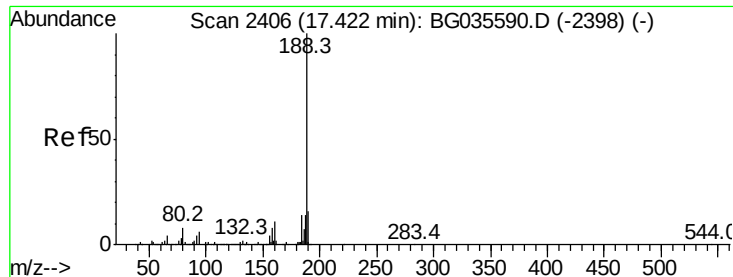

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.38 min Scan# 2398

Delta R.T. -0.02 min

Lab File: BG036139.D

Acq: 6 Aug 2018 22:42

Instrument :

BNA_G

ClientSampled :

T40-CLAY-1


Tot Ion:188 Resp: 201206

Ion Ratio Lower Upper

188 100

94 5.3 6.9 10.3#




80 8.5 7.7 11.5

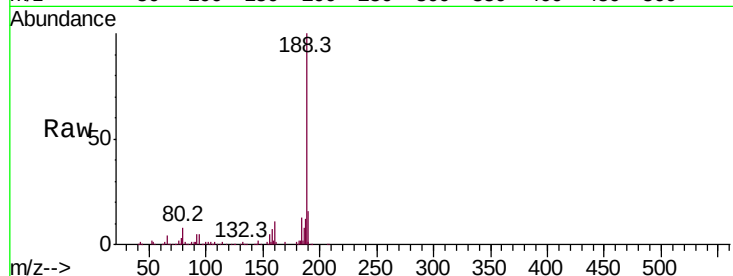

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

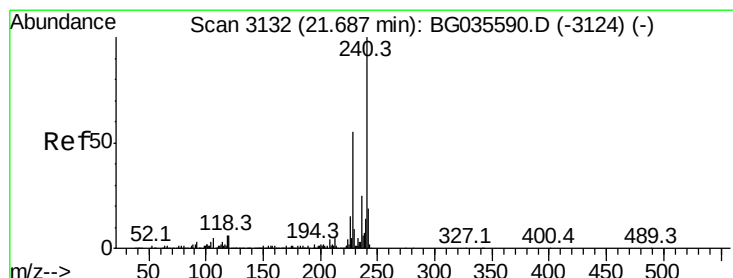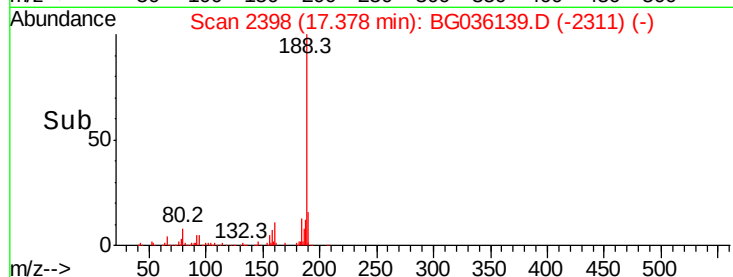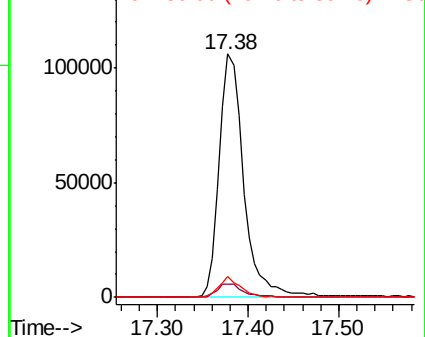

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.64 min Scan# 3124

Delta R.T. -0.02 min

Lab File: BG036139.D

Acq: 6 Aug 2018 22:42


Tgt Ion:240 Resp: 221152

Ion Ratio Lower Upper

240 100

120 5.6 6.8 10.2#



236 26.4 20.9 31.3

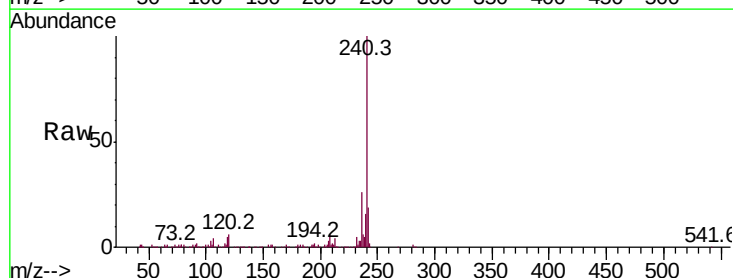


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

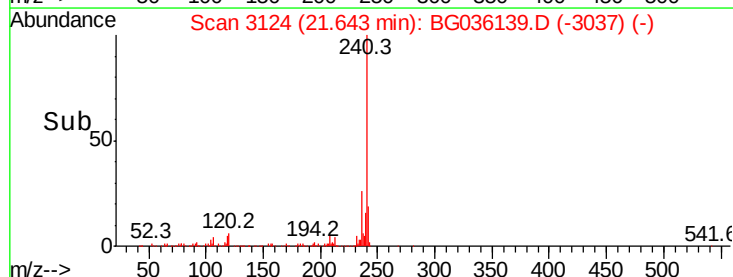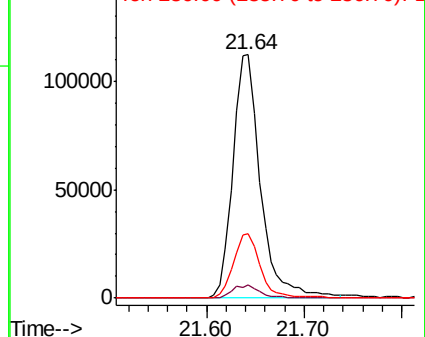

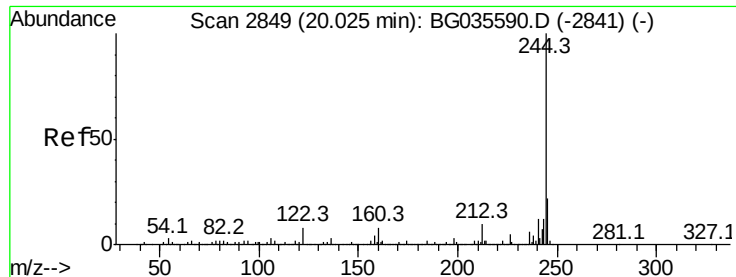

#78

Terphenyl-d14

Concen: 120.557 ng

RT: 19.99 min Scan# 2842

Delta R.T. -0.02 min

Lab File: BG036139.D

Acq: 6 Aug 2018 22:42

Instrument :

BNA_G

ClientSampleId :

T40-CLAY-1


Tot Ion:244 Resp: 1209518

Ion Ratio Lower Upper

244 100

212 9.8 5.8 8.8#




122 6.0 7.0 10.4#

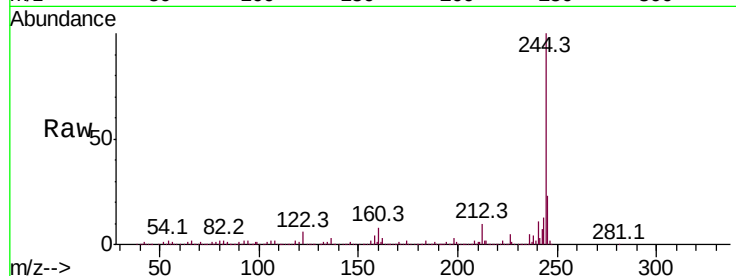

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

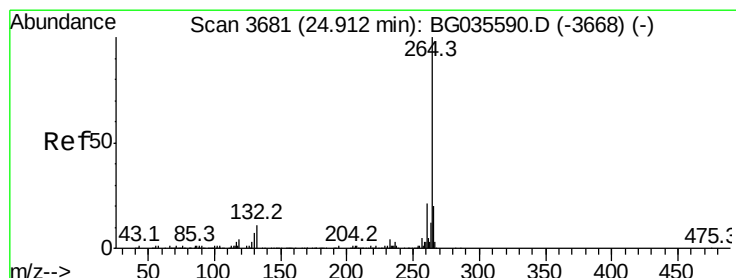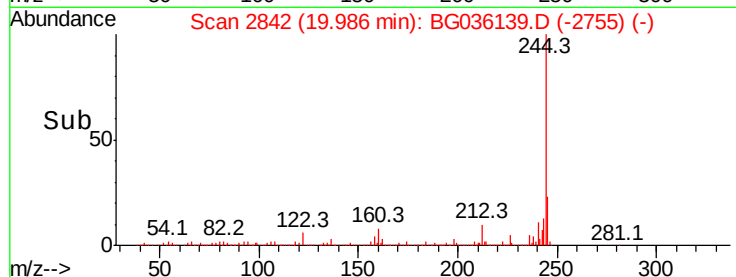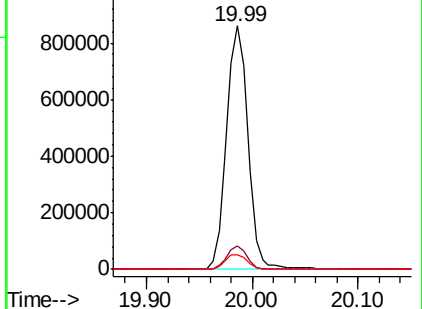

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.83 min Scan# 3666

Delta R.T. -0.03 min

Lab File: BG036139.D

Acq: 6 Aug 2018 22:42


Tgt Ion:264 Resp: 201291

Ion Ratio Lower Upper

264 100

260 22.7 17.4 26.0

265 23.8 17.7 26.5

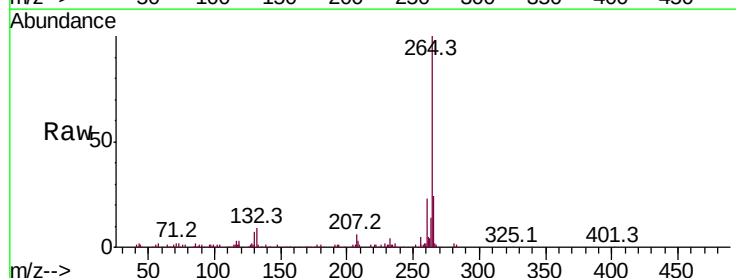

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

