


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080618\
 Data File : BG036126.D
 Acq On : 6 Aug 2018 14:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

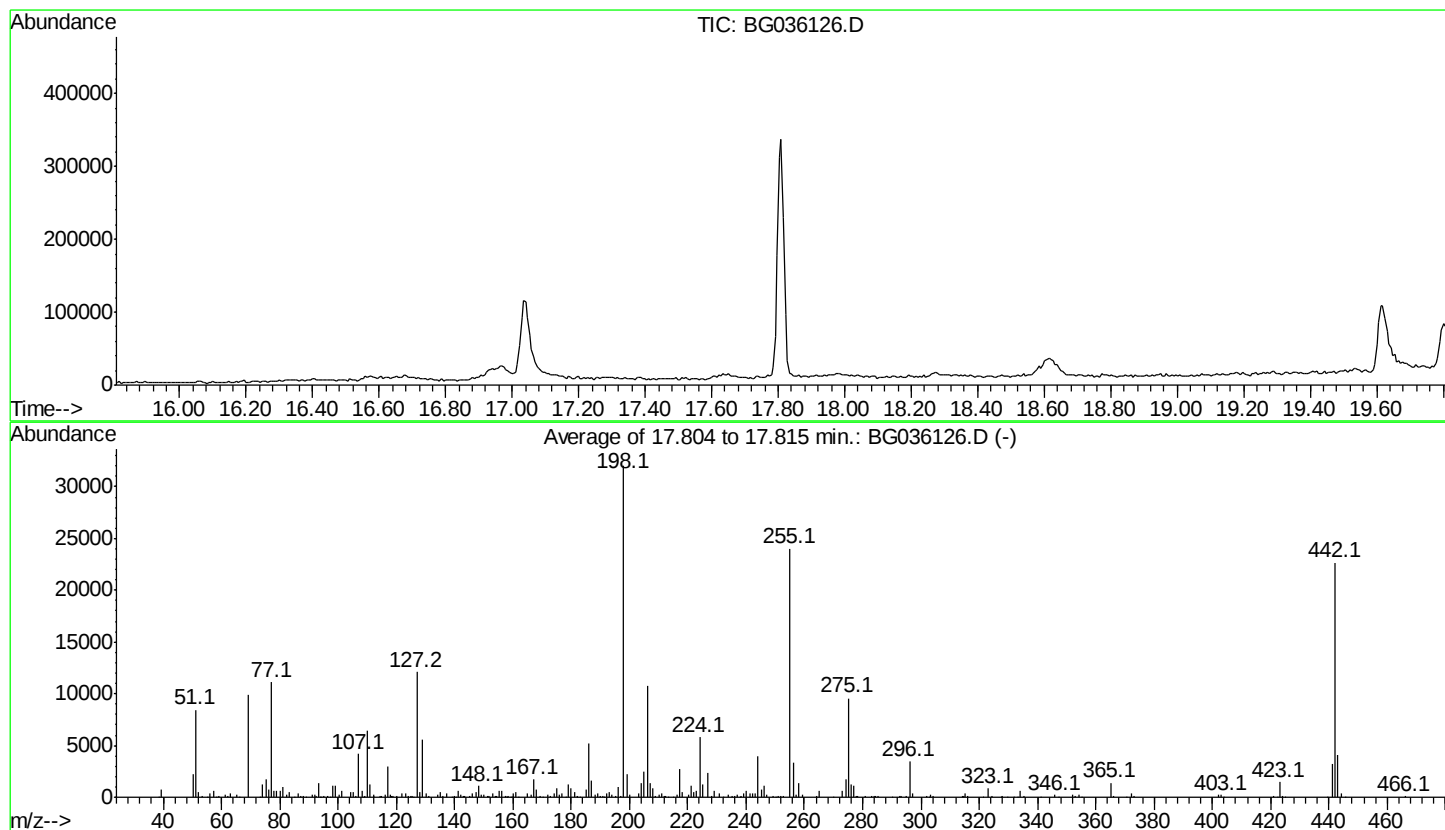

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	8467	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.8	9884	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.7	12073	PASS
197	198	0.00	2	0.6	180	PASS
198	198	100	100	100.0	32040	PASS
199	198	5	9	7.0	2241	PASS
275	198	10	60	29.8	9543	PASS
365	198	1	100	4.3	1374	PASS
441	198	0.01	100	9.9	3175	PASS
442	198	50	100	70.7	22640	PASS
443	442	15	24	18.0	4082	PASS