
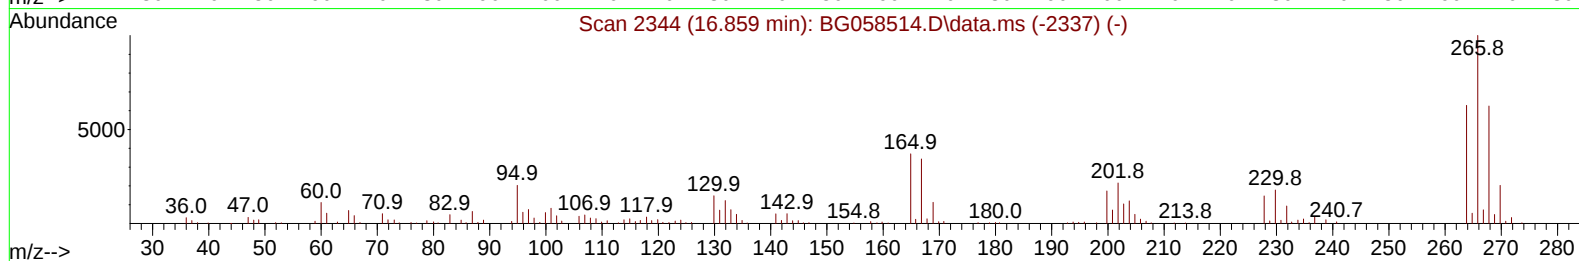
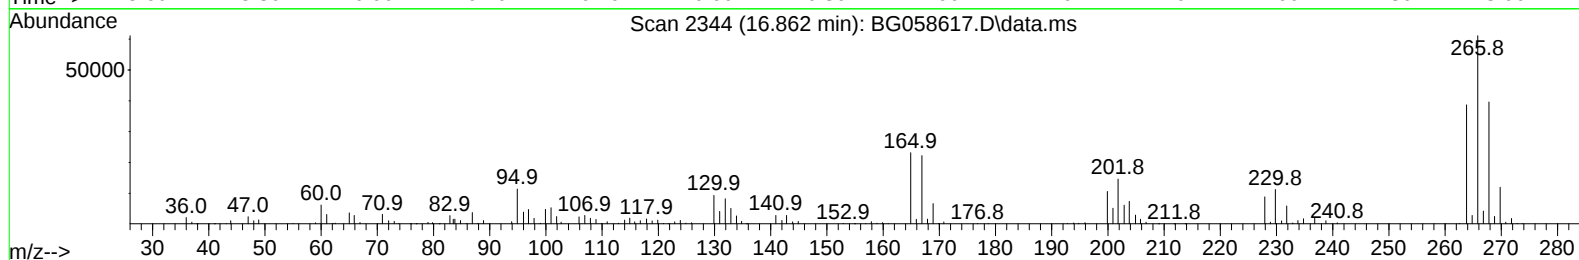


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080723\
Data File : BG058617.D
Acq On : 7 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 08:44:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

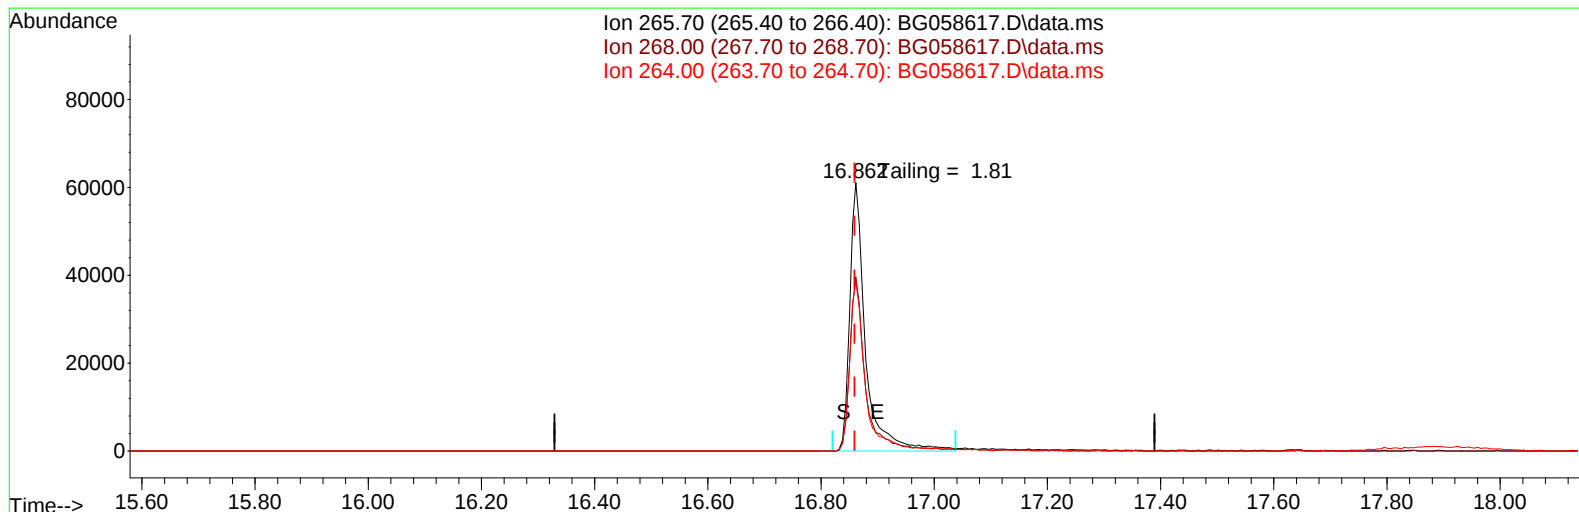

TIC: BG058617.D\data.ms

(70) Pentachlorophenol (C)




16.862min (+ 0.003) 24019.42 ng

response 118819

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.84
264.00	62.80	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080723\
Data File : BG058617.D
Acq On : 7 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 08:44:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

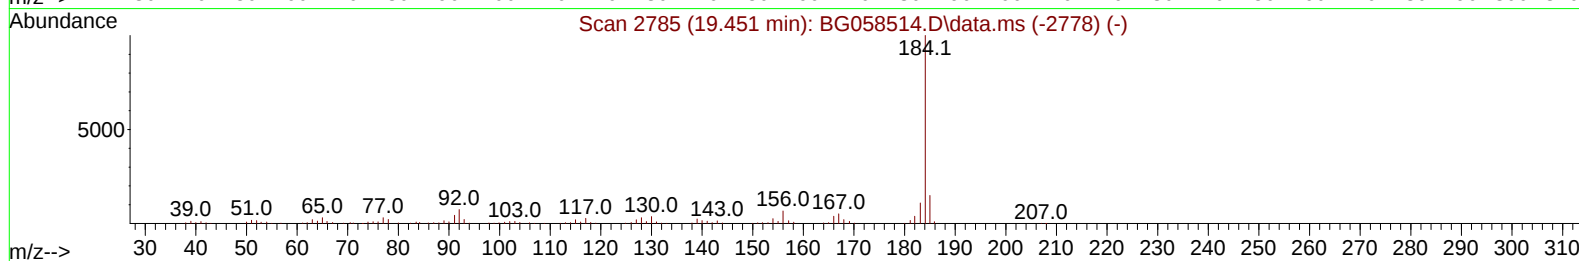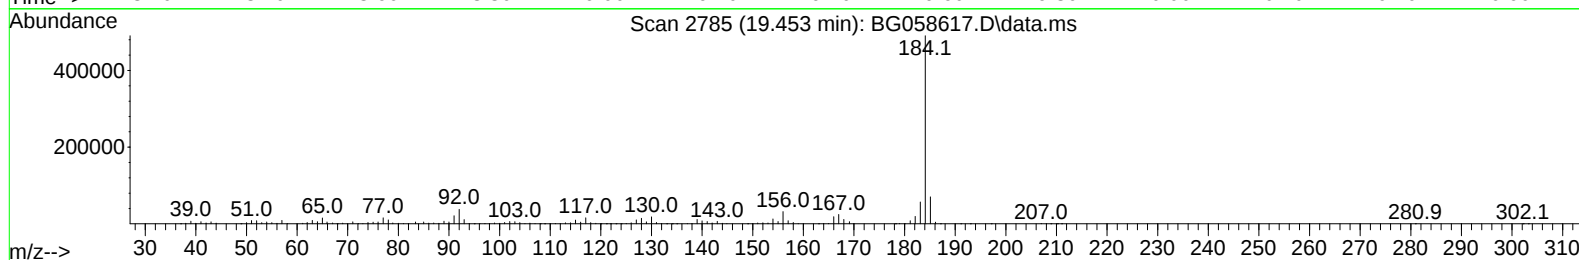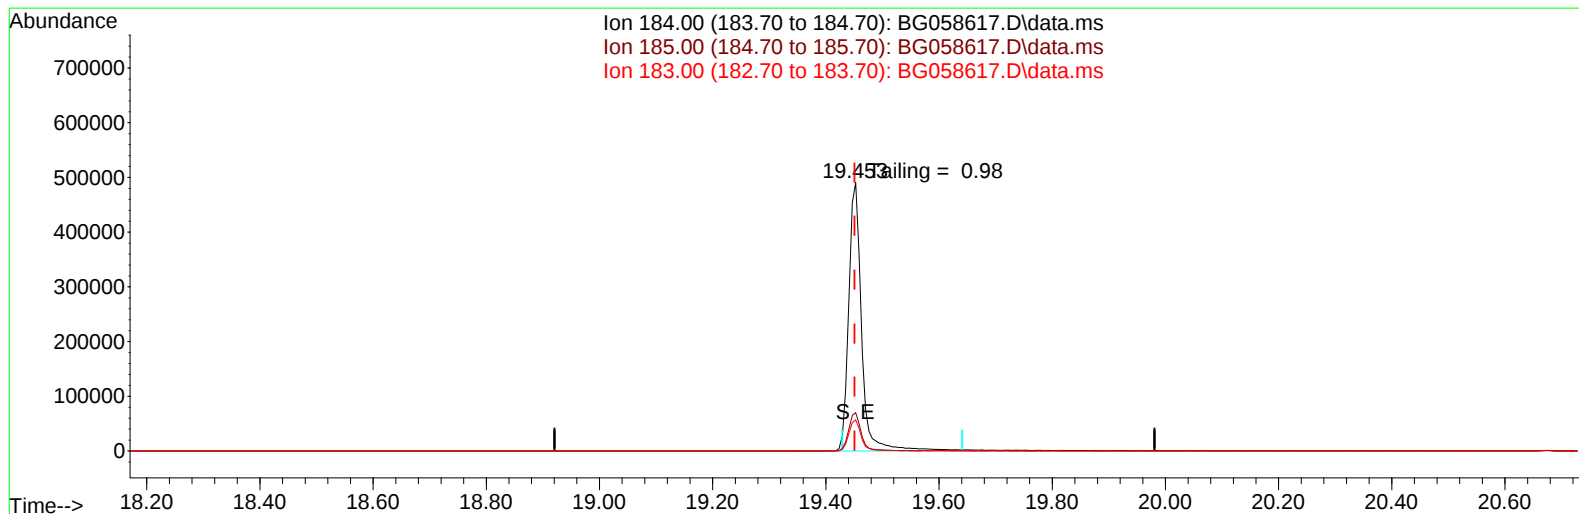

TIC: BG058617.D\data.ms

(77) Benzidine**19.453min (+ 0.002) 885399.21 ng****response 738443**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.30
183.00	10.90	11.64
0.00	0.00	0.00