

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080723\
 Data File : BG058619.D
 Acq On : 7 Aug 2023 9:27
 Operator : MA/JU
 Sample : PB154526BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB154526BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG058619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.386	384	391	403	rBV	845697	1317241	33.67%	9.262%
2	6.984	656	663	683	rBV	782572	1336662	34.16%	9.398%
3	7.812	797	804	816	rBV	127515	210463	5.38%	1.480%
4	8.975	994	1002	1019	rBV	438645	802203	20.50%	5.640%
5	10.615	1269	1281	1297	rBV	153090	304904	7.79%	2.144%
6	13.082	1694	1701	1714	rBV	1103300	1831037	46.80%	12.874%
7	14.463	1929	1936	1947	rBV	277916	447203	11.43%	3.144%
8	15.950	2183	2189	2207	rBV	951388	1628682	41.63%	11.451%
9	17.207	2395	2403	2417	rBV	411477	652195	16.67%	4.586%
10	19.827	2843	2849	2860	rBV	2880372	3912733	100.00%	27.511%
11	21.449	3119	3125	3139	rBV	485002	835294	21.35%	5.873%
12	24.522	3638	3648	3661	rBV2	314889	943890	24.12%	6.637%




Sum of corrected areas: 14222507

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080723\
Data File : BG058619.D
Acq On : 7 Aug 2023 9:27
Operator : MA/JU
Sample : PB154526BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154526BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

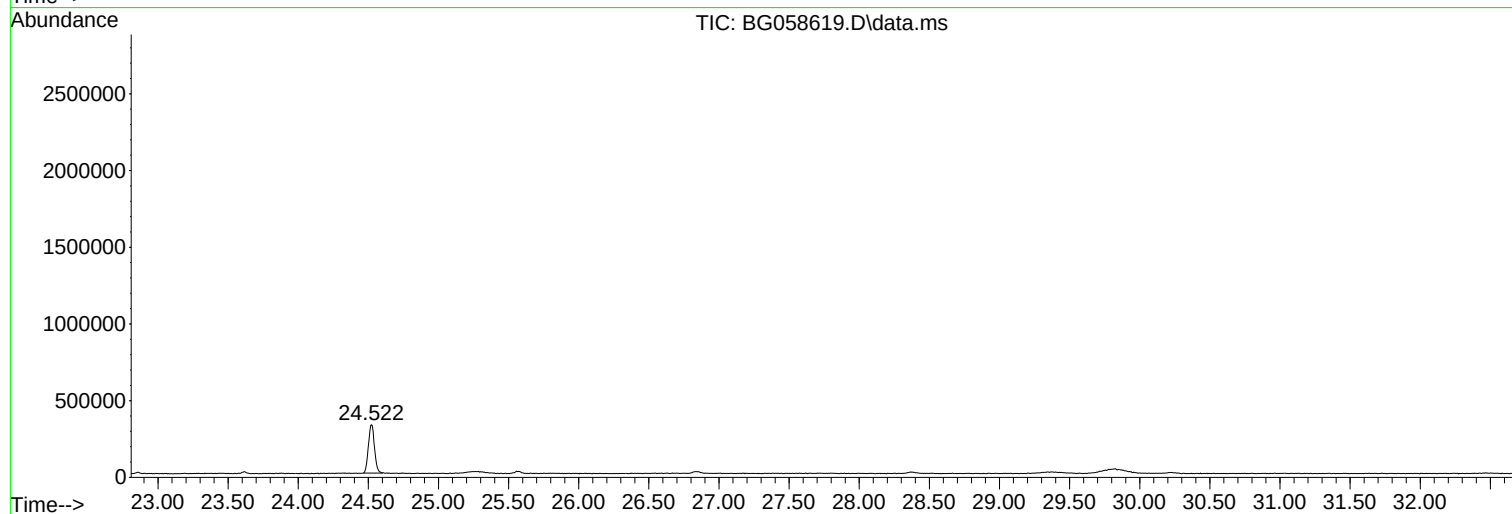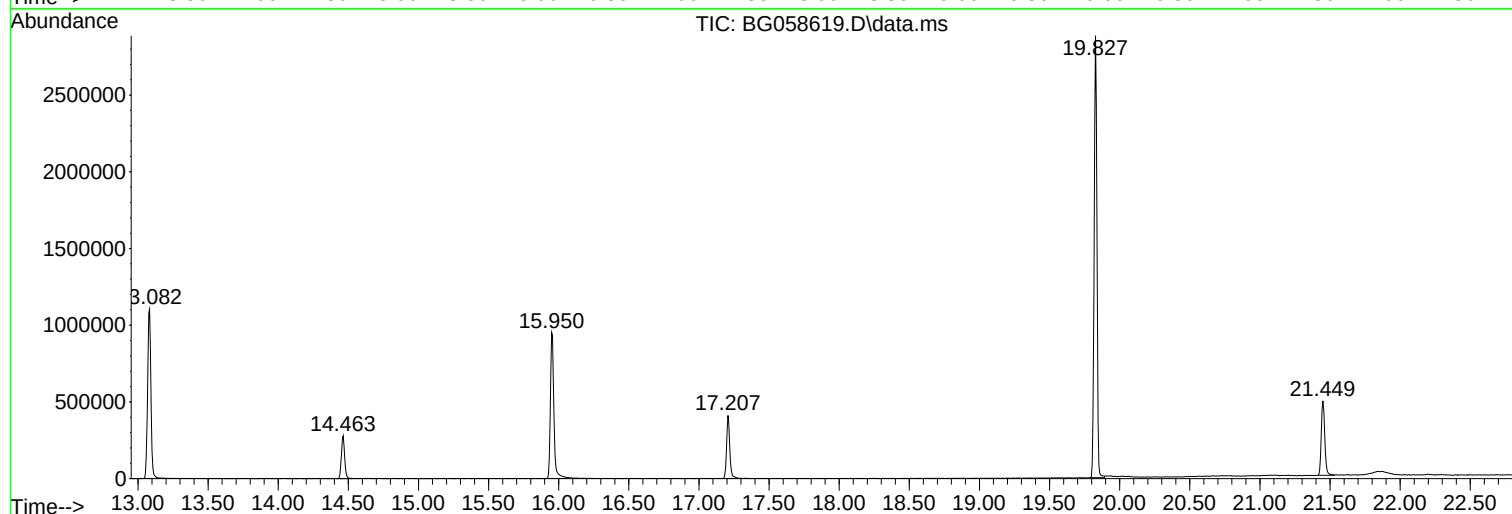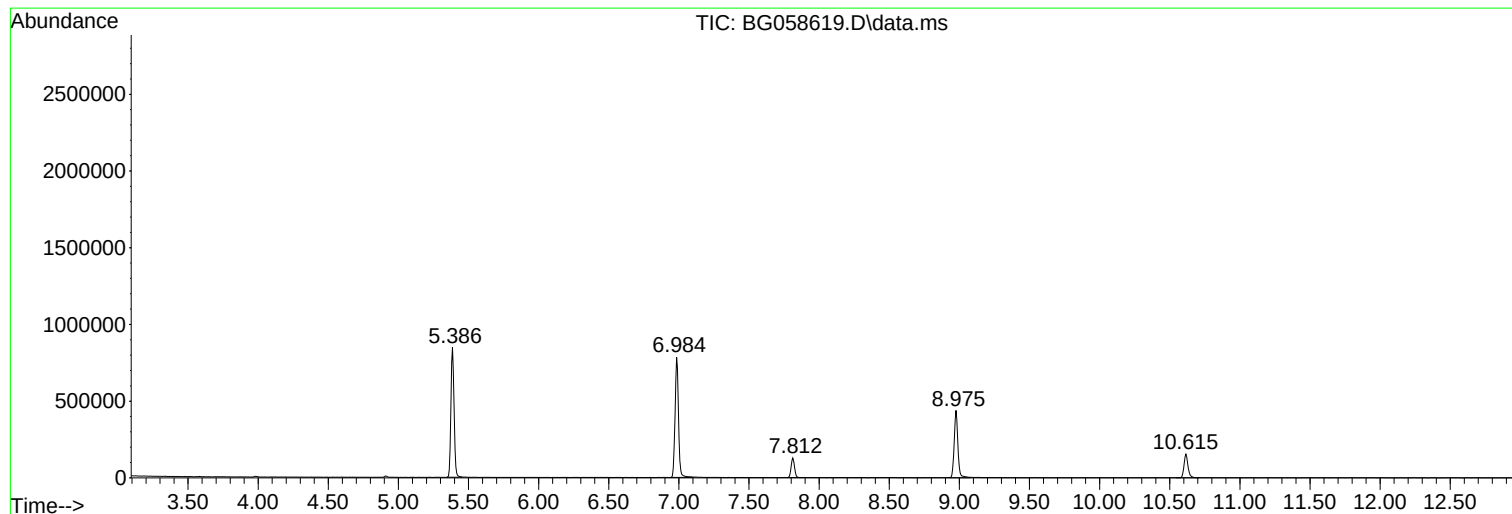

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080723\
Data File : BG058619.D
Acq On : 7 Aug 2023 9:27
Operator : MA/JU
Sample : PB154526BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154526BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080723\
Data File : BG058619.D
Acq On : 7 Aug 2023 9:27
Operator : MA/JU
Sample : PB154526BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154526BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------