


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080723\
Data File : BG058617.D
Acq On : 7 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

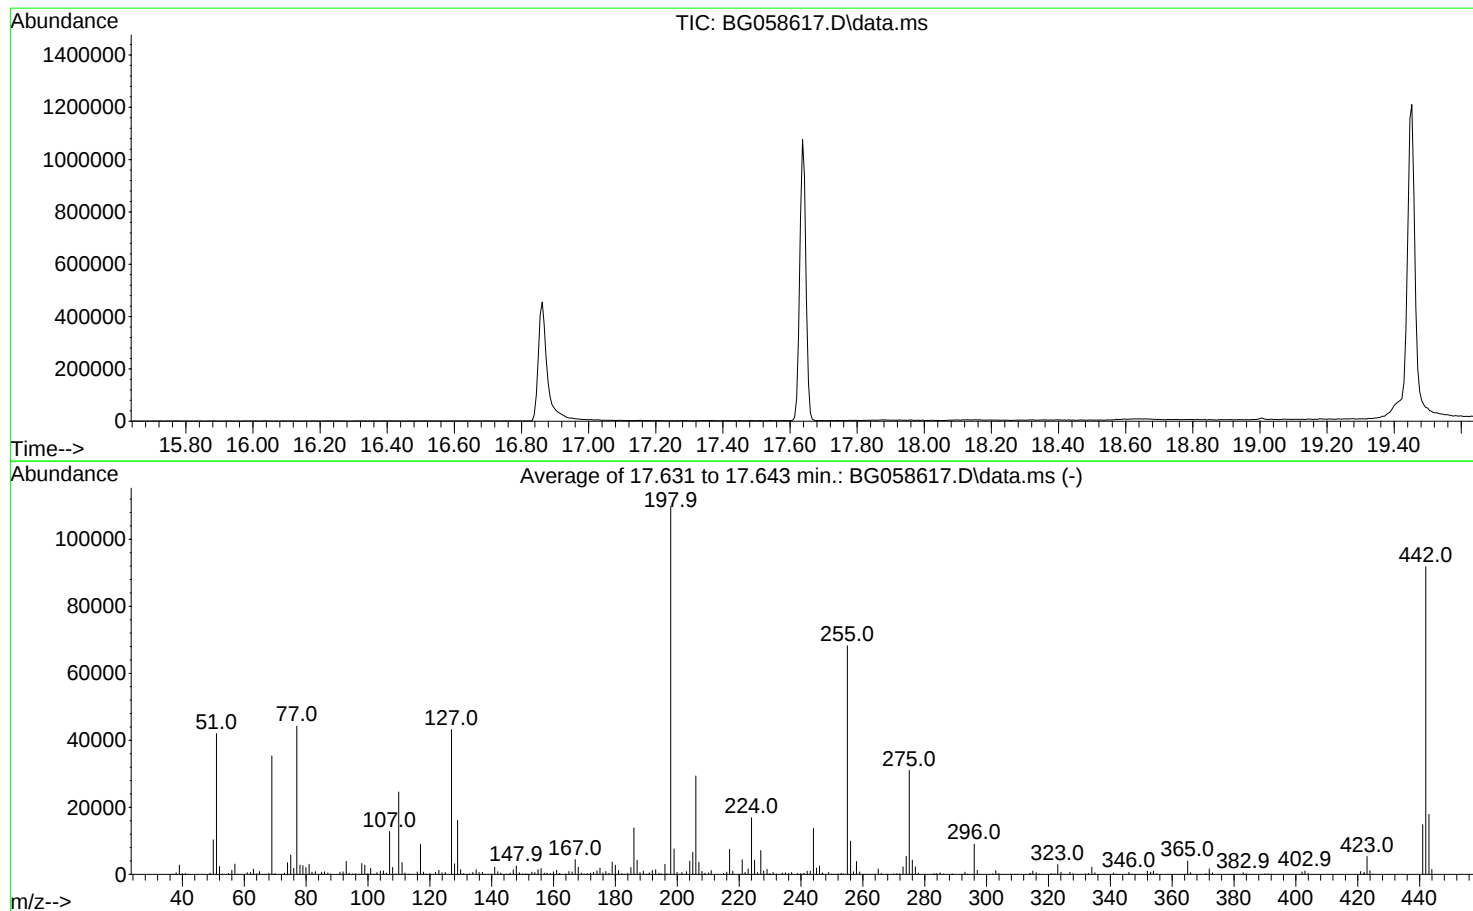




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	42027	PASS
68	69	0.00	2	1.1	374	PASS
69	198	0.00	100	32.2	35341	PASS
70	69	0.00	2	0.6	226	PASS
127	198	10	80	39.4	43216	PASS
197	198	0.00	2	0.2	184	PASS
198	198	100	100	100.0	109787	PASS
199	198	5	9	6.9	7608	PASS
275	198	10	60	28.3	31032	PASS
365	198	1	100	3.6	3960	PASS
441	198	0.01	100	13.5	14868	PASS
442	442	50	100	100.0	91827	PASS
443	442	15	24	19.5	17907	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080723\
Data File : BG058617.D
Acq On : 7 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 07 08:44:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

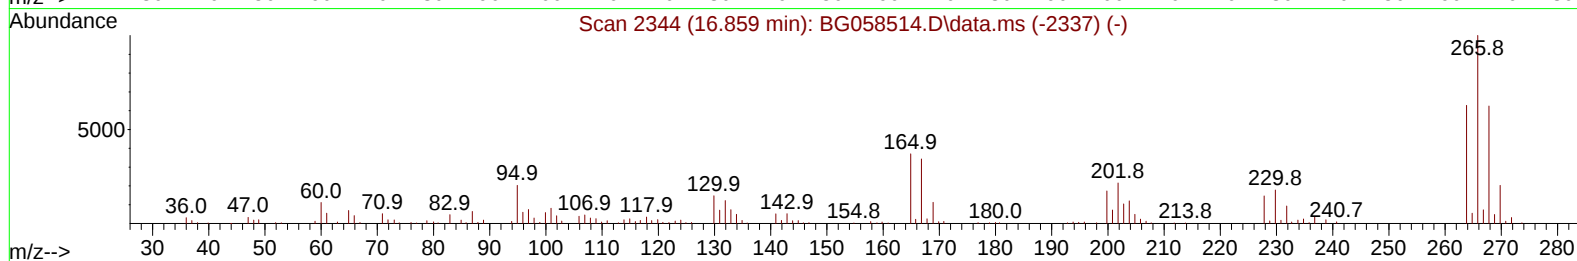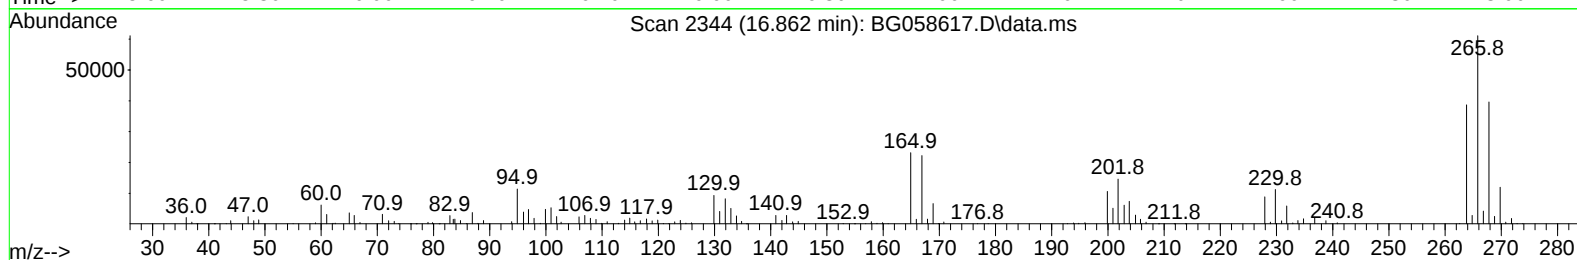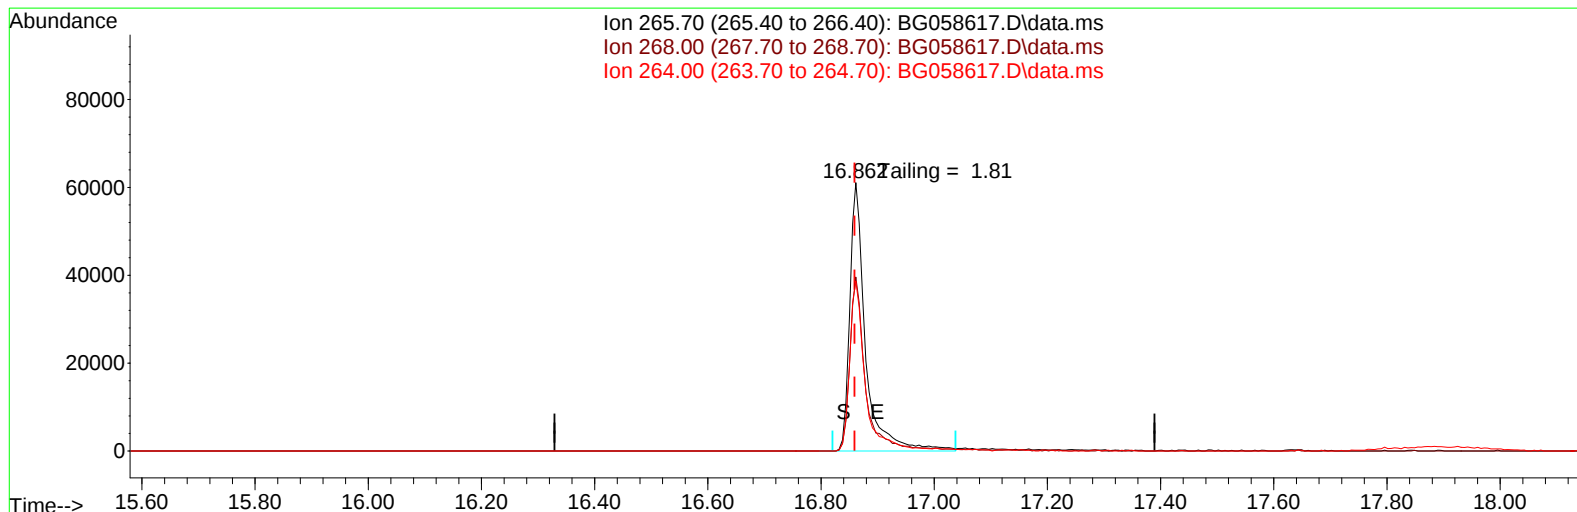

TIC: BG058617.D\data.ms

(70) Pentachlorophenol (C)

16.862min (+ 0.003) 24019.42 ng




response 118819

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.84
264.00	62.80	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080723\
Data File : BG058617.D
Acq On : 7 Aug 2023 8:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 07 08:44:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

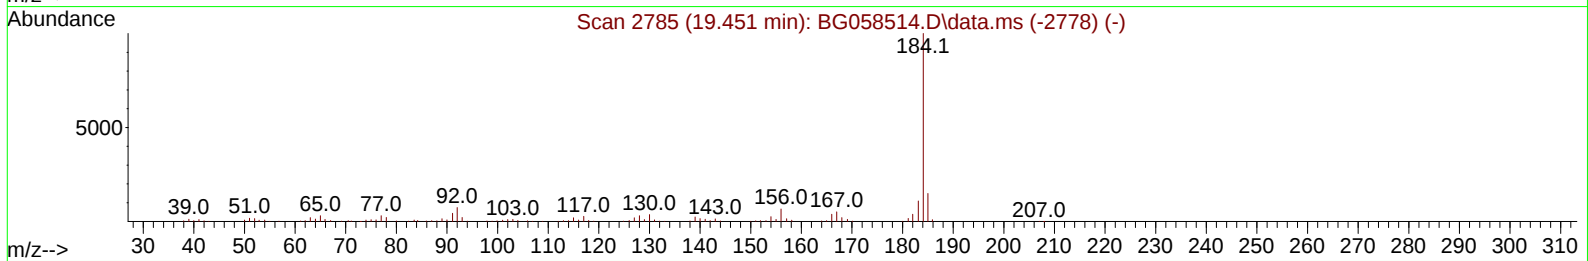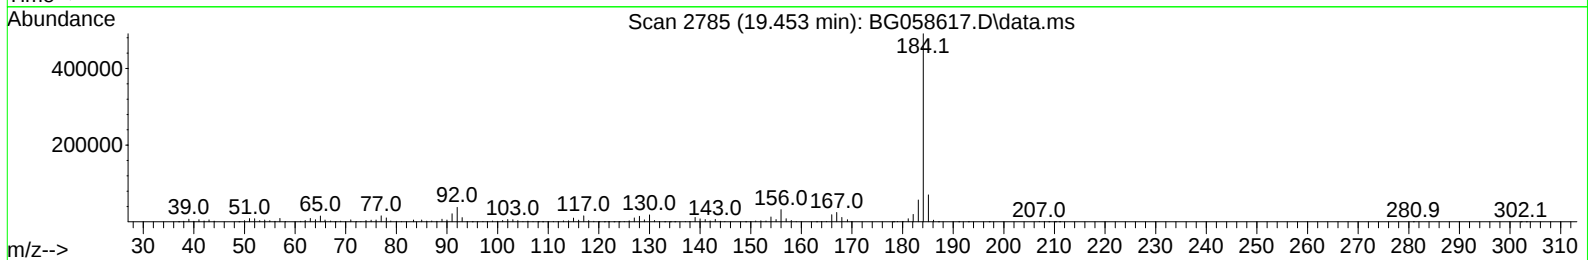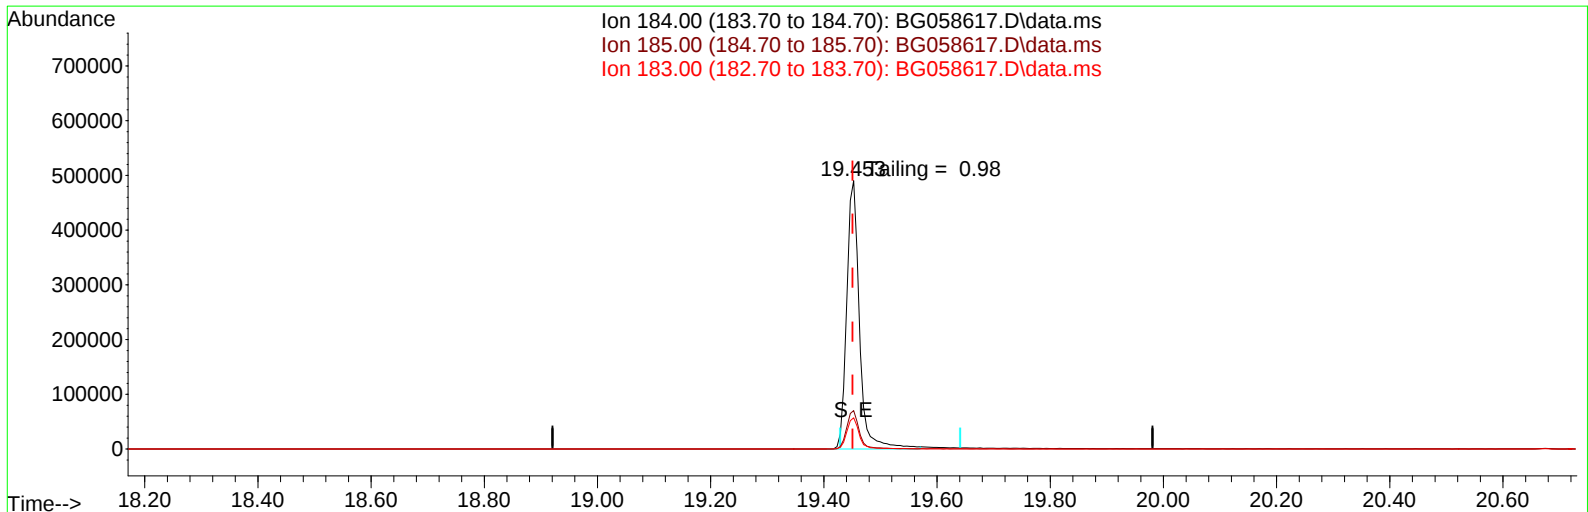

TIC: BG058617.D\data.ms

(77) Benzidine

19.453min (+ 0.002) 885399.21 ng

response 738443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.30
183.00	10.90	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/7/2023	BNA_G	<u>BG058617.D</u>
Compound Name	Response	Retention Time
DDT	360765	20.675
DDD	10890	20.24
DDE	237	19.741
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11127	371892	2.99

Instrument :
BNA_G
ClientSampleId :
DFTPP