

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG080818\
 Data File : BG036210.D
 Acq On : 8 Aug 2018 23:10
 Operator : JU/SJ
 Sample : J4360-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 155-CONCRETE

Quant Time: Aug 09 01:34:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 31 12:30:06 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	31782	20.00	ng	-0.02
21) Naphthalene-d8	10.82	136	110161	20.00	ng	-0.02
38) Acenaphthene-d10	14.63	164	81063	20.00	ng	-0.02
63) Phenanthrene-d10	17.38	188	222752	20.00	ng	-0.02
75) Chrysene-d12	21.64	240	238255	20.00	ng	-0.02
86) Perylene-d12	24.83	264	216080	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	252524	131.91	ng	0.00
7) Phenol-d6	7.19	99	325175	113.85	ng	-0.01
23) Nitrobenzene-d5	9.17	82	264822	100.42	ng	-0.02
41) 2,4,6-Tribromophenol	16.13	330	181039	169.44	ng	-0.02
44) 2-Fluorobiphenyl	13.25	172	607145	100.34	ng	-0.02
78) Terphenyl-d14	19.99	244	1199344	110.96	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.17	70	36858	15.325	ng	# 69
50) 2,6-Dinitrotoluene	14.63	165	10759	7.439	ng	# 18
53) 2,4-Dinitrophenol	15.00	184	63	6.660	ng	# 1
56) 2,4-Dinitrotoluene	14.63	165	10759	5.185	ng	# 16
66) 4-Bromophenyl-phenylether	16.12	248	14567	5.637	ng	# 1
76) Benzidine	19.99	184	20160	3.219	ng	# 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG080818\
Data File : BG036210.D
Acq On : 8 Aug 2018 23:10
Operator : JU/SJ
Sample : J4360-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
155-CONCRETE

Quant Time: Aug 09 01:34:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

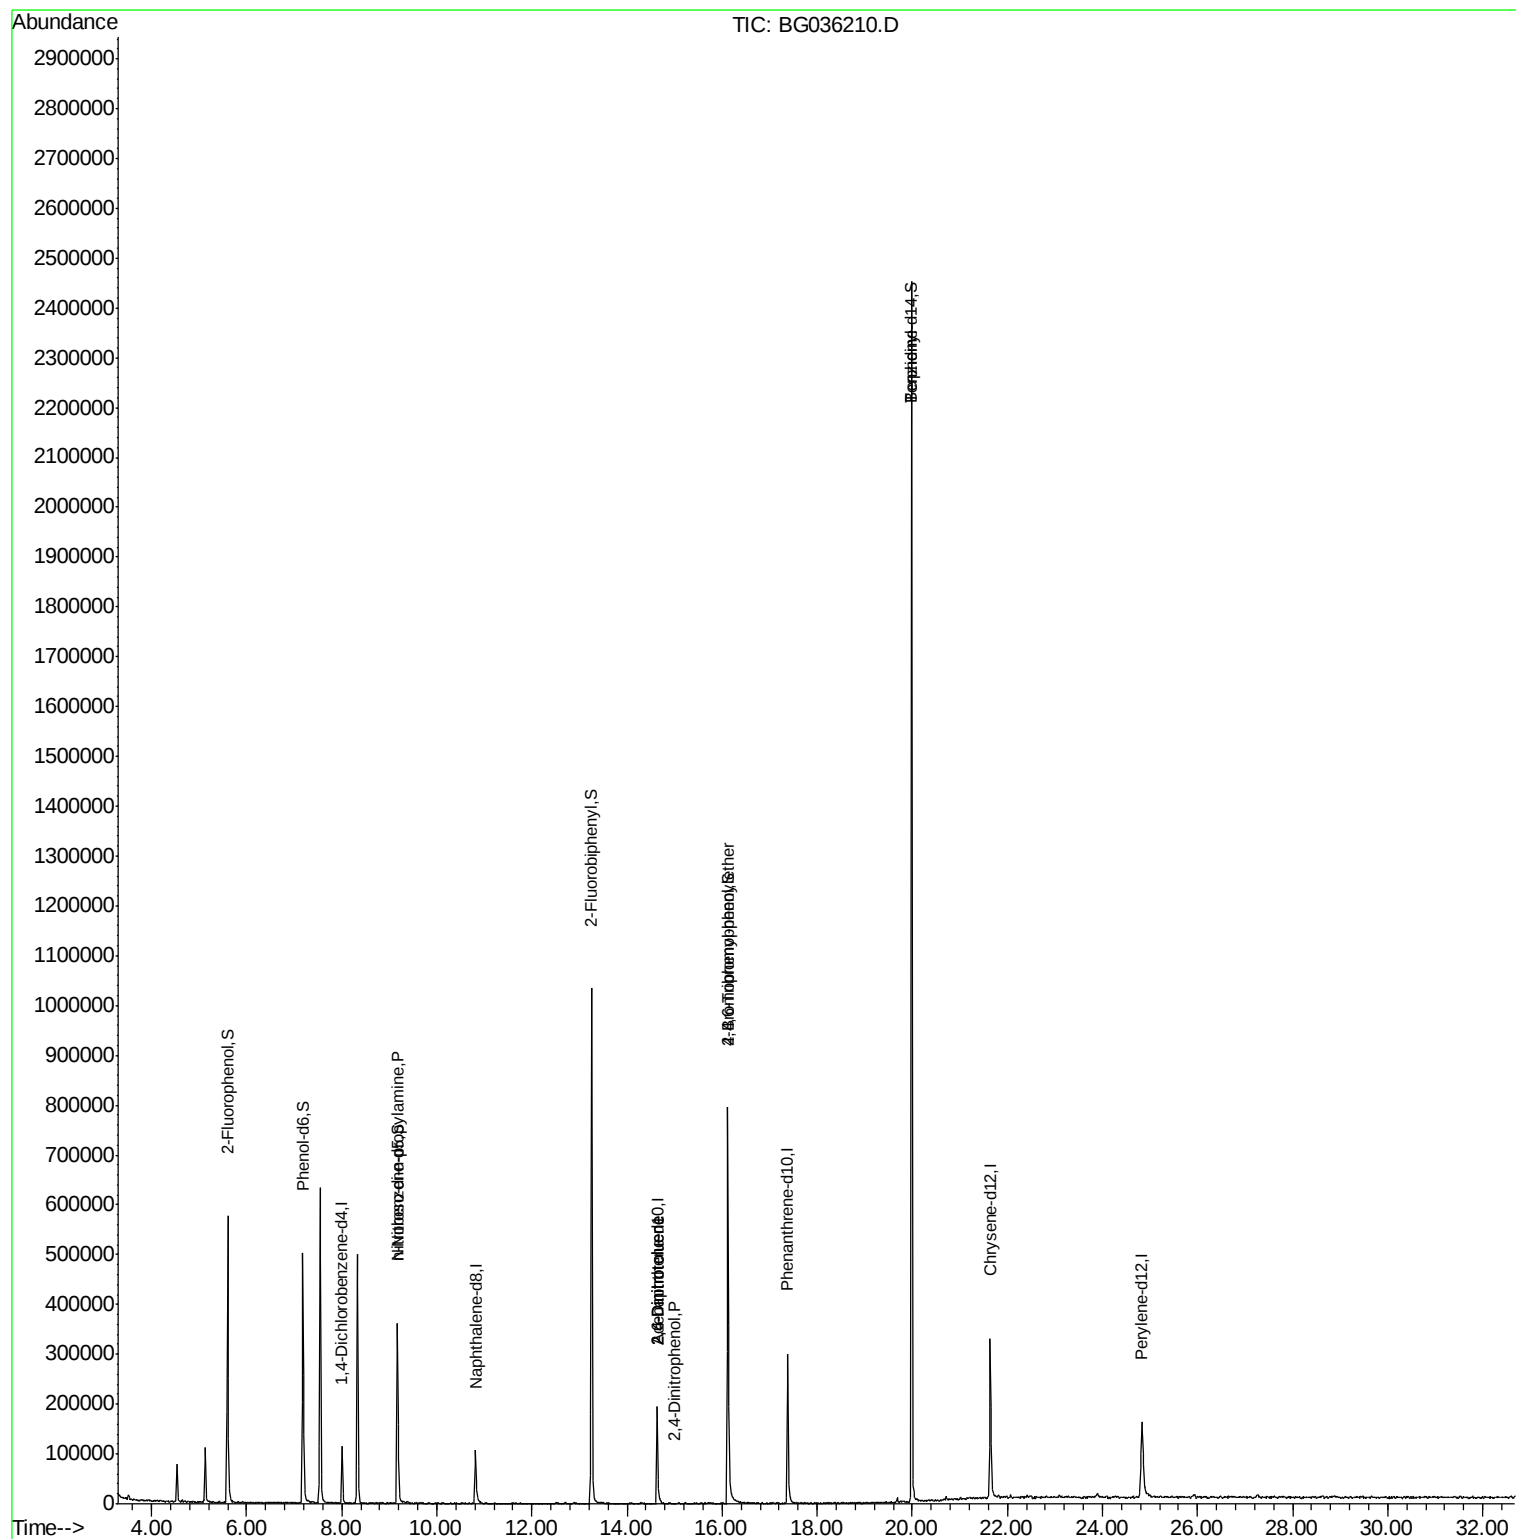




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 803
Delta R.T. -0.02 min
Lab File: BG036210.D
Acq: 8 Aug 2018 23:10

Instrument :
BNA_G
ClientSampleId :
155-CONCRETE

Tgt Ion:152 Resp: 31782
Ion Ratio Lower Upper
152 100
150 152.5 126.6 189.8
115 63.1 53.0 79.4

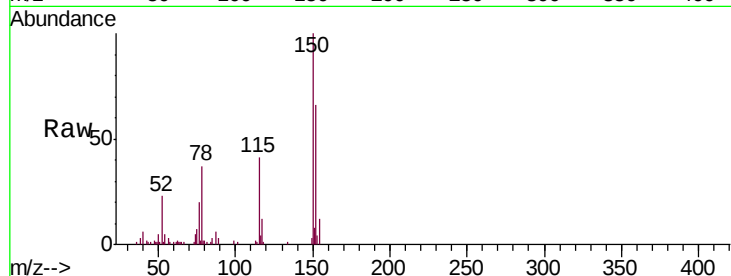


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

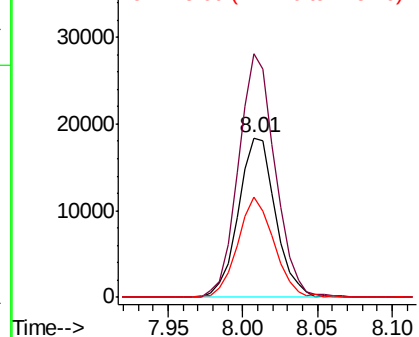



#5


2-Fluorophenol
Concen: 131.914 ng
RT: 5.60 min Scan# 393
Delta R.T. -0.00 min
Lab File: BG036210.D
Acq: 8 Aug 2018 23:10

Tgt Ion:112 Resp: 252524
Ion Ratio Lower Upper
112 100
64 63.7 56.3 84.5
63 35.7 30.1 45.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

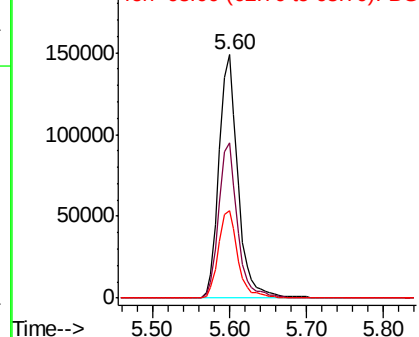



#7

Phenol-d6

Concen: 113.852 ng

RT: 7.19 min Scan# 663

Delta R.T. -0.01 min

Lab File: BG036210.D

Acq: 8 Aug 2018 23:10

Instrument :

BNA_G

ClientSampleId :

155-CONCRETE


Tgt Ion: 99 Resp: 325175

Ion Ratio Lower Upper




99 100

42 16.8 14.1 21.1

71 42.8 26.1 39.1#



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

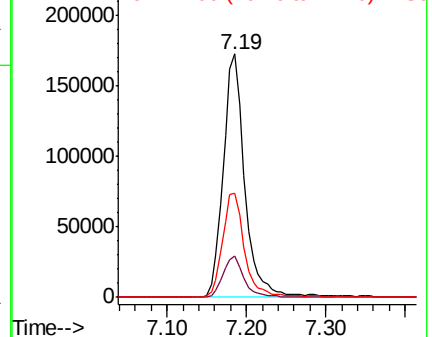

#19

n-Nitroso-di-n-propylamine

Concen: 15.325 ng

RT: 9.17 min Scan# 1001

Delta R.T. 0.34 min

Lab File: BG036210.D

Acq: 8 Aug 2018 23:10

Tgt Ion: 70 Resp: 36858


Ion Ratio Lower Upper

70 100



42 38.2 49.1 73.7#


101 0.0 8.5 12.7#

130 2.5 13.4 20.0#



Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

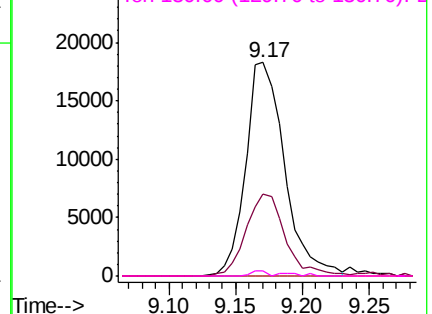







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.82 min Scan# 1281
Delta R.T. -0.02 min
Lab File: BG036210.D
Acq: 8 Aug 2018 23:10

Instrument :
BNA_G
ClientSampleId :
155-CONCRETE

Tgt Ion:	136	Resp:	110161
Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.2	13.8
54	7.6	10.3	15.5#
68	5.8	4.5	6.7

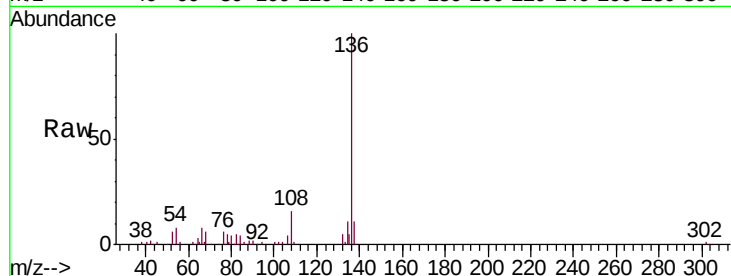


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


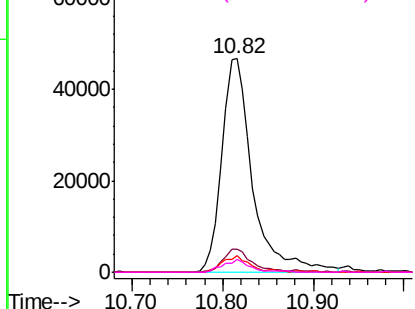


#23
Nitrobenzene-d5
Concen: 100.425 ng
RT: 9.17 min Scan# 1001
Delta R.T. -0.02 min
Lab File: BG036210.D
Acq: 8 Aug 2018 23:10

Tgt Ion:	82	Resp:	264822
Ion	Ratio	Lower	Upper
82	100		
128	36.0	29.7	44.5
54	43.2	43.1	64.7



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

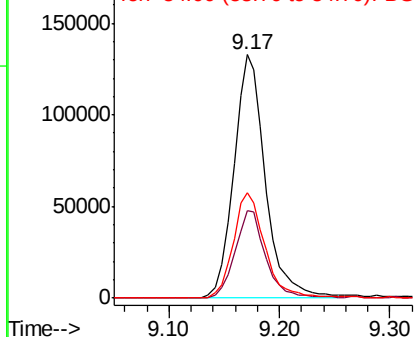



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.63 min Scan# 1931

Delta R.T. -0.02 min

Lab File: BG036210.D

Acq: 8 Aug 2018 23:10

Instrument :

BNA_G

ClientSampleId :

155-CONCRETE


Tgt Ion:164 Resp: 81063

Ion Ratio Lower Upper

164 100

162 103.1 78.8 118.2




160 47.4 35.4 53.0

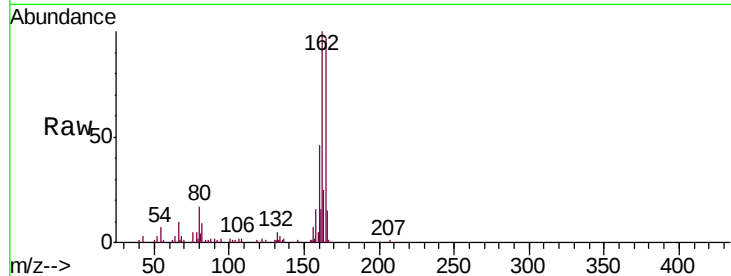

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

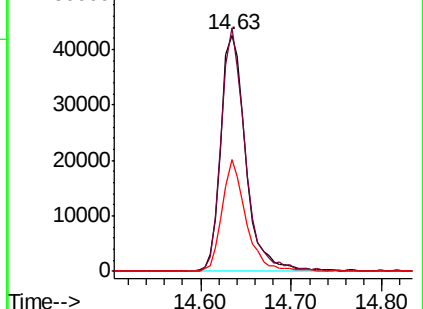

#41

2,4,6-Tribromophenol

Concen: 169.439 ng

RT: 16.13 min Scan# 2185

Delta R.T. -0.02 min

Lab File: BG036210.D

Acq: 8 Aug 2018 23:10


Tgt Ion:330 Resp: 181039

Ion Ratio Lower Upper

330 100

332 96.6 77.0 115.6



141 36.9 25.2 37.8




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



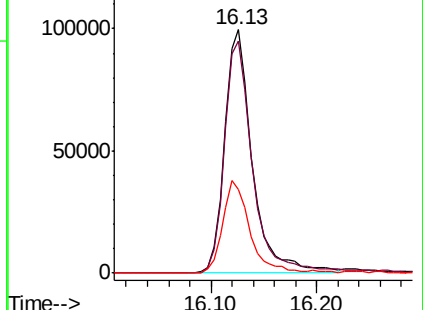



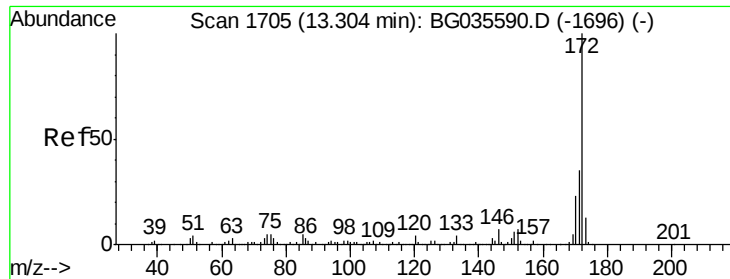

#44
 2-Fluorobiphenyl
 Concen: 100.344 ng
 RT: 13.25 min Scan# 1696
 Delta R.T. -0.02 min
 Lab File: BG036210.D
 Acq: 8 Aug 2018 23:10




Instrument :
 BNA_G
 ClientSampleId :
 155-CONCRETE


Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.8	30.0	45.0
170	22.9	19.5	29.3

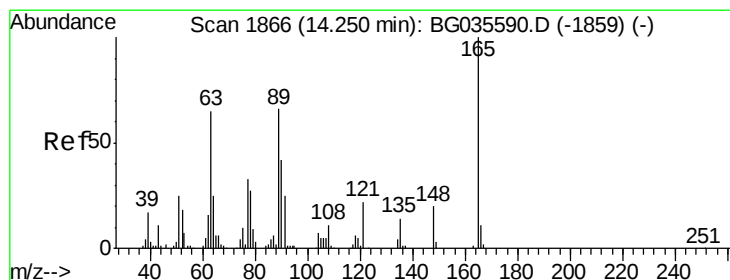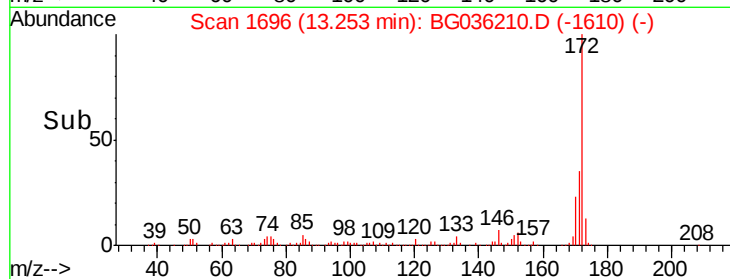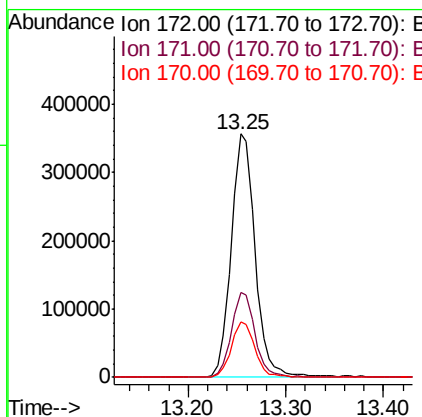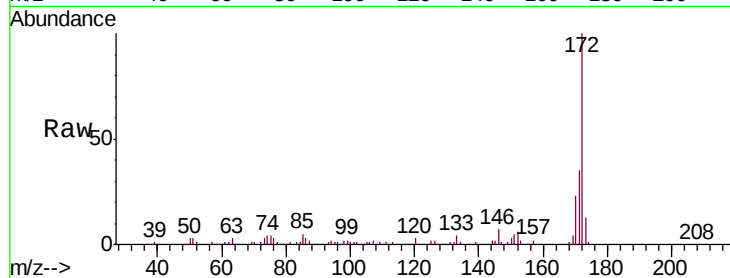

#50
 2,6-Dinitrotoluene
 Concen: 7.439 ng
 RT: 14.63 min Scan# 1931
 Delta R.T. 0.41 min
 Lab File: BG036210.D
 Acq: 8 Aug 2018 23:10

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	52.7	79.1#
89	0.0	49.2	73.8#

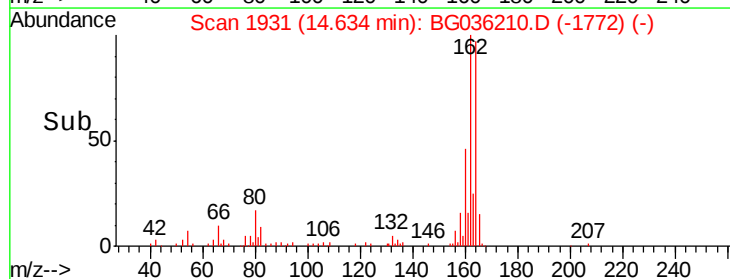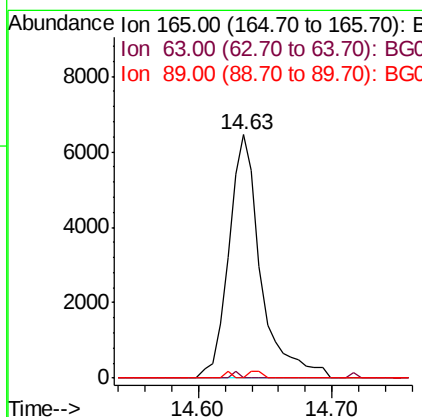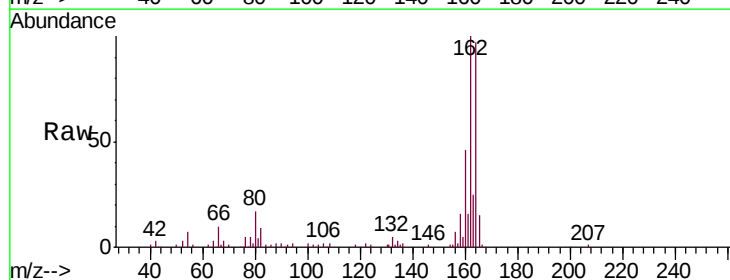


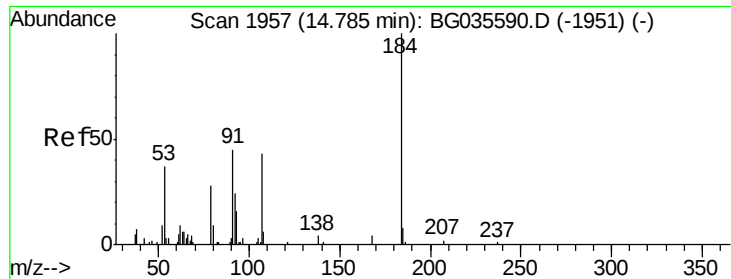




#53
 2,4-Dinitrophenol
 Concen: 6.660 ng
 RT: 15.00 min Scan# 1993
 Delta R.T. 0.24 min
 Lab File: BG036210.D
 Acq: 8 Aug 2018 23:10

Instrument :
 BNA_G
 ClientSampleId :
 155-CONCRETE

Tgt Ion:184 Resp: 63
 Ion Ratio Lower Upper
 184 100
 63 0.0 59.8 89.8#
 154 0.0 101.8 152.8#




Abundance Ion 184.00 (183.70 to 184.70): E
 Ion 63.00 (62.70 to 63.70): BG
 Ion 154.00 (153.70 to 154.70): E

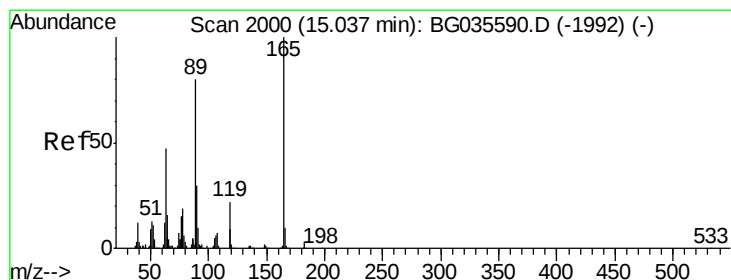
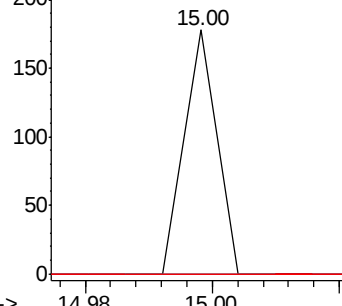



#56
 2,4-Dinitrotoluene
 Concen: 5.185 ng
 RT: 14.63 min Scan# 1931
 Delta R.T. -0.38 min
 Lab File: BG036210.D
 Acq: 8 Aug 2018 23:10

Tgt Ion:165 Resp: 10759
 Ion Ratio Lower Upper
 165 100
 63 0.0 42.0 63.0#
 89 0.0 66.9 100.3#
 182 0.0 2.6 3.8#

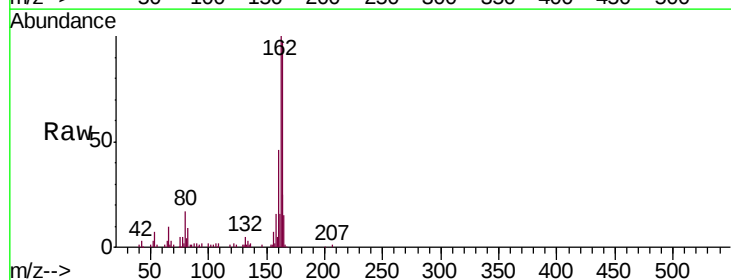

Abundance Ion 165.00 (164.70 to 165.70): E
 10000 Ion 63.00 (62.70 to 63.70): BG
 Ion 89.00 (88.70 to 89.70): BG
 Ion 182.00 (181.70 to 182.70): E



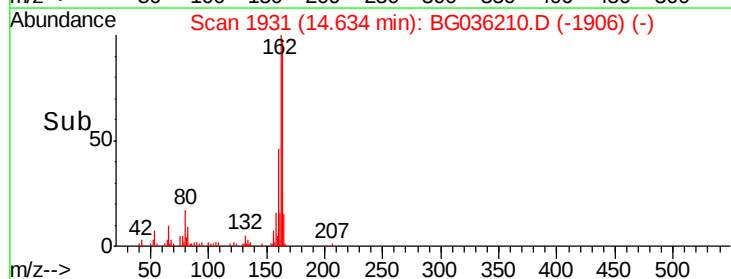
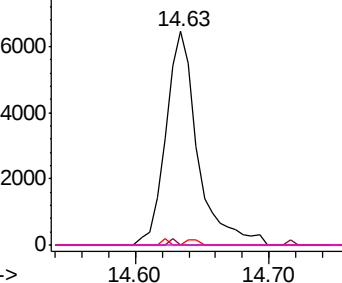




#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.38 min Scan# 2398
 Delta R.T. -0.02 min
 Lab File: BG036210.D
 Acq: 8 Aug 2018 23:10




Instrument :
 BNA_G
 ClientSampleId :
 155-CONCRETE

Tgt Ion:188 Resp: 222752
 Ion Ratio Lower Upper
 188 100
 94 5.9 6.9 10.3#
 80 7.0 7.7 11.5#

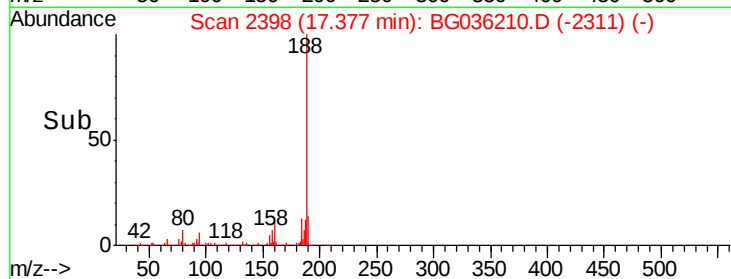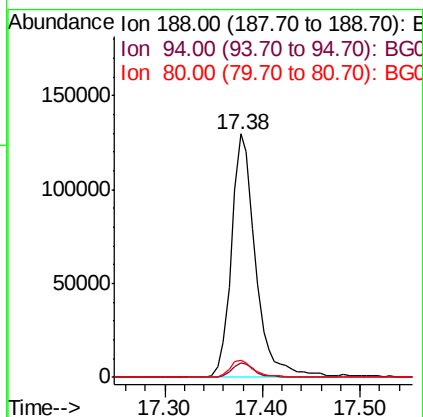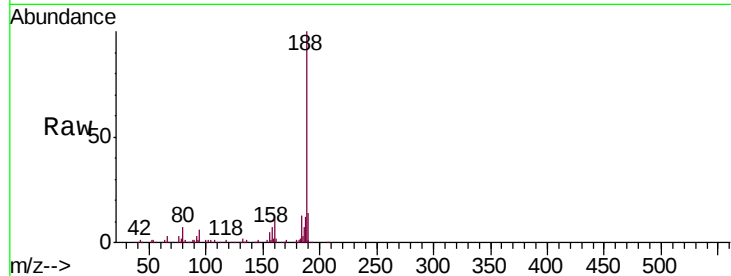

#66
 4-Bromophenyl-phenylether
 Concen: 5.637 ng
 RT: 16.12 min Scan# 2184
 Delta R.T. -0.46 min
 Lab File: BG036210.D
 Acq: 8 Aug 2018 23:10

Tgt Ion:248 Resp: 14567
 Ion Ratio Lower Upper
 248 100
 250 178.8 77.1 115.7#
 141 450.6 50.8 76.2#

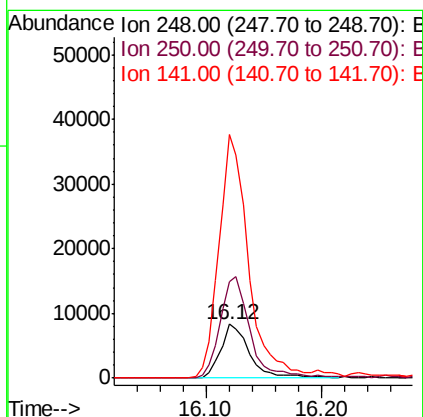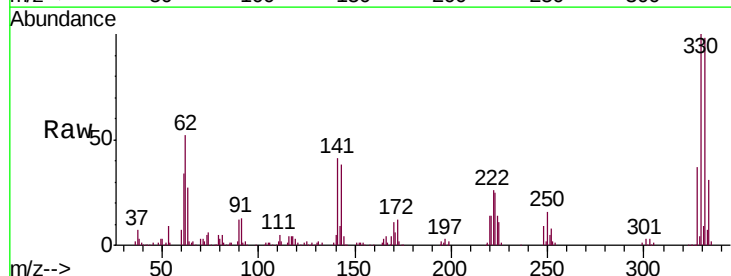



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.64 min Scan# 3124

Delta R.T. -0.02 min

Lab File: BG036210.D

Acq: 8 Aug 2018 23:10

Instrument :

BNA_G

ClientSampleId :

155-CONCRETE


Tgt Ion:240 Resp: 238255

Ion Ratio Lower Upper

240 100

120 4.5 6.8 10.2#




236 25.1 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

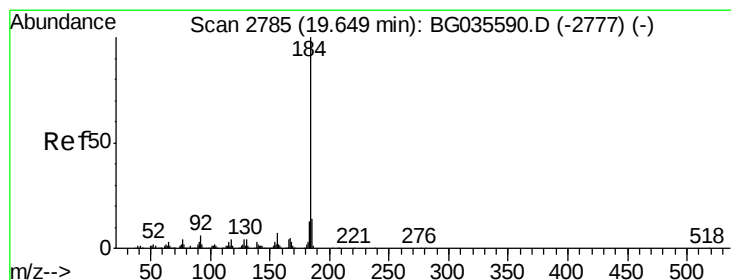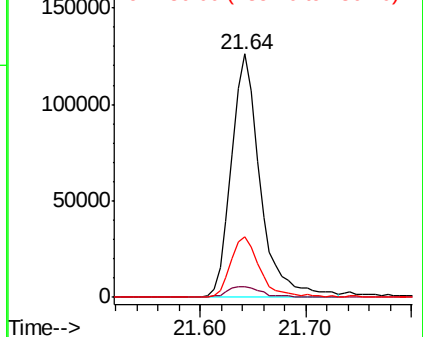

#76

Benzidine

Concen: 3.219 ng

RT: 19.99 min Scan# 2842

Delta R.T. 0.36 min

Lab File: BG036210.D

Acq: 8 Aug 2018 23:10


Tgt Ion:184 Resp: 20160

Ion Ratio Lower Upper

184 100

185 14.5 11.1 16.7



183 7.2 10.6 16.0#




Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

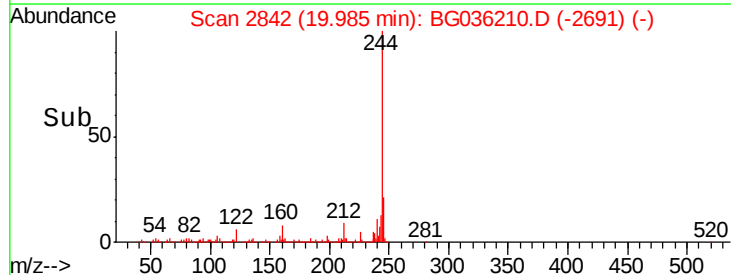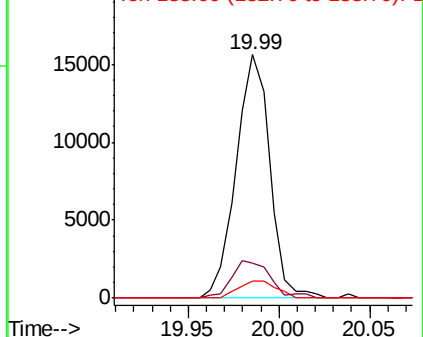

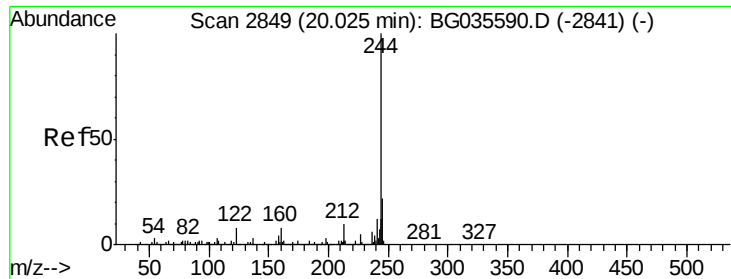

#78

Terphenyl-d14

Concen: 110.962 ng

RT: 19.99 min Scan# 2842

Delta R.T. -0.02 min

Lab File: BG036210.D

Acq: 8 Aug 2018 23:10

Instrument :

BNA_G

ClientSampleId :

155-CONCRETE


Tgt Ion:244 Resp: 1199344

Ion Ratio Lower Upper




244 100

212 9.1 5.8 8.8#

122 6.3 7.0 10.4#

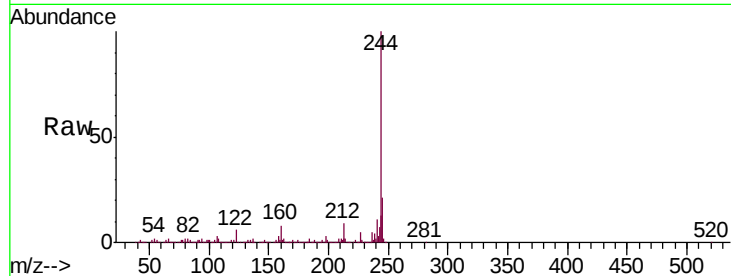

Abundance Ion 244.00 (243.70 to 244.70): E
1200000
Ion 212.00 (211.70 to 212.70): E
1000000
Ion 122.00 (121.70 to 122.70): E

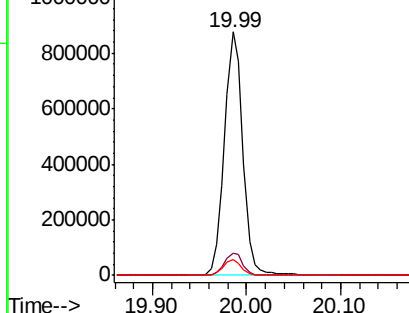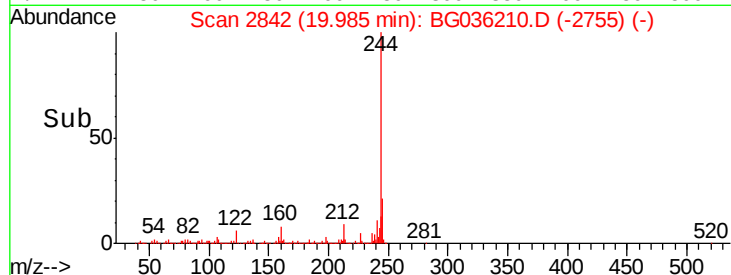

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.83 min Scan# 3667

Delta R.T. -0.03 min

Lab File: BG036210.D

Acq: 8 Aug 2018 23:10


Tgt Ion:264 Resp: 216080

Ion Ratio Lower Upper

264 100

260 23.1 17.4 26.0

265 21.4 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E
80000
Ion 260.00 (259.70 to 260.70): E
60000
Ion 265.00 (264.70 to 265.70): E

