
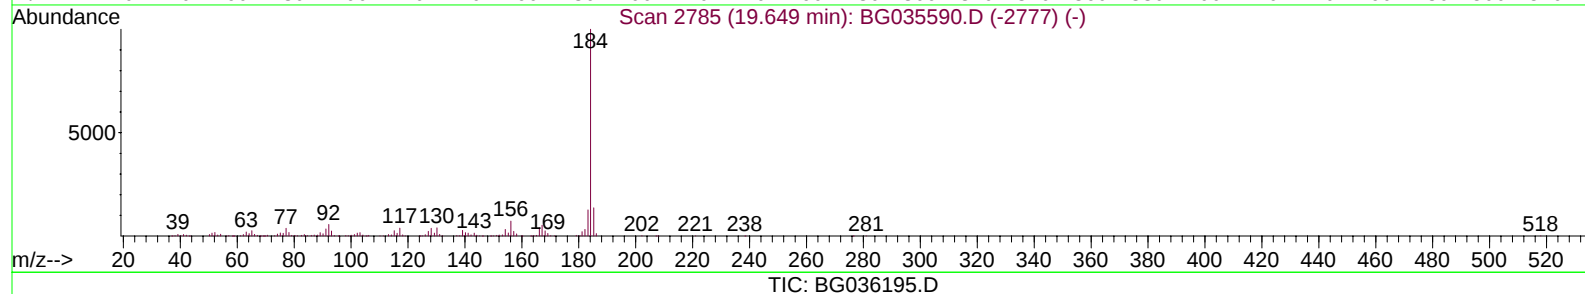
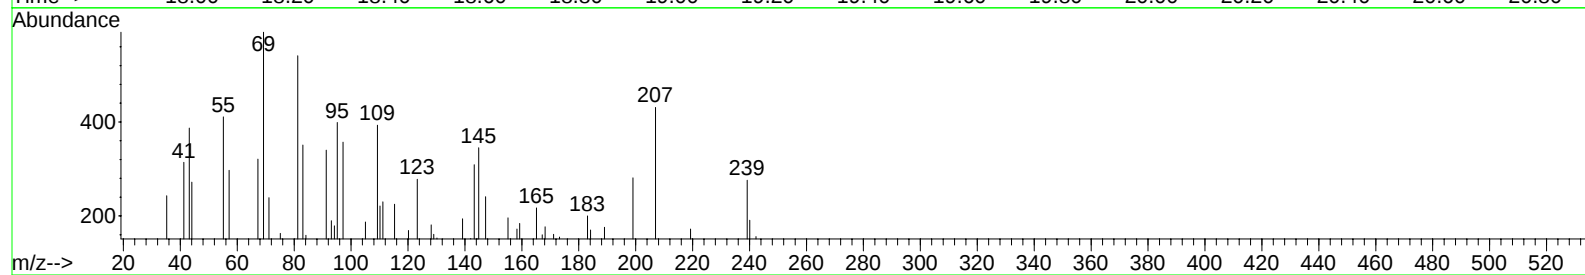


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080818\
Data File : BG036195.D
Acq On : 8 Aug 2018 13:19
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 18:32:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

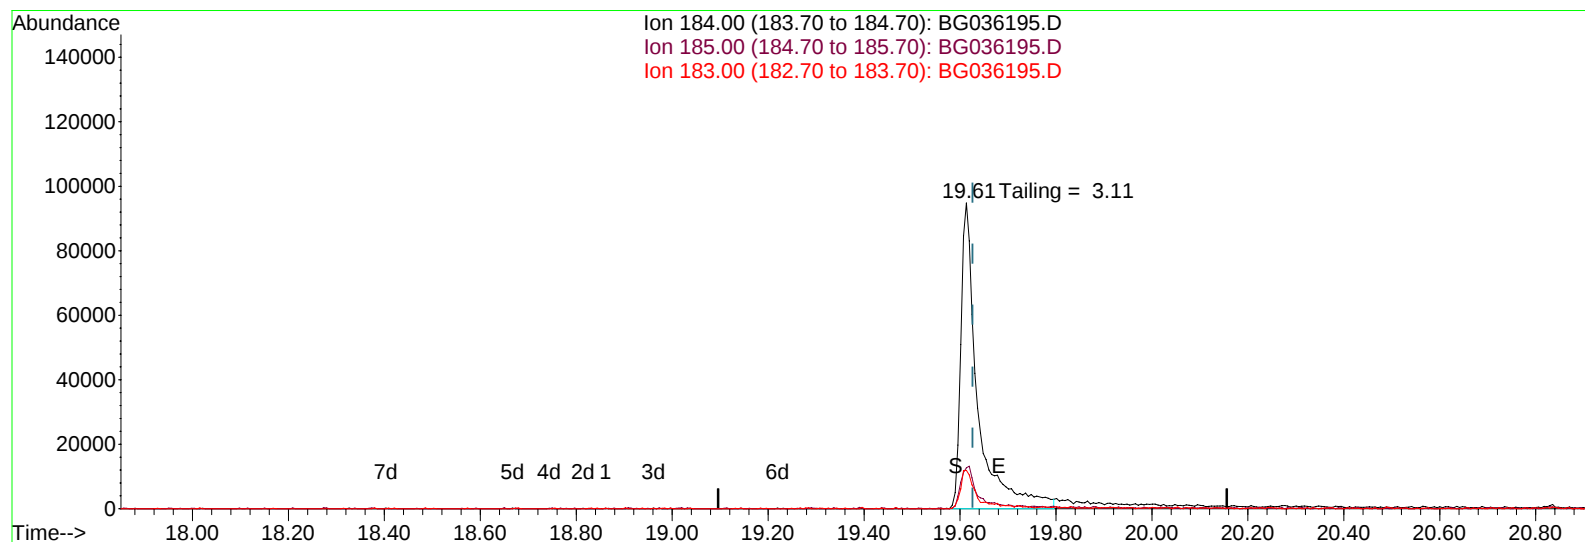

(76) Benzidine




18.861min (-0.765) 0.76ng

response 60

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	117.65#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080818\
Data File : BG036195.D
Acq On : 8 Aug 2018 13:19
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 18:32:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

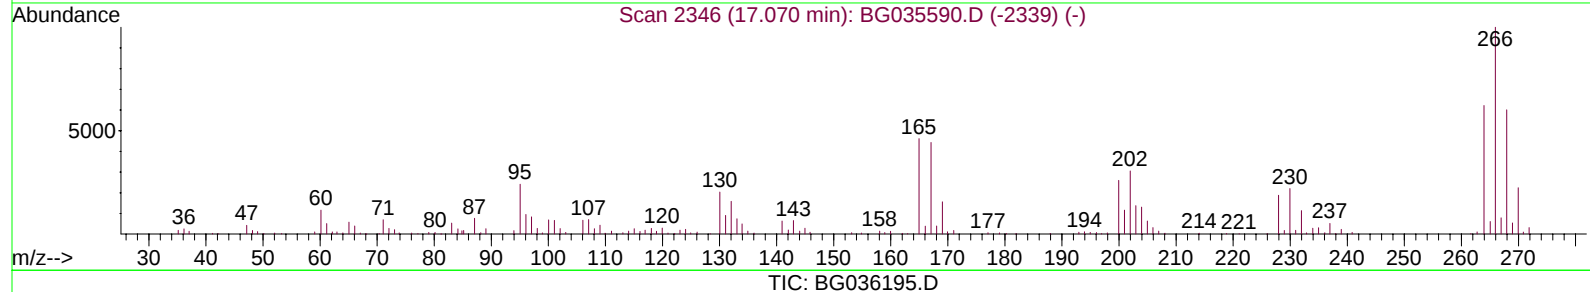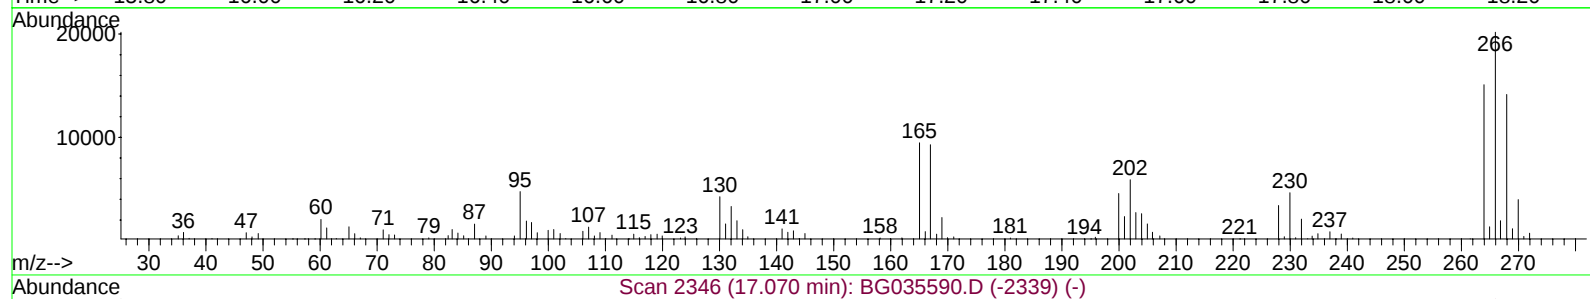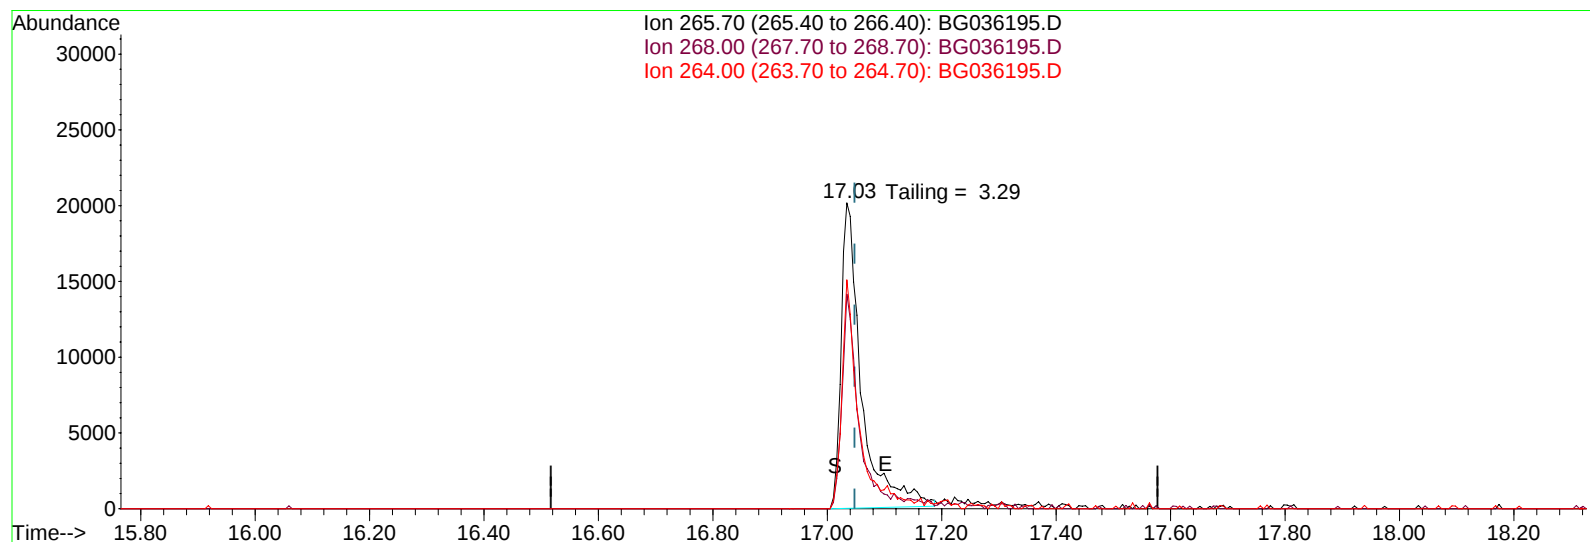

(69) Pentachlorophenol (C)

17.034min (-0.013) 107900.20ng

response 48683

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.18
264.00	62.00	74.81#
0.00	0.00	0.00